
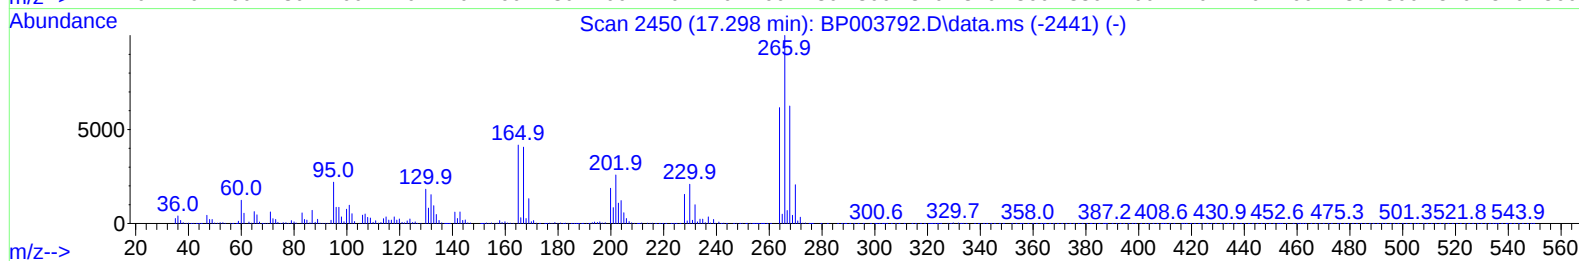
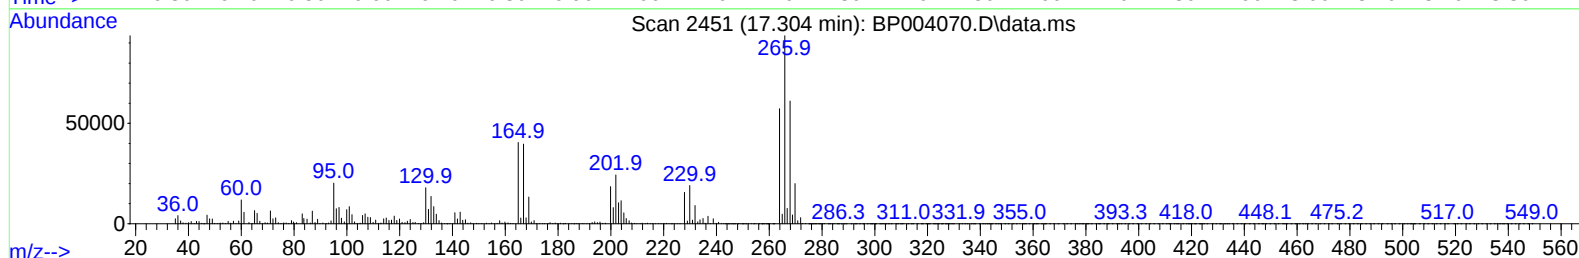


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112420\
 Data File : BP004070.D
 Acq On : 24 Nov 2020 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 05:33:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 16:42:41 2020
 Response via : Initial Calibration

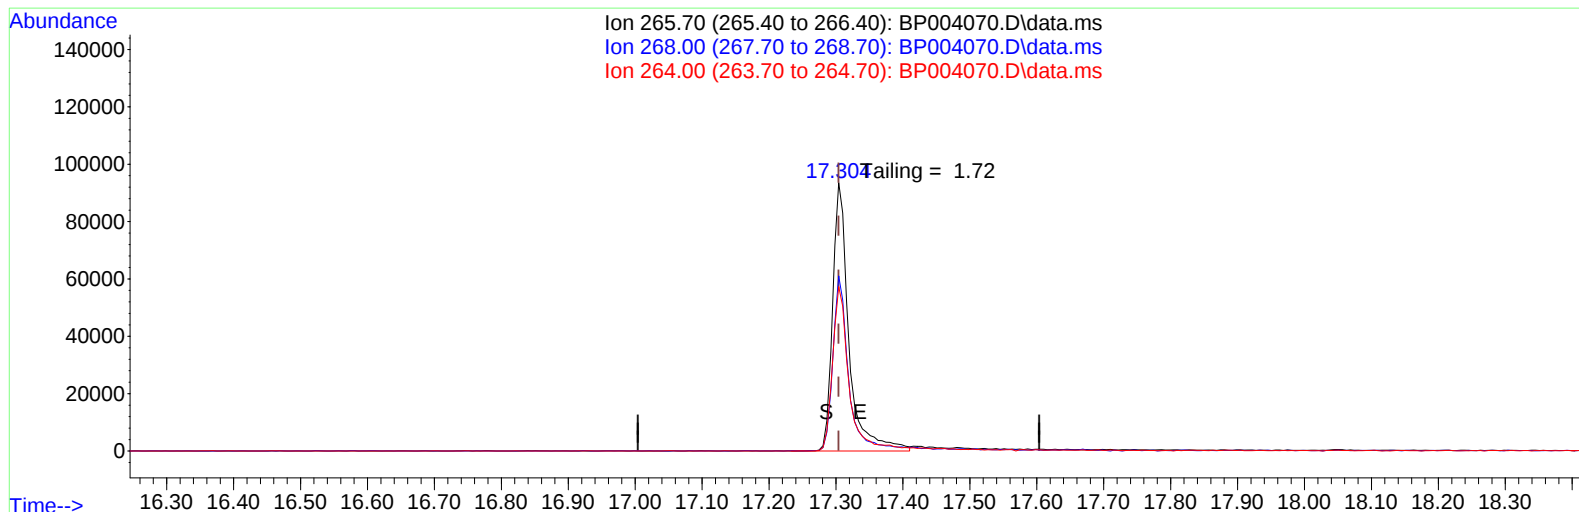

TIC: BP004070.D\data.ms

(70) Pentachlorophenol (C)




17.304min (+ 0.000) 53746.22 ng

response 158923

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.24
264.00	63.30	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112420\
Data File : BP004070.D
Acq On : 24 Nov 2020 11:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 05:33:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 16:42:41 2020
Response via : Initial Calibration

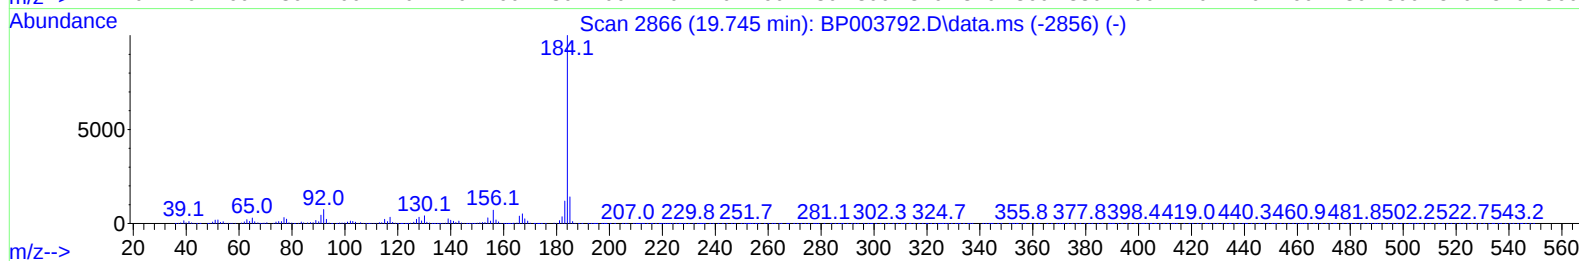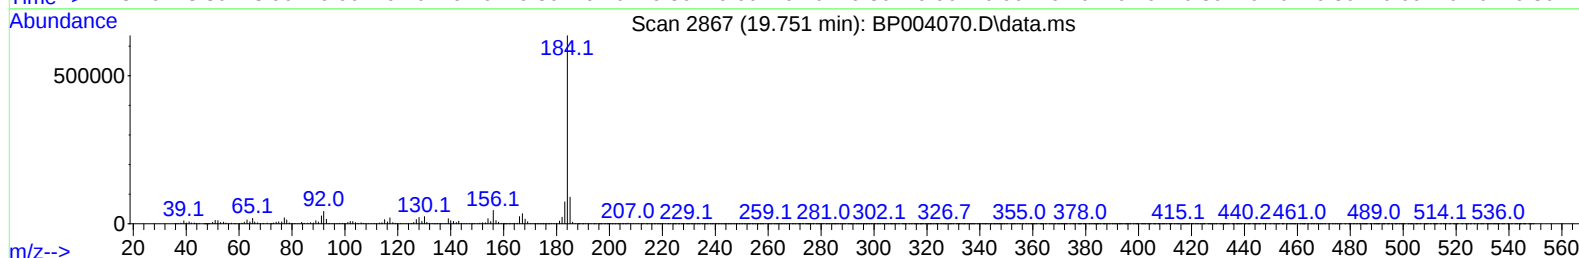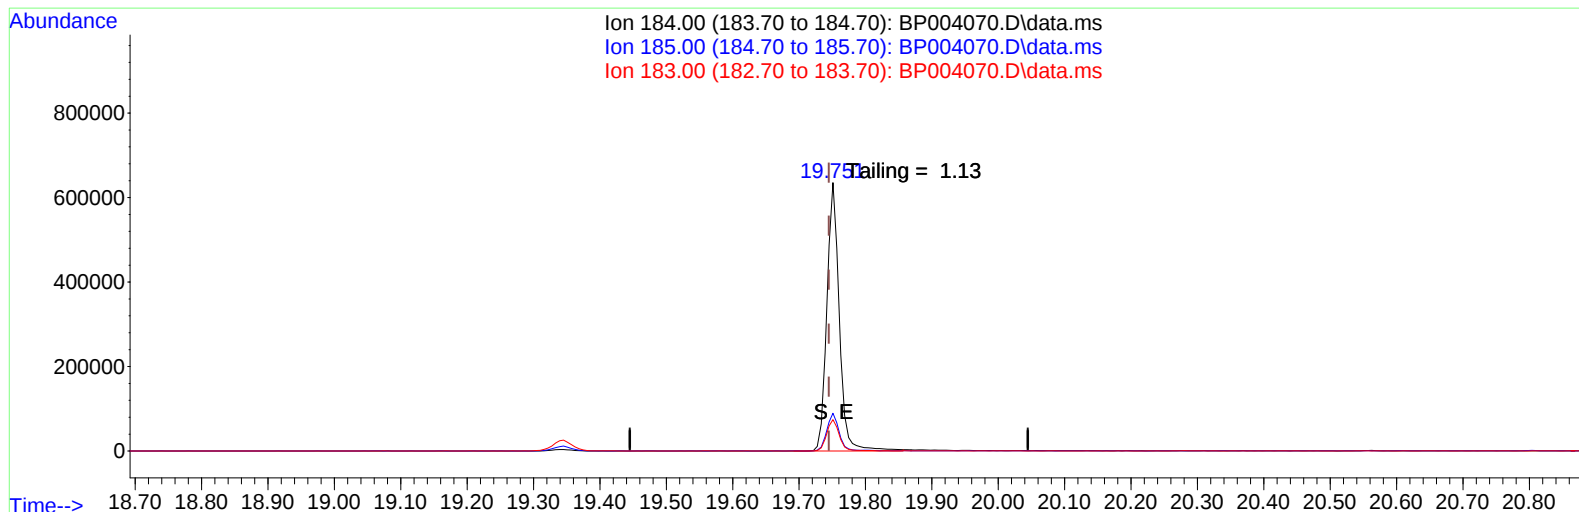

TIC: BP004070.D\data.ms

(77) Benzidine

19.751min (+ 0.006) 42806.65 ng

response 833007

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.11
183.00	12.00	11.69
0.00	0.00	0.00