
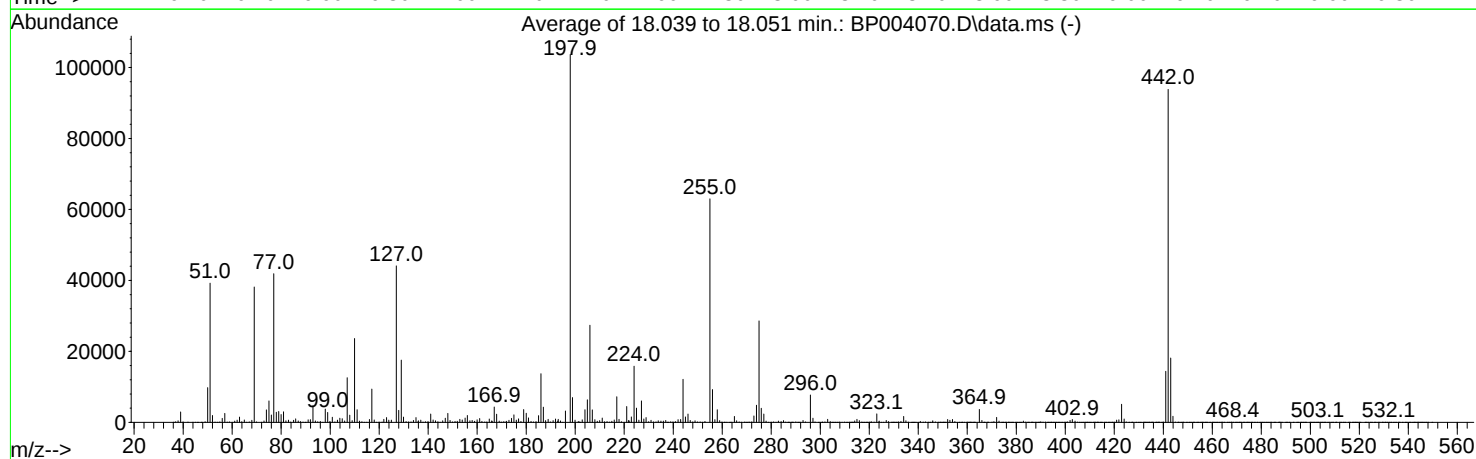


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112420\
 Data File : BP004070.D
 Acq On : 24 Nov 2020 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 23 16:42:41 2020

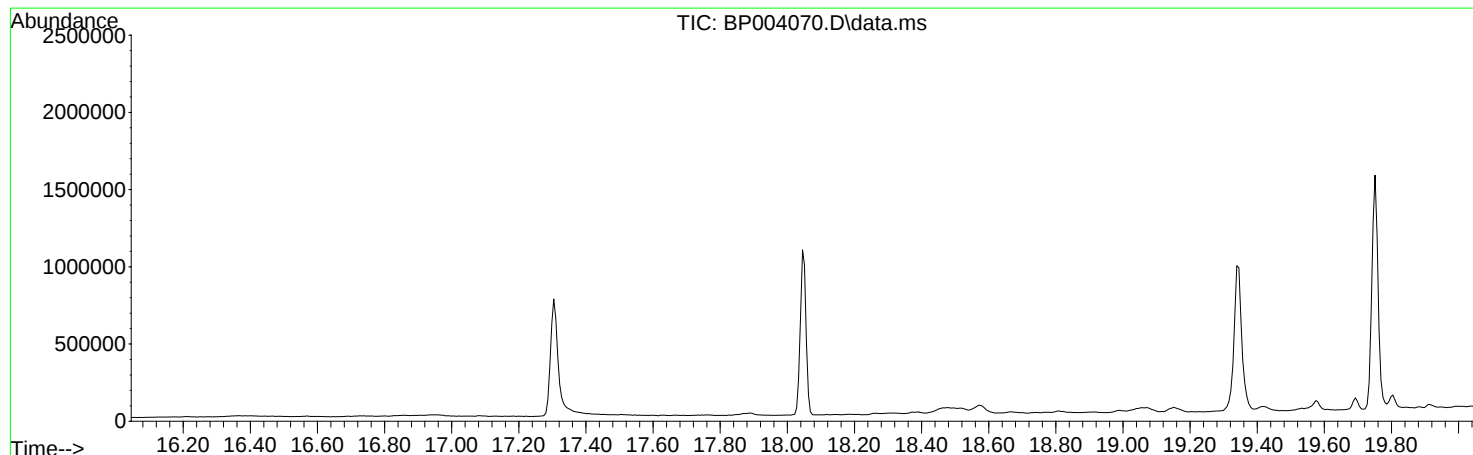

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	39234	PASS
68	69	0.00	2	1.5	583	PASS
69	198	0.00	100	36.8	38168	PASS
70	69	0.00	2	0.3	116	PASS
127	198	10	80	42.5	44084	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103668	PASS
199	198	5	9	6.7	6997	PASS
275	198	10	60	27.6	28597	PASS
365	198	1	100	3.5	3661	PASS
441	198	0.01	100	13.9	14378	PASS
442	442	100	100	100.0	93843	PASS
443	442	15	24	19.3	18113	PASS