

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018356.D
 Acq On : 25 Nov 2023 08:01
 Operator : MA/JU
 Sample : 05264-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKS2

Quant Time: Nov 26 23:58:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	303047	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	1090231	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	600911	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	1255772	20.000	ng/ul	0.00
79) Chrysene-d12	21.351	240	1233546	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	1494699	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	27021	3.340	ng/uL	0.00
4) Pyridine-d5	3.693	84	57519	2.587	ng/ul	0.00
7) Phenol-d5	7.028	99	167752	6.057	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	427288	25.800	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	497201	21.382	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	284204	12.716	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	284631	32.143	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	274324	33.544	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	512432	25.972	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	498930	18.749	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	1606313	30.042	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1821380	29.895	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	44248	5.994	ng/ul	0.00
60) Fluorene-d10	15.492	176	1376268	30.773	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	140589	26.299	ng/ul	0.00
73) Anthracene-d10	17.351	188	1955530	29.135	ng/ul	0.00
81) Pyrene-d10	19.586	212	2527199	25.742	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.627	264	2712608	31.303	ng/ul	0.00
Target Compounds						
84) 3,3'-Dichlorobenzidine	21.274	252	34094	1.143	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018356.D
Acq On : 25 Nov 2023 08:01
Operator : MA/JU
Sample : 05264-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKS2

Quant Time: Nov 26 23:58:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 24 22:02:00 2023
Response via : Initial Calibration

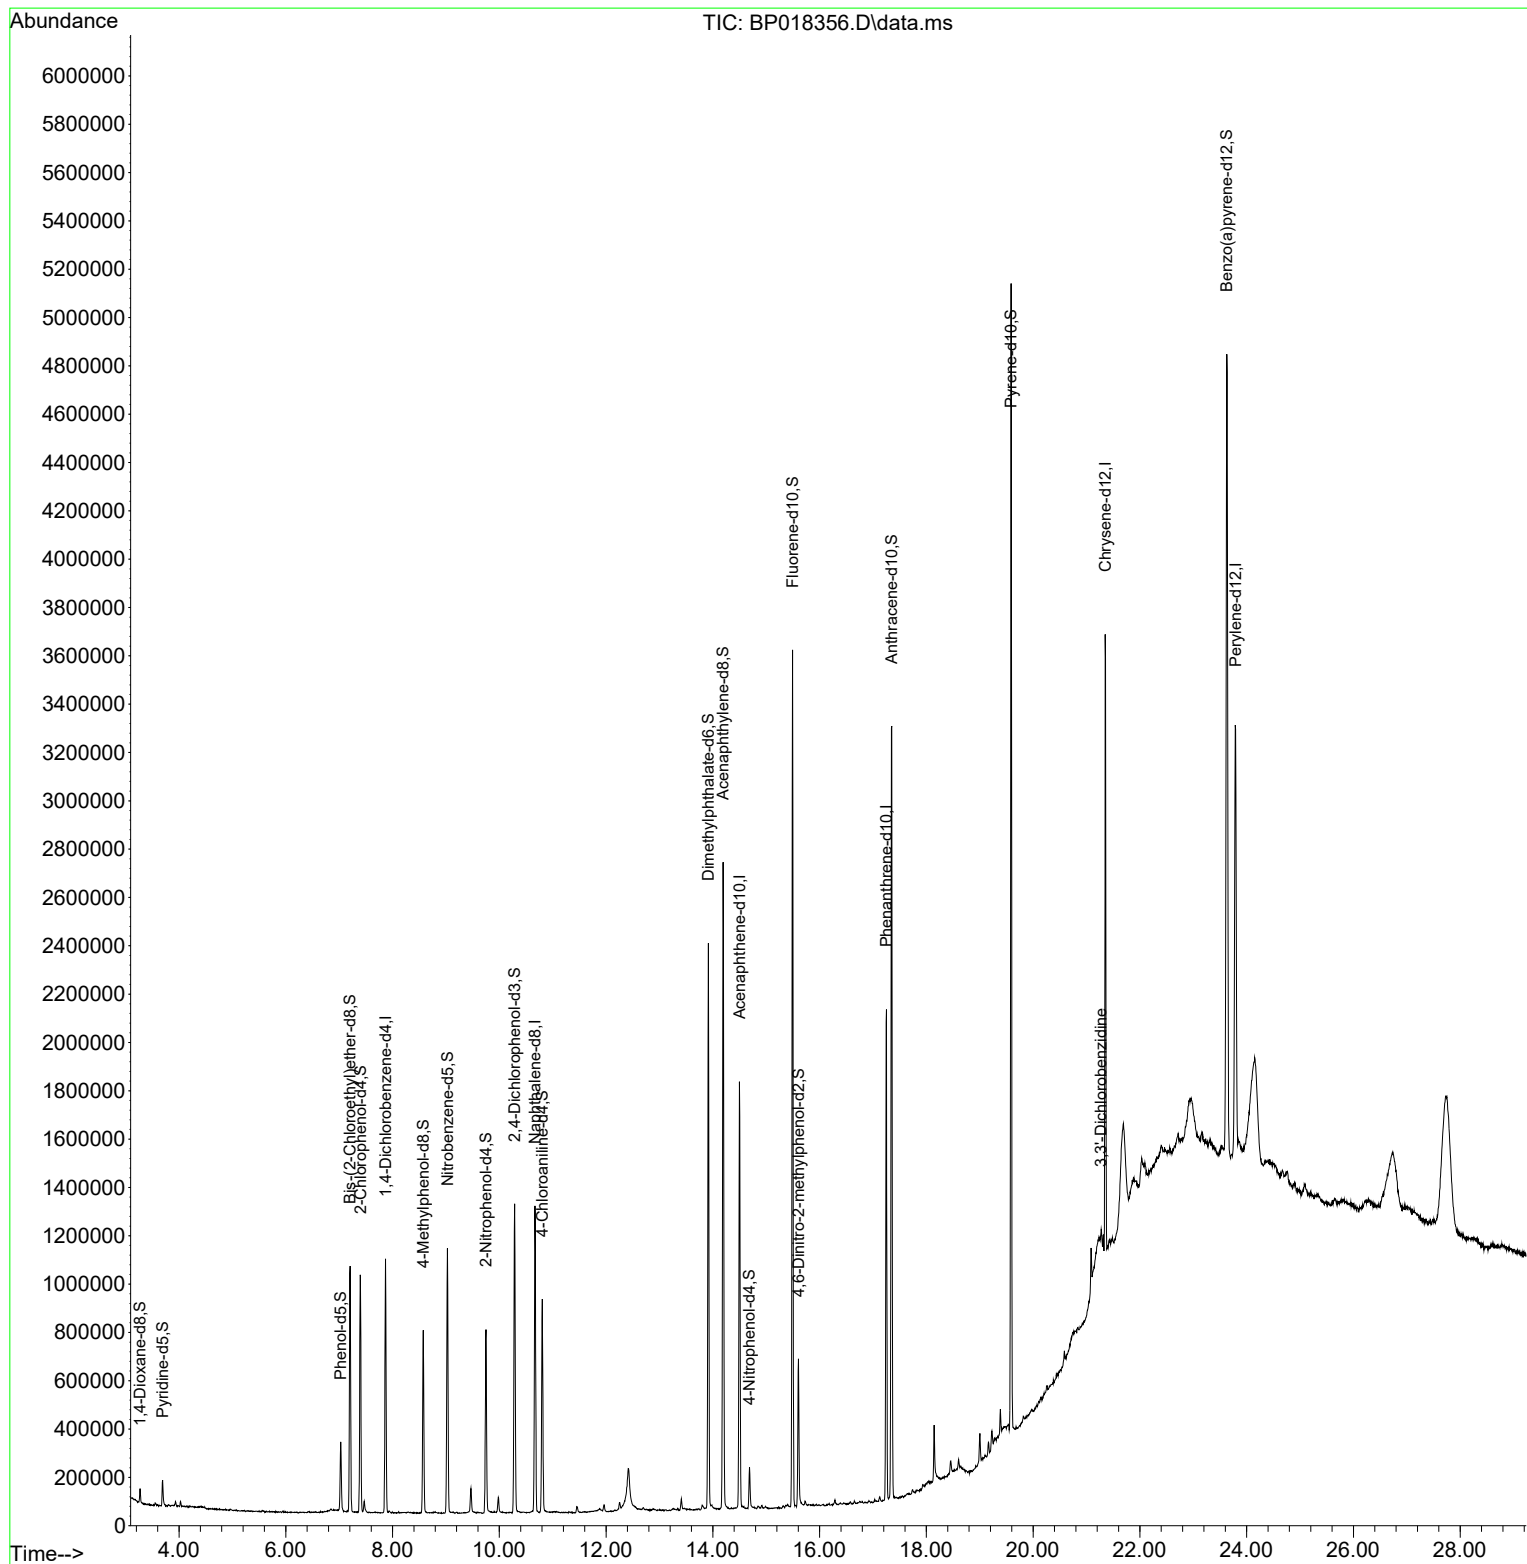

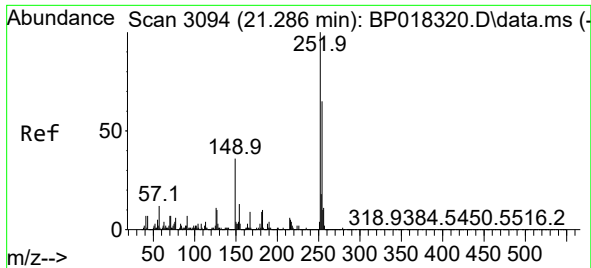

#84

3,3'-Dichlorobenzidine

Concen: 1.143 ng/ul

RT: 21.274 min Scan# 3092

Delta R.T. 0.000 min

Lab File: BP018356.D


Acq: 25 Nov 2023 08:01

Instrument :

BNA_P

ClientSampleId :

DCKS2

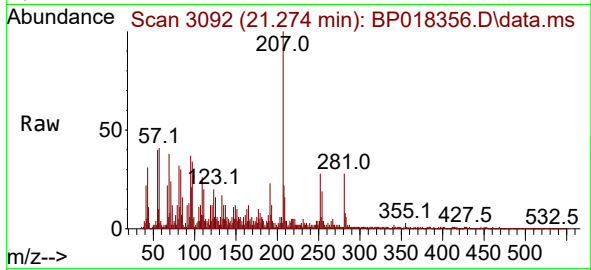

Tgt Ion:252 Resp: 34094

Ion Ratio Lower Upper

252 100

254 66.5 51.1 76.7

126 19.5 8.6 12.8#

