

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018366.D
 Acq On : 25 Nov 2023 13:39
 Operator : MA/JU
 Sample : 05261-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKQ5

Quant Time: Nov 27 00:00:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	370552	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	1355386	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	736711	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	1509607	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	1637344	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	1938048	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	22375	2.262	ng/uL	0.00
4) Pyridine-d5	3.693	84	55335	2.035	ng/ul	0.00
7) Phenol-d5	7.028	99	385507	11.384	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	229402	11.328	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	347556	12.224	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	236211	8.643	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	153763	13.967	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	157130	15.455	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	296742	12.098	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	252432	7.630	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	899203	13.717	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1021595	13.677	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	31318	3.461	ng/ul	0.00
60) Fluorene-d10	15.492	176	765213	13.956	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	20982	3.265	ng/ul	0.00
73) Anthracene-d10	17.345	188	1191726	14.770	ng/ul	0.00
81) Pyrene-d10	19.586	212	1644918	12.623	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	1804408	16.059	ng/ul	0.01
Target Compounds						
					Qvalue	
8) Phenol	7.058	94	51404	1.547	ng/ul	97
16) Acetophenone	8.693	105	152930	3.657	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018366.D
Acq On : 25 Nov 2023 13:39
Operator : MA/JU
Sample : 05261-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKQ5

Quant Time: Nov 27 00:00:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 24 22:02:00 2023
Response via : Initial Calibration




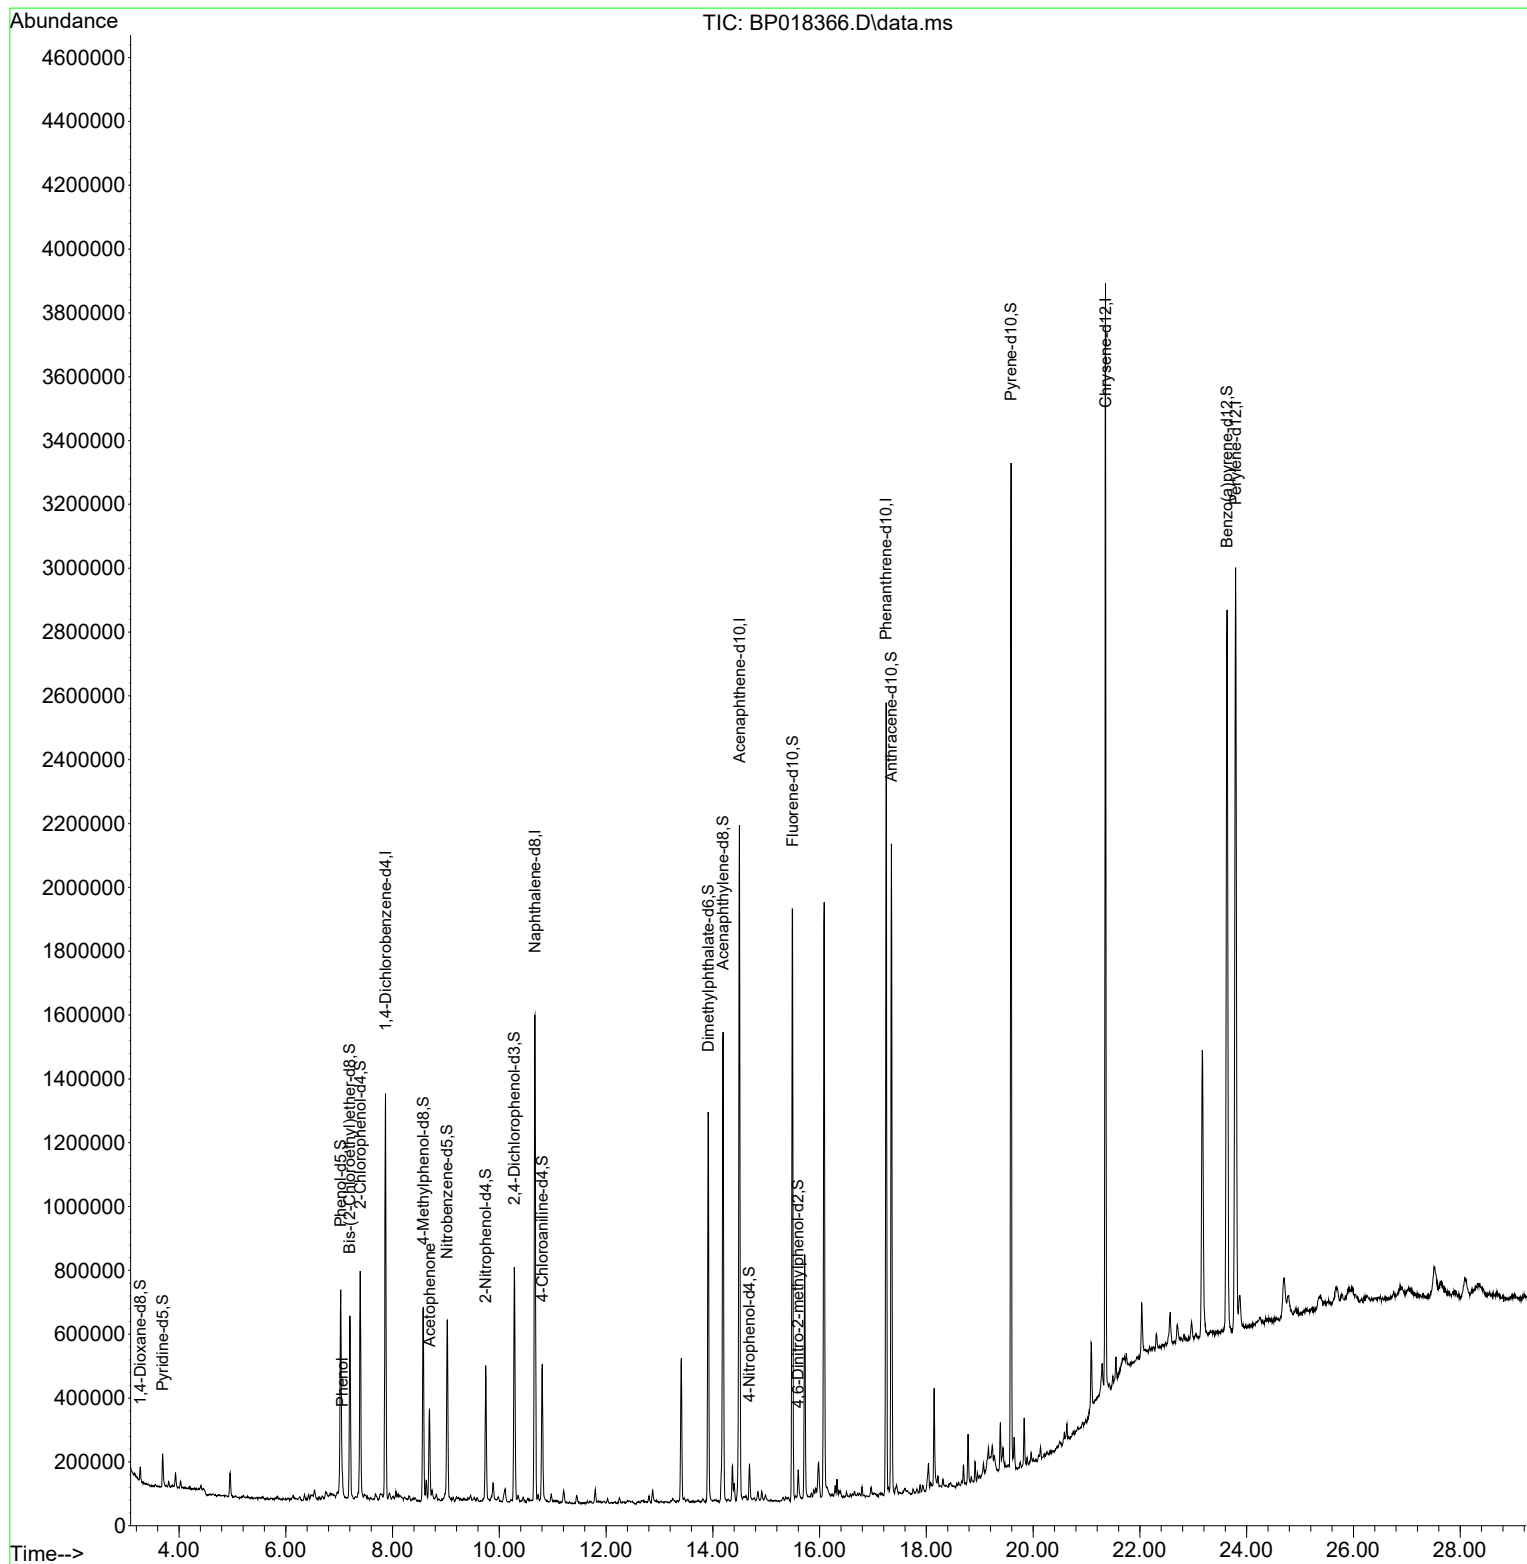


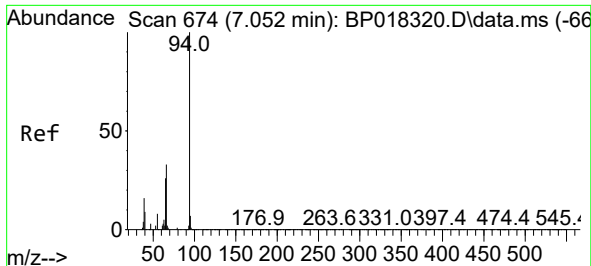

#8
Phenol
Concen: 1.547 ng/ul
RT: 7.058 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP018366.D
Acq: 25 Nov 2023 13:39

Instrument :
BNA_P
ClientSampleId :
DCKQ5

Tgt Ion: 94 Resp: 51404
Ion Ratio Lower Upper
94 100
65 25.8 21.2 31.8
66 33.0 28.0 42.0

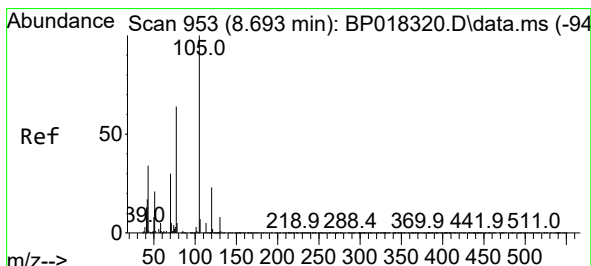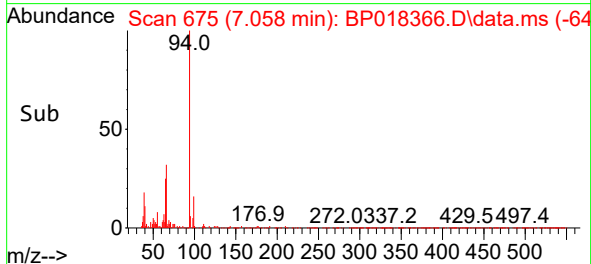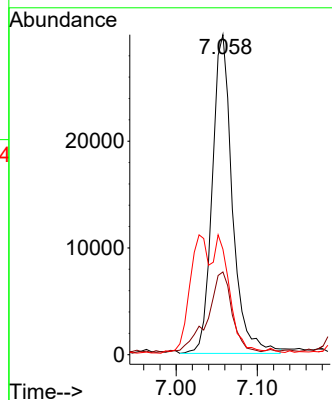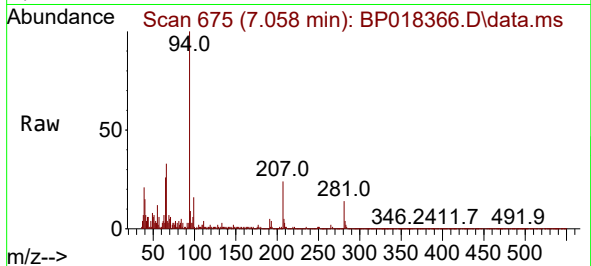

#16
Acetophenone
Concen: 3.657 ng/ul
RT: 8.693 min Scan# 953
Delta R.T. 0.000 min
Lab File: BP018366.D
Acq: 25 Nov 2023 13:39

Tgt Ion: 105 Resp: 152930
Ion Ratio Lower Upper
105 100
77 73.1 59.5 89.3
51 21.9 20.5 30.7

