

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018394.D
 Acq On : 26 Nov 2023 07:09
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Nov 27 00:10:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	490140	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	2015822	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	1214691	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	2330974	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	1607942	20.000	ng/ul	0.00
88) Perylene-d12	23.810	264	1849058	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	99123	7.575	ng/uL	0.00
4) Pyridine-d5	3.687	84	673368	18.724	ng/ul	0.00
7) Phenol-d5	7.028	99	880606	19.659	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	496413	18.533	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	745754	19.829	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	729485	20.180	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	355878	21.735	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	360790	23.860	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	775830	21.266	ng/ul	0.00
31) 4-Chloroaniline-d4	10.799	131	1014488	20.618	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	2120561	19.620	ng/ul	-0.01
49) Acenaphthylene-d8	14.187	160	2442720	19.835	ng/ul	0.00
54) 4-Nitrophenol-d4	14.693	143	277384	18.590	ng/ul	0.00
60) Fluorene-d10	15.487	176	1763936	19.512	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	216997	21.868	ng/ul	0.00
73) Anthracene-d10	17.345	188	2467174	19.802	ng/ul	0.00
81) Pyrene-d10	19.586	212	2410690	18.838	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.645	264	2118848	19.765	ng/ul	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.305	88	99710	7.106	ng/uL#	90
5) Pyridine	3.705	79	670601	18.507	ng/ul	97
6) Benzaldehyde	7.005	77	497154	20.973	ng/ul	95
8) Phenol	7.058	94	869028	19.778	ng/ul	96
10) Bis(2-Chloroethyl)ether	7.293	93	712213	19.459	ng/ul	95
12) 2-Chlorophenol	7.422	128	739069	19.588	ng/ul	96
13) 2-Methylphenol	8.311	108	682411	19.939	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.393	45	857191	16.476	ng/ul	96
16) Acetophenone	8.687	105	1076695	19.465	ng/ul	95
17) N-Nitroso-di-n-propyla...	8.681	70	494013	15.987	ng/ul	92
18) 4-Methylphenol	8.640	108	731688	20.020	ng/ul	99
19) Hexachloroethane	8.946	117	293223	18.609	ng/ul	91
22) Nitrobenzene	9.069	77	750190	19.557	ng/ul	94
23) Isophorone	9.599	82	1462801	17.110	ng/ul	97
25) 2-Nitrophenol	9.775	139	396270	23.292	ng/ul	94
26) 2,4-Dimethylphenol	9.840	107	736938	19.293	ng/ul	98
27) Bis(2-Chloroethoxy)met...	10.081	93	968886	18.765	ng/ul	100
29) 2,4-Dichlorophenol	10.310	162	736193	21.067	ng/ul	98
30) Naphthalene	10.710	128	2384713	19.560	ng/ul	100
32) 4-Chloroaniline	10.828	127	956347	20.597	ng/ul	99
33) Hexachlorobutadiene	10.999	225	524798	22.019	ng/ul	100
34) Caprolactam	11.593	113	187611	18.630	ng/ul	87
35) 4-Chloro-3-methylphenol	11.946	107	690890	18.491	ng/ul	95
36) 2-Methylnaphthalene	12.322	142	1657692	19.212	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018394.D
 Acq On : 26 Nov 2023 07:09
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Nov 27 00:10:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.540	142	1651859	19.019	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.687	216	965711	22.511	ng/ul	99
40) Hexachlorocyclopentadiene	12.669	237	467600	19.245	ng/ul	99
41) 2,4,6-Trichlorophenol	12.928	196	585902	22.741	ng/ul	99
42) 2,4,5-Trichlorophenol	12.999	196	619163	22.225	ng/ul	99
43) 1,1'-Biphenyl	13.334	154	2159890	20.408	ng/ul	99
44) 2-Chloronaphthalene	13.375	162	1723409	20.574	ng/ul	98
45) 2-Nitroaniline	13.575	65	355467	19.722	ng/ul	88
47) Dimethylphthalate	13.957	163	2076694	19.637	ng/ul	99
48) 2,6-Dinitrotoluene	14.075	165	397622	22.301	ng/ul	90
50) Acenaphthylene	14.216	152	2703587	19.694	ng/ul	99
51) 3-Nitroaniline	14.399	138	378593	21.371	ng/ul#	96
52) Acenaphthene	14.557	153	1758656	19.611	ng/ul	100
53) 2,4-Dinitrophenol	14.604	184	121953	19.605	ng/ul	96
55) 4-Nitrophenol	14.704	109	194821	17.624	ng/ul	94
56) Dibenzofuran	14.893	168	2431088	19.829	ng/ul	98
57) 2,4-Dinitrotoluene	14.857	165	533288	22.133	ng/ul	90
58) 2,3,4,6-Tetrachlorophenol	15.116	232	488747	22.338	ng/ul	96
59) Diethylphthalate	15.328	149	1989521	18.728	ng/ul	99
61) Fluorene	15.546	166	1902877	19.033	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.546	204	1021604	20.122	ng/ul	96
63) 4-Nitroaniline	15.563	138	336294	20.115	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.616	198	240605	21.863	ng/ul	98
67) N-Nitrosodiphenylamine	15.757	169	1601096	20.255	ng/ul	100
68) 4-Bromophenyl-phenylether	16.440	248	606263	20.600	ng/ul	95
69) Hexachlorobenzene	16.545	284	735931	22.368	ng/ul	93
70) Atrazine	16.716	200	521094	21.594	ng/ul	98
71) Pentachlorophenol	16.892	266	367462	21.737	ng/ul	98
72) Phenanthrene	17.287	178	2785384	19.645	ng/ul	100
74) Anthracene	17.381	178	2813237	19.657	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.293	216	961514	23.998	ng/ul	100
76) Pentachlorobenzene	14.810	250	911777	23.427	ng/ul	99
77) Carbazole	17.651	167	2274390	19.616	ng/ul	99
78) Di-n-butylphthalate	18.216	149	3062050	18.986	ng/ul	100
80) Fluoranthene	19.263	202	2872924	18.792	ng/ul	96
82) Pyrene	19.616	202	2869915	18.642	ng/ul	96
83) Butylbenzylphthalate	20.510	149	998398	17.525	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.280	252	796029	20.469	ng/ul	100
85) Benzo(a)anthracene	21.345	228	2550698	19.465	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.298	149	1456033	17.035	ng/ul	99
87) Chrysene	21.398	228	2358603	19.779	ng/ul	100
89) Di-n-octyl phthalate	22.269	149	2105393	15.466	ng/ul	100
90) Benzo(b)fluoranthene	23.057	252	2546390	18.960	ng/ul	99
91) Benzo(k)fluoranthene	23.104	252	2536609	18.972	ng/ul	99
93) Benzo(a)pyrene	23.698	252	2438329	19.741	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.416	276	3022065	21.160	ng/ul	97
95) Dibenzo(a,h)anthracene	26.463	278	2502317	21.402	ng/ul	98
96) Benzo(g,h,i)perylene	27.215	276	2483293	21.470	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018394.D
 Acq On : 26 Nov 2023 07:09
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Nov 27 00:10:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration




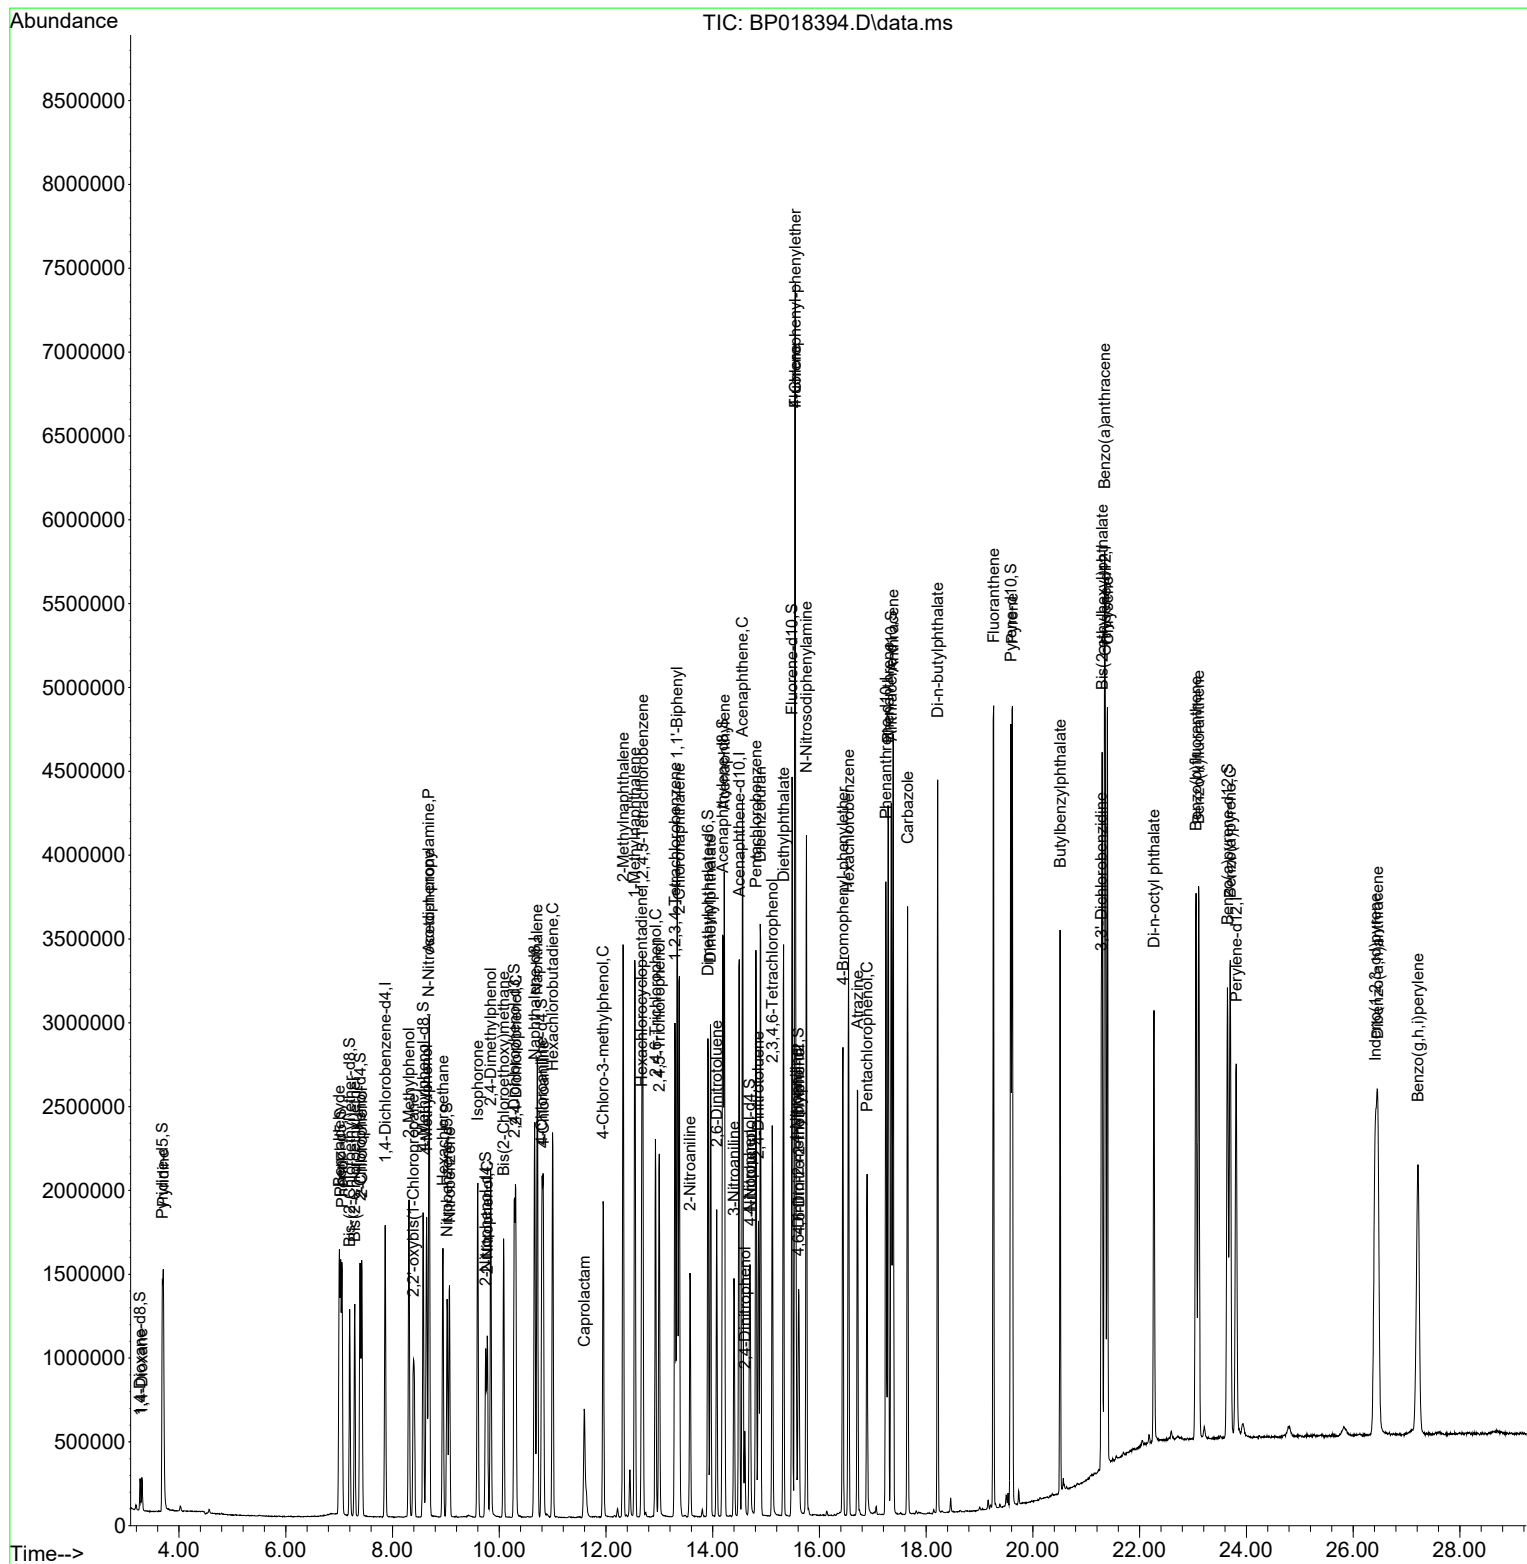


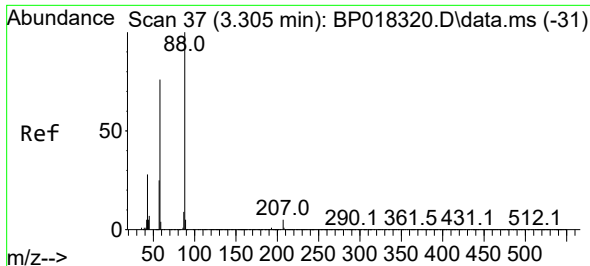

#2
1,4-Dioxane
Concen: 7.106 ng/uL
RT: 3.305 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 88 Resp: 99710
Ion Ratio Lower Upper
88 100
43 24.2 26.9 40.3#
58 68.6 59.6 89.4

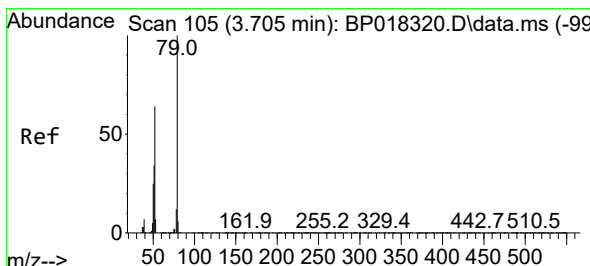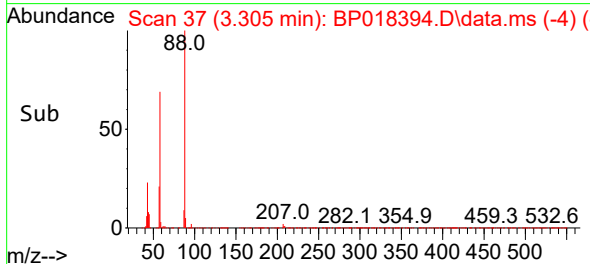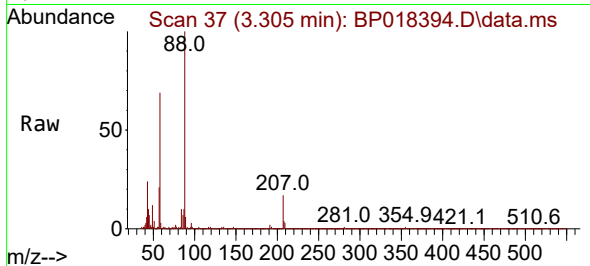

#5
Pyridine
Concen: 18.507 ng/uL
RT: 3.705 min Scan# 105
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion: 79 Resp: 670601
Ion Ratio Lower Upper
79 100
52 69.5 57.7 86.5
51 32.7 27.8 41.8


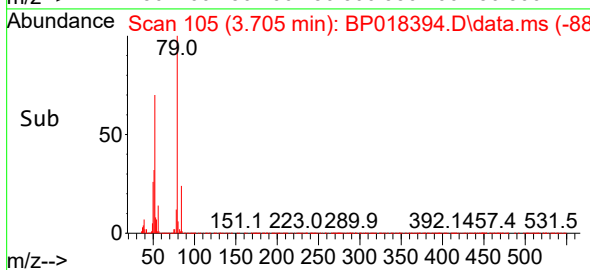

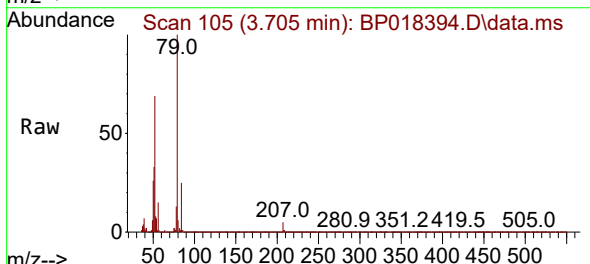




#6
Benzaldehyde
Concen: 20.973 ng/ul
RT: 7.005 min Scan# 666
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 497154
Ion Ratio Lower Upper
77 100
105 106.9 81.5 122.3
106 102.2 77.9 116.9



#8
Phenol
Concen: 19.778 ng/ul
RT: 7.058 min Scan# 675
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion: 94 Resp: 869028
Ion Ratio Lower Upper
94 100
65 24.9 21.2 31.8
66 32.5 28.0 42.0



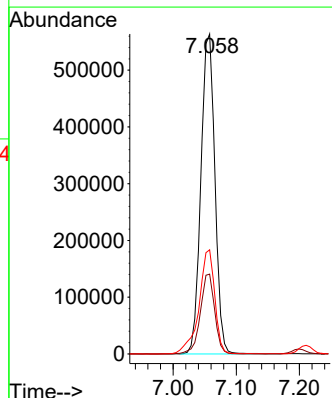



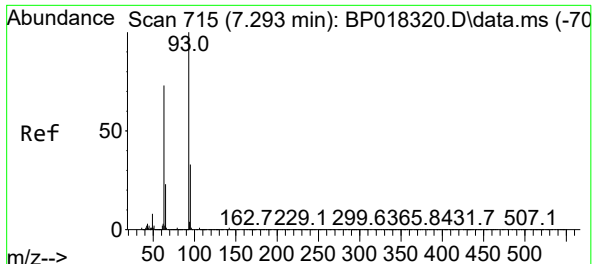

#10
Bis(2-Chloroethyl)ether
Concen: 19.459 ng/ul
RT: 7.293 min Scan# 715
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 93 Resp: 712213
Ion Ratio Lower Upper
93 100
63 67.7 58.2 87.4
95 32.9 25.6 38.4

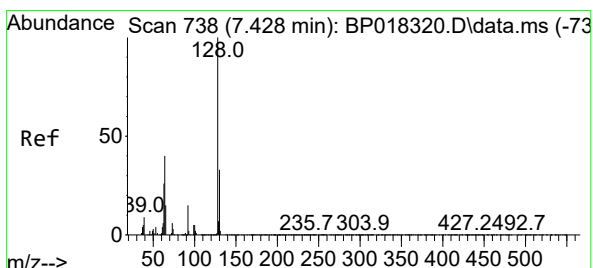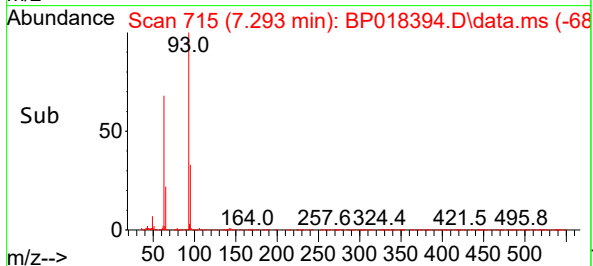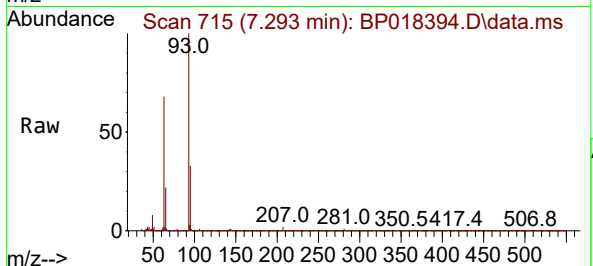

#12
2-Chlorophenol
Concen: 19.588 ng/ul
RT: 7.422 min Scan# 737
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:128 Resp: 739069
Ion Ratio Lower Upper
128 100
64 39.6 34.8 52.2
130 32.1 25.5 38.3


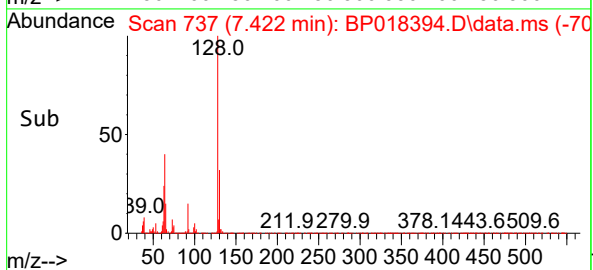

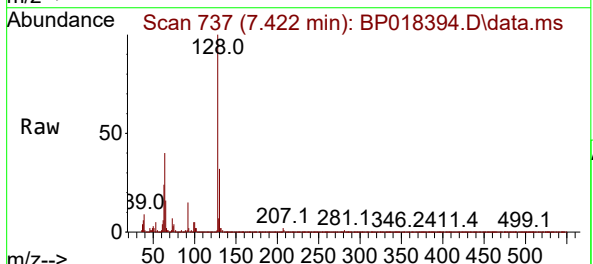




#13
2-Methylphenol
Concen: 19.939 ng/ul
RT: 8.311 min Scan# 888
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:108 Resp: 682411
Ion Ratio Lower Upper
108 100
107 89.3 70.9 106.3



#14
2,2'-oxybis(1-Chloropropane)
Concen: 16.476 ng/ul
RT: 8.393 min Scan# 902
Delta R.T. -0.012 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion: 45 Resp: 857191
Ion Ratio Lower Upper
45 100
77 16.0 11.4 17.2
79 12.1 8.4 12.6









#16
Acetophenone
Concen: 19.465 ng/ul
RT: 8.687 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:105 Resp: 1076695
Ion Ratio Lower Upper
105 100
77 70.5 59.5 89.3
51 22.0 20.5 30.7



#17
N-Nitroso-di-n-propylamine
Concen: 15.987 ng/ul
RT: 8.681 min Scan# 951
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion: 70 Resp: 494013
Ion Ratio Lower Upper
70 100
42 51.0 46.8 70.2
101 10.4 8.4 12.6
130 25.3 18.5 27.7









#18
4-Methylphenol
Concen: 20.020 ng/ul
RT: 8.640 min Scan# 944
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:108 Resp: 731688
Ion Ratio Lower Upper
108 100
107 111.2 89.5 134.3



#19
Hexachloroethane
Concen: 18.609 ng/ul
RT: 8.946 min Scan# 996
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:117 Resp: 293223
Ion Ratio Lower Upper
117 100
201 117.5 85.6 128.4
199 73.7 54.2 81.4



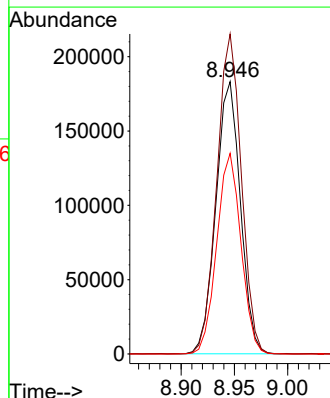





#22
Nitrobenzene
Concen: 19.557 ng/ul
RT: 9.069 min Scan# 1017
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 750190
Ion Ratio Lower Upper
77 100
123 51.8 37.7 56.5
65 13.2 10.5 15.7



#23
Isophorone
Concen: 17.110 ng/ul
RT: 9.599 min Scan# 1107
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion: 82 Resp: 1462801
Ion Ratio Lower Upper
82 100
95 7.3 5.8 8.6
138 20.5 14.9 22.3









#25
2-Nitrophenol
Concen: 23.292 ng/ul
RT: 9.775 min Scan# 1137
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:139 Resp: 396270
Ion Ratio Lower Upper
139 100
65 42.2 38.3 57.5
109 28.5 23.4 35.0



#26
2,4-Dimethylphenol
Concen: 19.293 ng/ul
RT: 9.840 min Scan# 1148
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:107 Resp: 736938
Ion Ratio Lower Upper
107 100
121 53.0 40.0 60.0
122 88.9 70.4 105.6

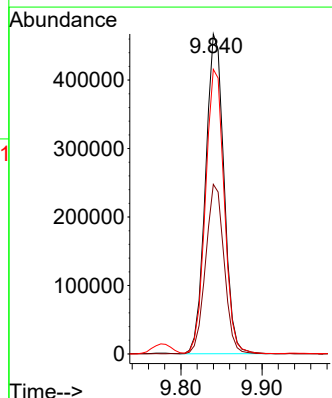



#27

Bis(2-Chloroethoxy)methane

Concen: 18.765 ng/ul

RT: 10.081 min Scan# 1189

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion: 93 Resp: 968886

Ion Ratio Lower Upper

93 100

95 32.3 26.0 39.0

123 11.7 9.1 13.7

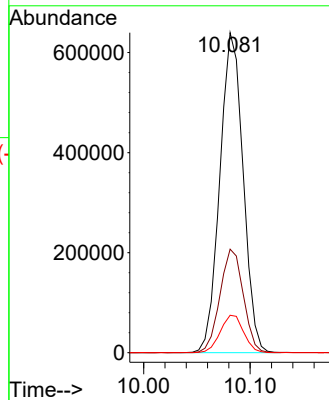

#29

2,4-Dichlorophenol

Concen: 21.067 ng/ul

RT: 10.310 min Scan# 1228

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:162 Resp: 736193


Ion Ratio Lower Upper

162 100

164 65.8 53.0 79.6

98 31.5 27.7 41.5


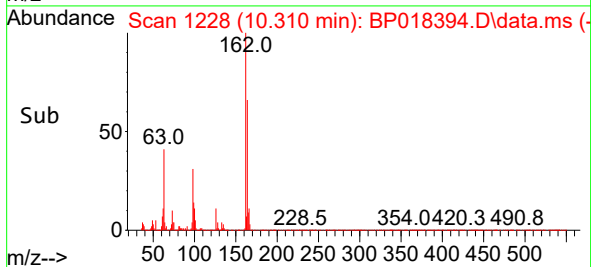
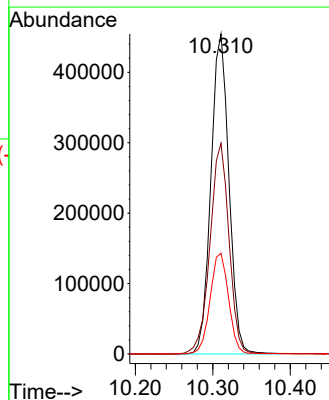
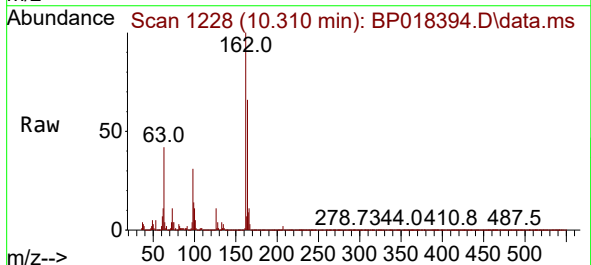




#30
Naphthalene
Concen: 19.560 ng/ul
RT: 10.710 min Scan# 1298
Delta R.T. -0.012 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:128 Resp: 2384713
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 12.9 10.4 15.6

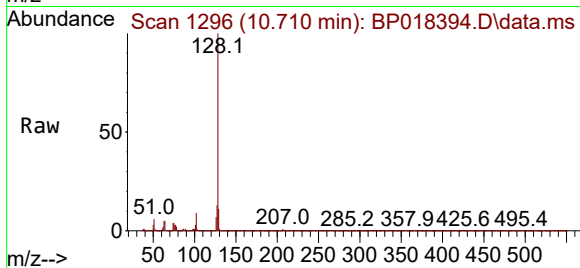

#32
4-Chloroaniline
Concen: 20.597 ng/ul
RT: 10.828 min Scan# 1316
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09


Tgt Ion:127 Resp: 956347
Ion Ratio Lower Upper
127 100
129 31.7 25.8 38.8








#33
Hexachlorobutadiene
Concen: 22.019 ng/ul
RT: 10.999 min Scan# 11
Delta R.T. -0.012 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09


Instrument :
BNA_P
ClientSampleId :





Tgt Ion:225 Resp: 524798
Ion Ratio Lower Upper
225 100
223 62.7 50.2 75.4
227 63.3 50.4 75.6




#34
Caprolactam
Concen: 18.630 ng/ul
RT: 11.593 min Scan# 1446
Delta R.T. 0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09



Tgt Ion:113 Resp: 187611
Ion Ratio Lower Upper
113 100
55 141.5 129.0 193.4
56 108.2 94.8 142.2



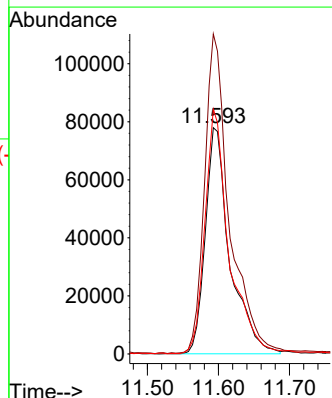





#35
4-Chloro-3-methylphenol
Concen: 18.491 ng/ul
RT: 11.946 min Scan# 1507
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:107 Resp: 690890
Ion Ratio Lower Upper
107 100
144 28.7 21.6 32.4
142 86.9 65.4 98.0



#36
2-Methylnaphthalene
Concen: 19.212 ng/ul
RT: 12.322 min Scan# 1570
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:142 Resp: 1657692
Ion Ratio Lower Upper
142 100
141 88.6 71.0 106.4





#37

1-Methylnaphthalene

Concen: 19.019 ng/ul

RT: 12.540 min Scan# 1

Delta R.T. -0.012 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:142 Resp: 1651859

Ion Ratio Lower Upper

142 100

141 91.7 73.9 110.9

116 3.6 3.0 4.4



#39

1,2,4,5-Tetrachlorobenzene

Concen: 22.511 ng/ul

RT: 12.687 min Scan# 1632

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Tgt Ion:216 Resp: 965711




Ion Ratio Lower Upper


216 100

214 79.4 63.3 94.9

179 20.3 17.3 25.9

108 14.6 13.4 20.0

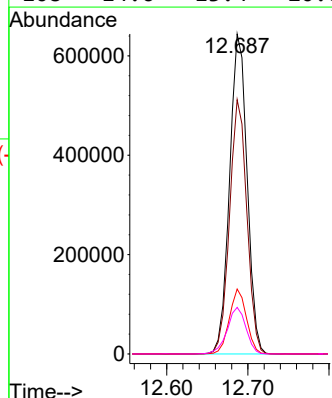



#40

Hexachlorocyclopentadiene

Concen: 19.245 ng/ul

RT: 12.669 min Scan# 1629

Delta R.T. -0.012 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:237 Resp: 467600

Ion Ratio Lower Upper

237 100

235 63.2 50.7 76.1

272 13.7 10.3 15.5

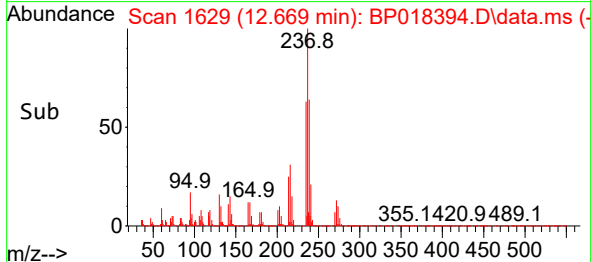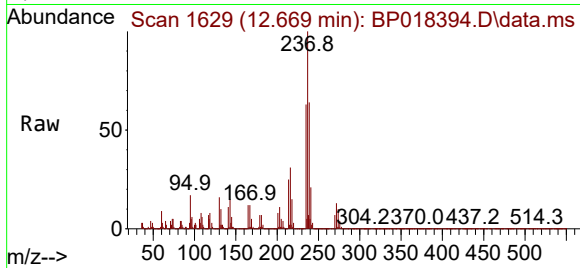

#41

2,4,6-Trichlorophenol

Concen: 22.741 ng/ul

RT: 12.928 min Scan# 1673

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:196 Resp: 585902


Ion Ratio Lower Upper

196 100

198 96.4 78.0 117.0

200 30.9 24.6 37.0


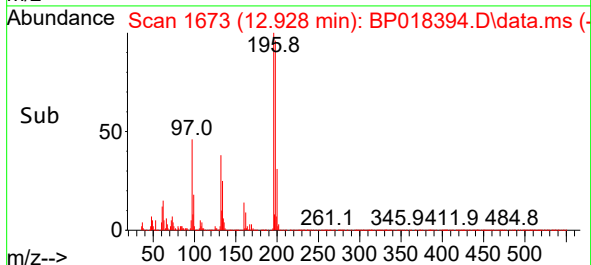
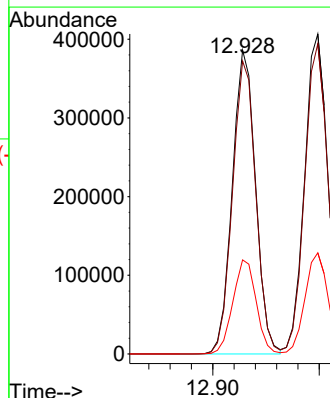
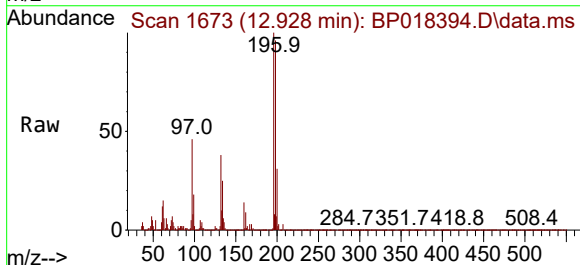


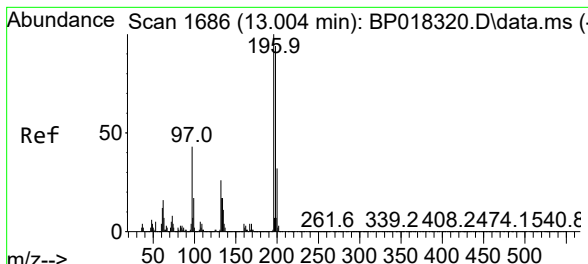

#42
 2,4,5-Trichlorophenol
 Concen: 22.225 ng/ul
 RT: 12.999 min Scan# 1685
 Delta R.T. 0.000 min
 Lab File: BP018394.D
 Acq: 26 Nov 2023 07:09




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion:	196	Resp:	619163
Ion Ratio	Lower	Upper	
196	100		
198	96.9	76.7	115.1
200	31.6	24.6	36.8

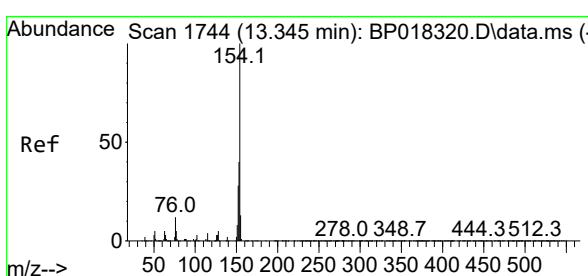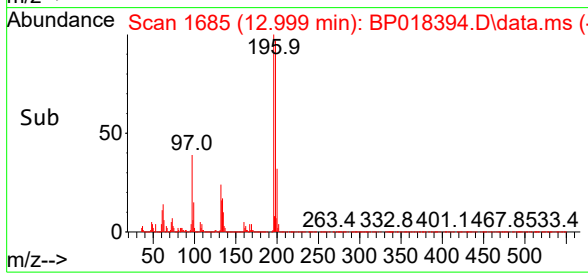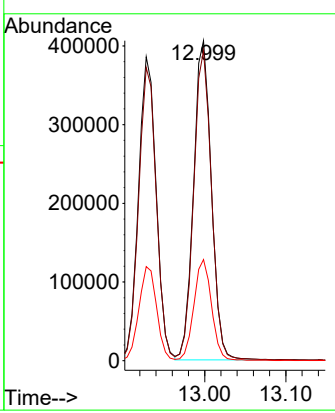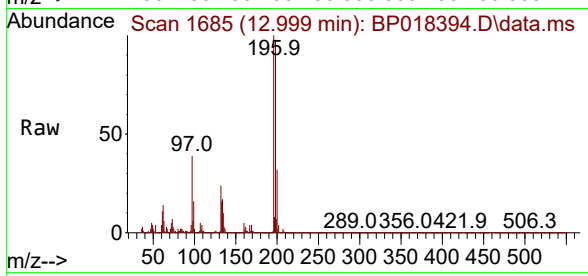

#43
 1,1'-Biphenyl
 Concen: 20.408 ng/ul
 RT: 13.334 min Scan# 1742
 Delta R.T. -0.006 min
 Lab File: BP018394.D
 Acq: 26 Nov 2023 07:09

Tgt Ion:	154	Resp:	2159890
Ion Ratio	Lower	Upper	
154	100		
153	39.7	32.2	48.2
76	11.3	9.9	14.9


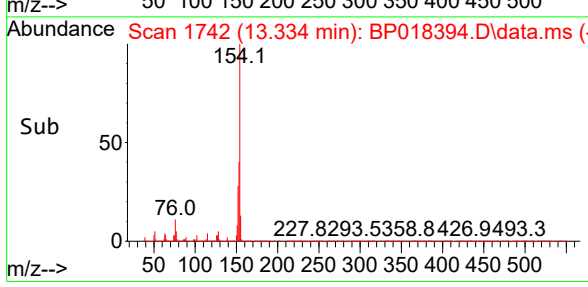
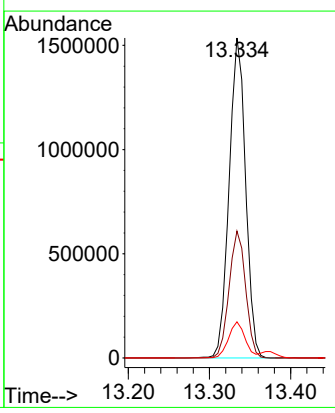
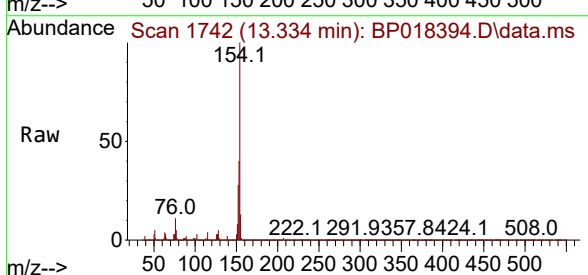




#44
2-Chloronaphthalene
Concen: 20.574 ng/ul
RT: 13.375 min Scan# 1749
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:162 Resp: 1723409
Ion Ratio Lower Upper
162 100
164 33.2 26.2 39.4
127 36.4 30.6 45.8



#45
2-Nitroaniline
Concen: 19.722 ng/ul
RT: 13.575 min Scan# 1783
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion: 65 Resp: 355467
Ion Ratio Lower Upper
65 100
92 77.3 57.4 86.2
138 130.4 90.6 136.0









#47
Dimethylphthalate
Concen: 19.637 ng/ul
RT: 13.957 min Scan# 1848
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:163 Resp: 2076694
Ion Ratio Lower Upper
163 100
194 4.2 3.1 4.7
164 10.4 7.9 11.9



#48
2,6-Dinitrotoluene
Concen: 22.301 ng/ul
RT: 14.075 min Scan# 1868
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:165 Resp: 397622
Ion Ratio Lower Upper
165 100
89 48.6 45.8 68.6
121 19.7 17.8 26.8


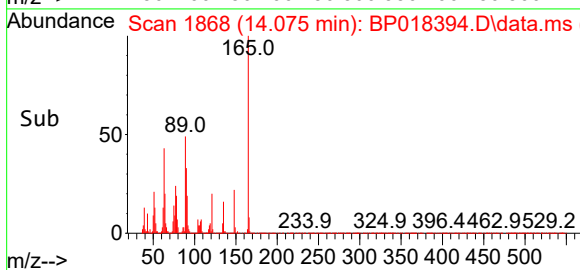






#50
Acenaphthylene
Concen: 19.694 ng/ul
RT: 14.216 min Scan# 1892
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:152 Resp: 2703587
Ion Ratio Lower Upper
152 100
151 20.3 15.7 23.5
153 13.2 10.8 16.2



#51
3-Nitroaniline
Concen: 21.371 ng/ul
RT: 14.399 min Scan# 1923
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:138 Resp: 378593
Ion Ratio Lower Upper
138 100
108 12.5 13.2 19.8#
92 109.4 90.2 135.4



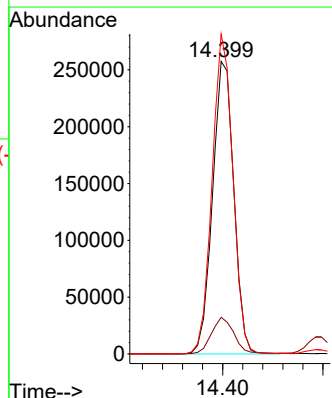





#52
Acenaphthene
Concen: 19.611 ng/ul
RT: 14.557 min Scan# 1950
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:153 Resp: 1758656
Ion Ratio Lower Upper
153 100
152 47.1 37.8 56.8
154 89.4 71.2 106.8



#53
2,4-Dinitrophenol
Concen: 19.605 ng/ul
RT: 14.604 min Scan# 1958
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:184 Resp: 121953
Ion Ratio Lower Upper
184 100
63 46.8 41.8 62.6
154 59.5 47.3 70.9



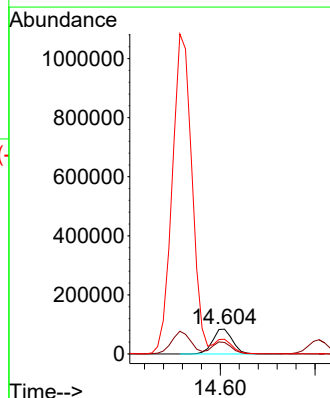





#55
4-Nitrophenol
Concen: 17.624 ng/ul
RT: 14.704 min Scan# 1975
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:109 Resp: 194821
Ion Ratio Lower Upper
109 100
139 149.1 113.0 169.4
65 119.0 99.6 149.4



#56
Dibenzofuran
Concen: 19.829 ng/ul
RT: 14.893 min Scan# 2007
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:168 Resp: 2431088
Ion Ratio Lower Upper
168 100
139 35.0 29.0 43.4





#57

2,4-Dinitrotoluene

Concen: 22.133 ng/ul

RT: 14.857 min Scan# 2002

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:165 Resp: 533288

Ion Ratio Lower Upper

165 100

63 33.3 32.1 48.1

182 3.0 2.0 3.0

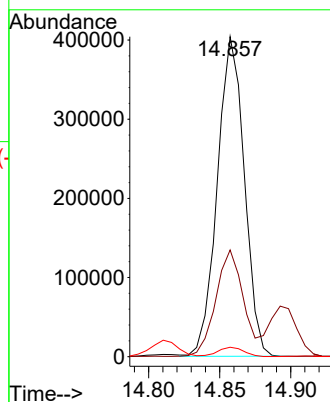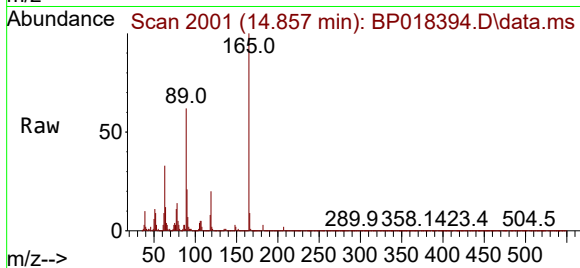

#58

2,3,4,6-Tetrachlorophenol

Concen: 22.338 ng/ul

RT: 15.116 min Scan# 2045

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Tgt Ion:232 Resp: 488747




Ion Ratio Lower Upper


232 100

131 39.9 34.1 51.1

130 2.1 1.8 2.6

166 29.2 24.8 37.2







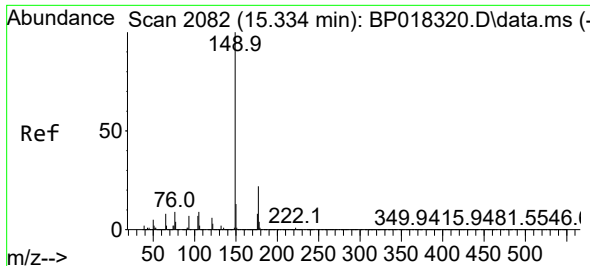

#59
Diethylphthalate
Concen: 18.728 ng/ul
RT: 15.328 min Scan# 2081
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:149 Resp: 1989521
Ion Ratio Lower Upper
149 100
177 23.6 18.2 27.2
150 12.6 10.2 15.2

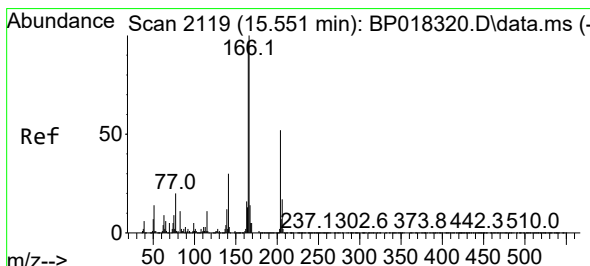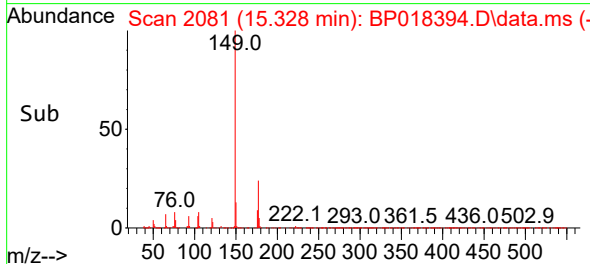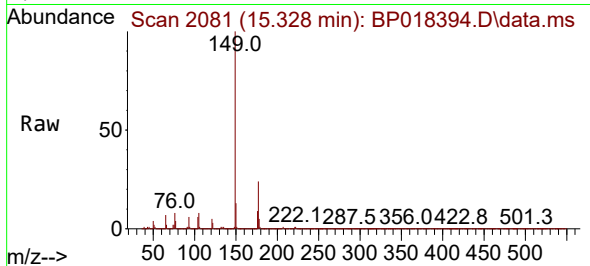

#61
Fluorene
Concen: 19.033 ng/ul
RT: 15.546 min Scan# 2118
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:166 Resp: 1902877
Ion Ratio Lower Upper
166 100
165 97.3 77.5 116.3
167 13.9 10.6 16.0


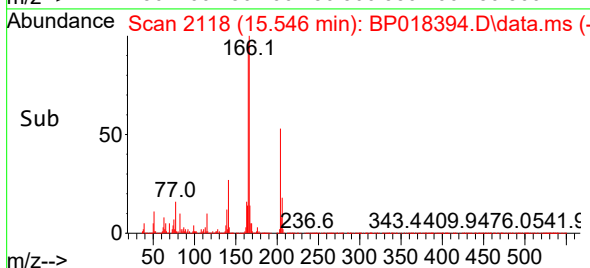
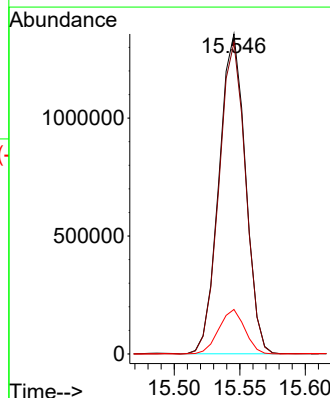
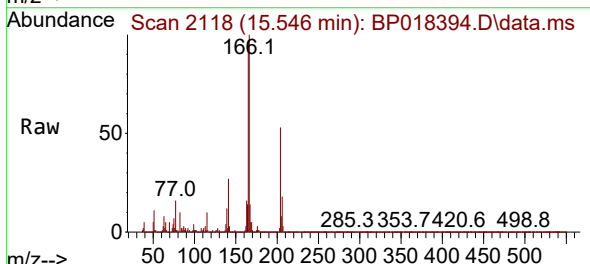




#62
4-Chlorophenyl-phenylether
Concen: 20.122 ng/ul
RT: 15.546 min Scan# 2118
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:204 Resp: 1021604
Ion Ratio Lower Upper
204 100
206 33.2 26.2 39.2
141 51.7 44.8 67.2

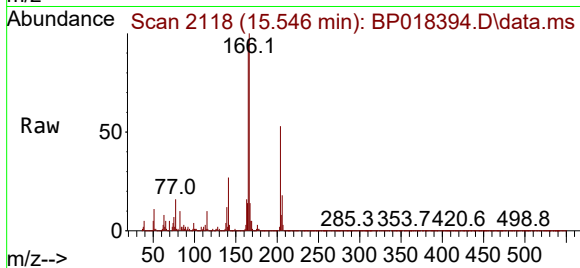

#63
4-Nitroaniline
Concen: 20.115 ng/ul
RT: 15.563 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:138 Resp: 336294
Ion Ratio Lower Upper
138 100
92 46.0 39.3 58.9
108 70.9 61.8 92.6









#66
4,6-Dinitro-2-methylphenol
Concen: 21.863 ng/ul
RT: 15.616 min Scan# 2130
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:198 Resp: 240605
Ion Ratio Lower Upper
198 100
182 4.2 3.0 4.4
77 20.9 17.3 25.9

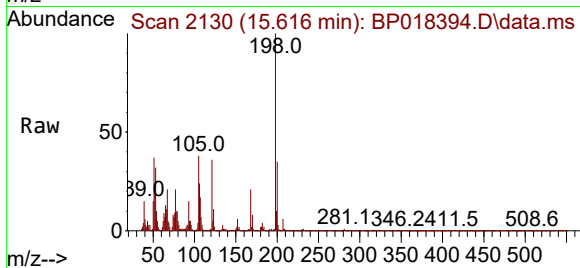

#67
N-Nitrosodiphenylamine
Concen: 20.255 ng/ul
RT: 15.757 min Scan# 2154
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:169 Resp: 1601096
Ion Ratio Lower Upper
169 100
168 66.1 53.1 79.7
167 36.0 28.8 43.2




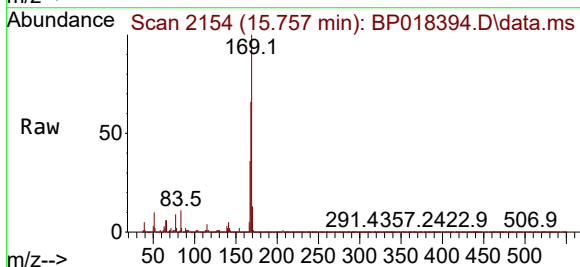




#68
4-Bromophenyl-phenylether
Concen: 20.600 ng/ul
RT: 16.440 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:248 Resp: 606263
Ion Ratio Lower Upper
248 100
250 98.2 77.4 116.2
141 61.6 56.0 84.0



#69
Hexachlorobenzene
Concen: 22.368 ng/ul
RT: 16.545 min Scan# 2288
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:284 Resp: 735931
Ion Ratio Lower Upper
284 100
142 30.5 28.9 43.3
249 30.2 26.0 39.0





#70

Atrazine

Concen: 21.594 ng/ul

RT: 16.716 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:200 Resp: 521094

Ion Ratio Lower Upper

200 100

173 25.5 21.1 31.7

215 48.9 38.3 57.5

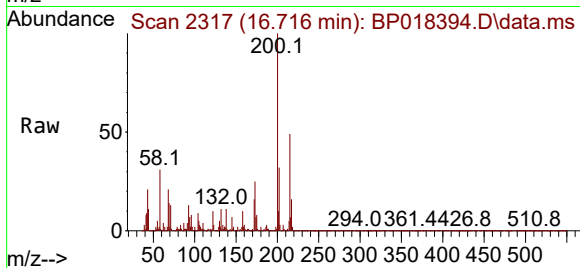

#71

Pentachlorophenol

Concen: 21.737 ng/ul

RT: 16.892 min Scan# 2347

Delta R.T. 0.000 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:266 Resp: 367462


Ion Ratio Lower Upper

266 100

264 64.2 50.1 75.1

268 63.8 50.1 75.1





#72

Phenanthrene

Concen: 19.645 ng/ul

RT: 17.287 min Scan# 2416

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:178 Resp: 2785384

Ion Ratio Lower Upper

178 100

179 15.6 12.4 18.6

176 19.1 15.1 22.7



#74

Anthracene

Concen: 19.657 ng/ul

RT: 17.381 min Scan# 2430

Delta R.T. -0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:178 Resp: 2813237


Ion Ratio Lower Upper

178 100

179 15.7 12.4 18.6

176 18.6 15.2 22.8


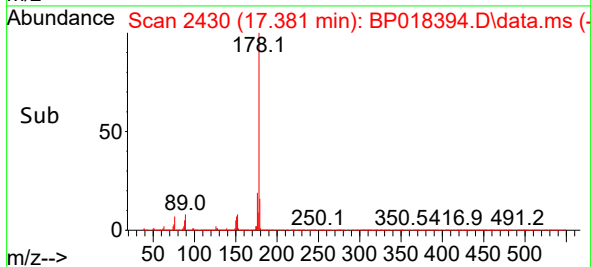

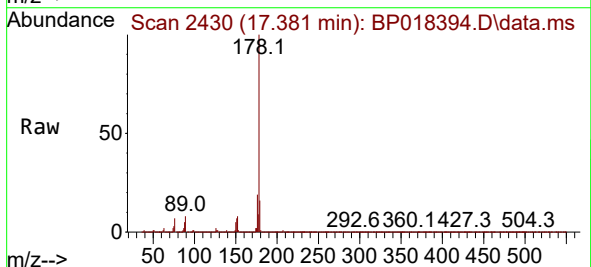




#75
1,2,3,4-Tetrachlorobenzene
Concen: 23.998 ng/uL
RT: 13.293 min Scan# 1735
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:216 Resp: 961514
Ion Ratio Lower Upper
216 100
214 77.2 62.0 93.0
218 48.4 38.6 57.8



#76
Pentachlorobenzene
Concen: 23.427 ng/uL
RT: 14.810 min Scan# 1993
Delta R.T. -0.006 min
Lab File: BP018394.D
Acq: 26 Nov 2023 07:09

Tgt Ion:250 Resp: 911777
Ion Ratio Lower Upper
250 100
248 63.3 51.0 76.6
252 63.6 51.5 77.3









#77
 Carbazole
 Concen: 19.616 ng/ul
 RT: 17.651 min Scan# 2476
 Delta R.T. 0.000 min
 Lab File: BP018394.D
 Acq: 26 Nov 2023 07:09




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion:167 Resp: 2274390
 Ion Ratio Lower Upper
 167 100
 166 21.5 17.5 26.3
 139 12.4 10.0 15.0



#78
 Di-n-butylphthalate
 Concen: 18.986 ng/ul
 RT: 18.216 min Scan# 2572
 Delta R.T. -0.006 min
 Lab File: BP018394.D
 Acq: 26 Nov 2023 07:09

Tgt Ion:149 Resp: 3062050
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.2
 104 4.5 3.8 5.6





#80

Fluoranthene

Concen: 18.792 ng/ul

RT: 19.263 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:202 Resp: 2872924

Ion Ratio Lower Upper

202 100

101 9.3 8.6 13.0

100 7.2 6.7 10.1



#82

Pyrene

Concen: 18.642 ng/ul

RT: 19.616 min Scan# 2810

Delta R.T. 0.000 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:202 Resp: 2869915


Ion Ratio Lower Upper

202 100

101 11.4 10.2 15.4

100 9.2 8.4 12.6

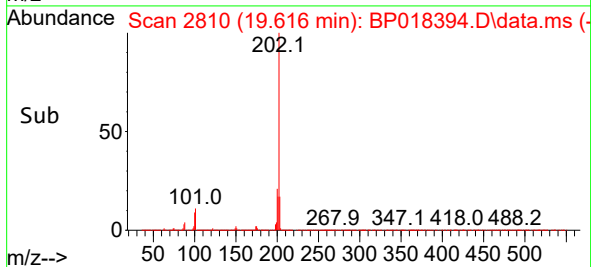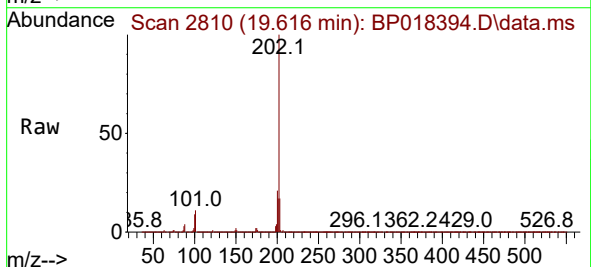



#83

Butylbenzylphthalate

Concen: 17.525 ng/ul

RT: 20.510 min Scan# 2963

Delta R.T. 0.000 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 998398

Ion Ratio Lower Upper

149 100

91 62.8 53.7 80.5

206 22.6 16.4 24.6

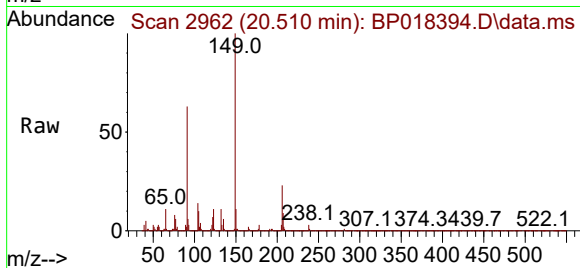

#84

3,3'-Dichlorobenzidine

Concen: 20.469 ng/ul

RT: 21.280 min Scan# 3093

Delta R.T. 0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:252 Resp: 796029


Ion Ratio Lower Upper

252 100

254 64.1 51.1 76.7

126 10.2 8.6 12.8





#85

Benzo(a)anthracene

Concen: 19.465 ng/ul

RT: 21.345 min Scan# 3104

Delta R.T. 0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 2550698

Ion Ratio Lower Upper

228 100

229 19.4 16.2 24.2

226 27.4 22.2 33.2

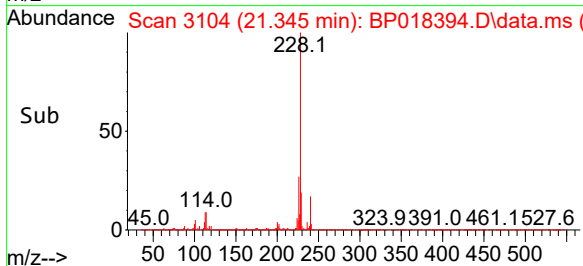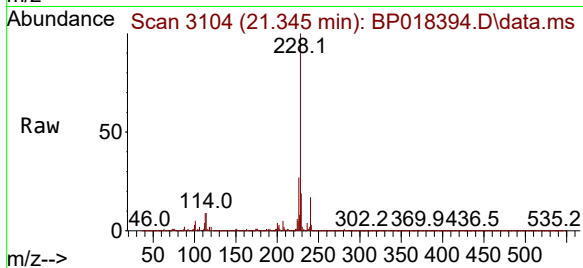

#86

Bis(2-ethylhexyl)phthalate

Concen: 17.035 ng/ul

RT: 21.298 min Scan# 3096

Delta R.T. 0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:149 Resp: 1456033


Ion Ratio Lower Upper

149 100

167 28.2 22.1 33.1

279 4.5 3.4 5.0

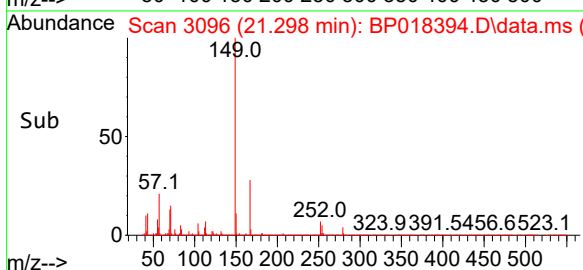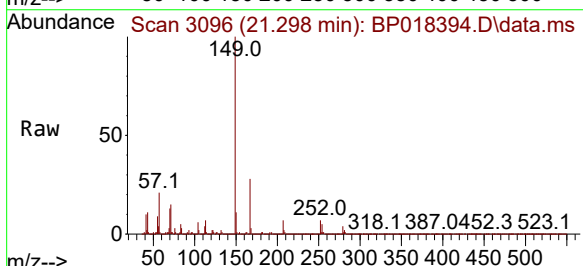



#87

Chrysene

Concen: 19.779 ng/ul

RT: 21.398 min Scan# 3113

Delta R.T. 0.006 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 2358603

Ion Ratio Lower Upper

228 100

226 30.3 24.2 36.4

229 19.7 16.1 24.1

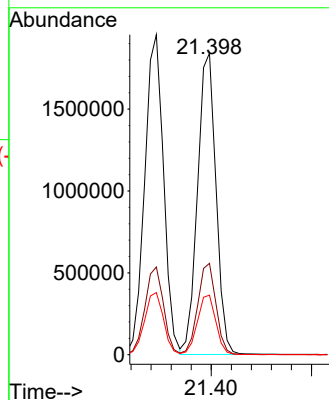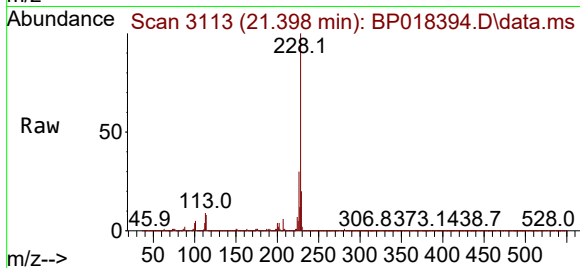

#89

Di-n-octyl phthalate

Concen: 15.466 ng/ul




RT: 22.269 min Scan# 3261


Delta R.T. 0.024 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Tgt Ion:149 Resp: 2105393

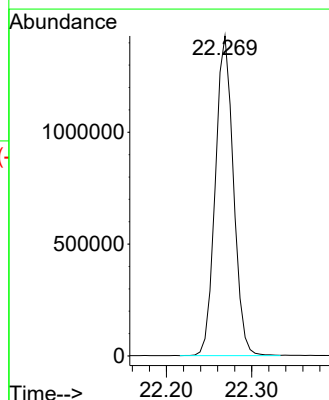



#90

Benzo(b)fluoranthene

Concen: 18.960 ng/ul

RT: 23.057 min Scan# 31

Delta R.T. 0.018 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 2546390

Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 9.1 8.4 12.6

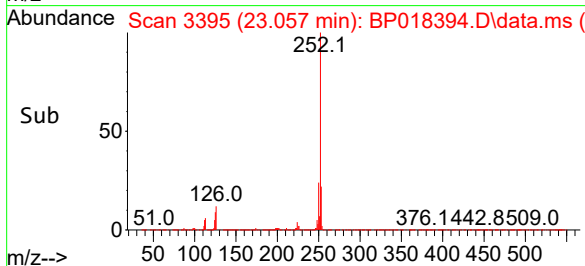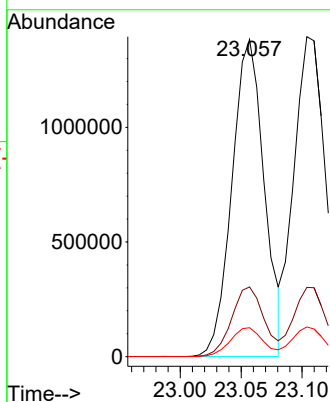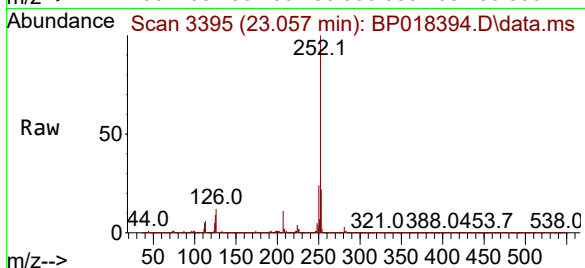

#91

Benzo(k)fluoranthene

Concen: 18.972 ng/ul

RT: 23.104 min Scan# 3403

Delta R.T. 0.018 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:252 Resp: 2536609


Ion Ratio Lower Upper

252 100

253 21.7 17.7 26.5

125 9.3 8.0 12.0

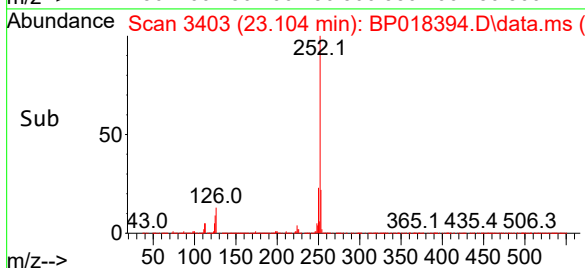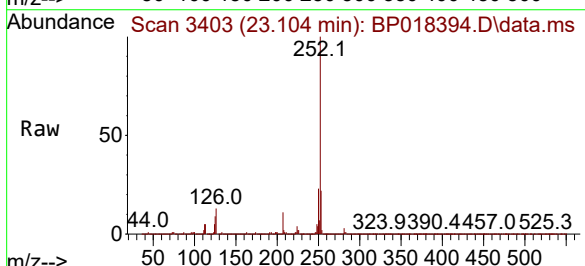



#93

Benzo(a)pyrene

Concen: 19.741 ng/ul

RT: 23.698 min Scan# 31

Delta R.T. 0.024 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 2438329

Ion Ratio Lower Upper

252 100

253 22.3 17.7 26.5

125 9.9 8.8 13.2



#94

Indeno(1,2,3-cd)pyrene

Concen: 21.160 ng/ul

RT: 26.416 min Scan# 3966

Delta R.T. 0.071 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09




Tgt Ion:276 Resp: 3022065


Ion Ratio Lower Upper

276 100

138 18.9 17.5 26.3

277 23.9 19.1 28.7





#95

Dibenzo(a,h)anthracene

Concen: 21.402 ng/ul

RT: 26.463 min Scan# 3962

Delta R.T. 0.083 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:278 Resp: 2502317

Ion Ratio Lower Upper

278 100

139 15.1 13.3 19.9

279 24.3 19.0 28.4

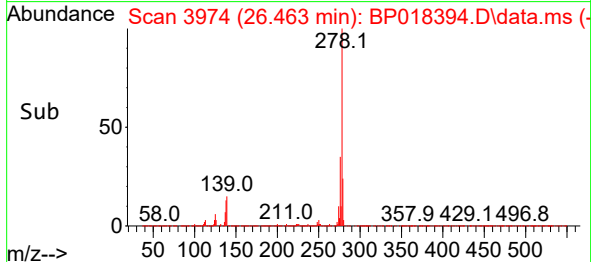

#96

Benzo(g,h,i)perylene

Concen: 21.470 ng/ul

RT: 27.215 min Scan# 4102

Delta R.T. 0.088 min

Lab File: BP018394.D

Acq: 26 Nov 2023 07:09

Tgt Ion:276 Resp: 2483293

Ion Ratio Lower Upper

276 100

138 20.8 17.7 26.5

277 24.2 18.6 28.0

