

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018363.D
 Acq On : 25 Nov 2023 11:57
 Operator : MA/JU
 Sample : 05261-15
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKR8

Quant Time: Nov 27 01:07:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	391609	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	1525311	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	882955	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	1531591	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	1348952	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	1692669	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	21196	2.027	ng/uL	0.00
4) Pyridine-d5	3.693	84	77173	2.686	ng/ul	0.00
7) Phenol-d5	7.028	99	458018	12.798	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	388223	18.140	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	411179	13.684	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	318745	11.036	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	204610	16.515	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143	198368	17.337	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	393806	14.266	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	459800	12.350	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	1212057	15.427	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1381821	15.436	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	101922	9.397	ng/ul	0.00
60) Fluorene-d10	15.492	176	1005499	15.301	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	77791	11.931	ng/ul	0.00
73) Anthracene-d10	17.345	188	1292130	15.784	ng/ul	0.00
81) Pyrene-d10	19.586	212	1441455	13.426	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.627	264	1603859	16.344	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.716	128	93218	1.010	ng/ul#	87
36) 2-Methylnaphthalene	12.328	142	75414	1.155	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.292	149	1079715	15.057	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018363.D
Acq On : 25 Nov 2023 11:57
Operator : MA/JU
Sample : 05261-15
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKR8

Quant Time: Nov 27 01:07:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 24 22:02:00 2023
Response via : Initial Calibration




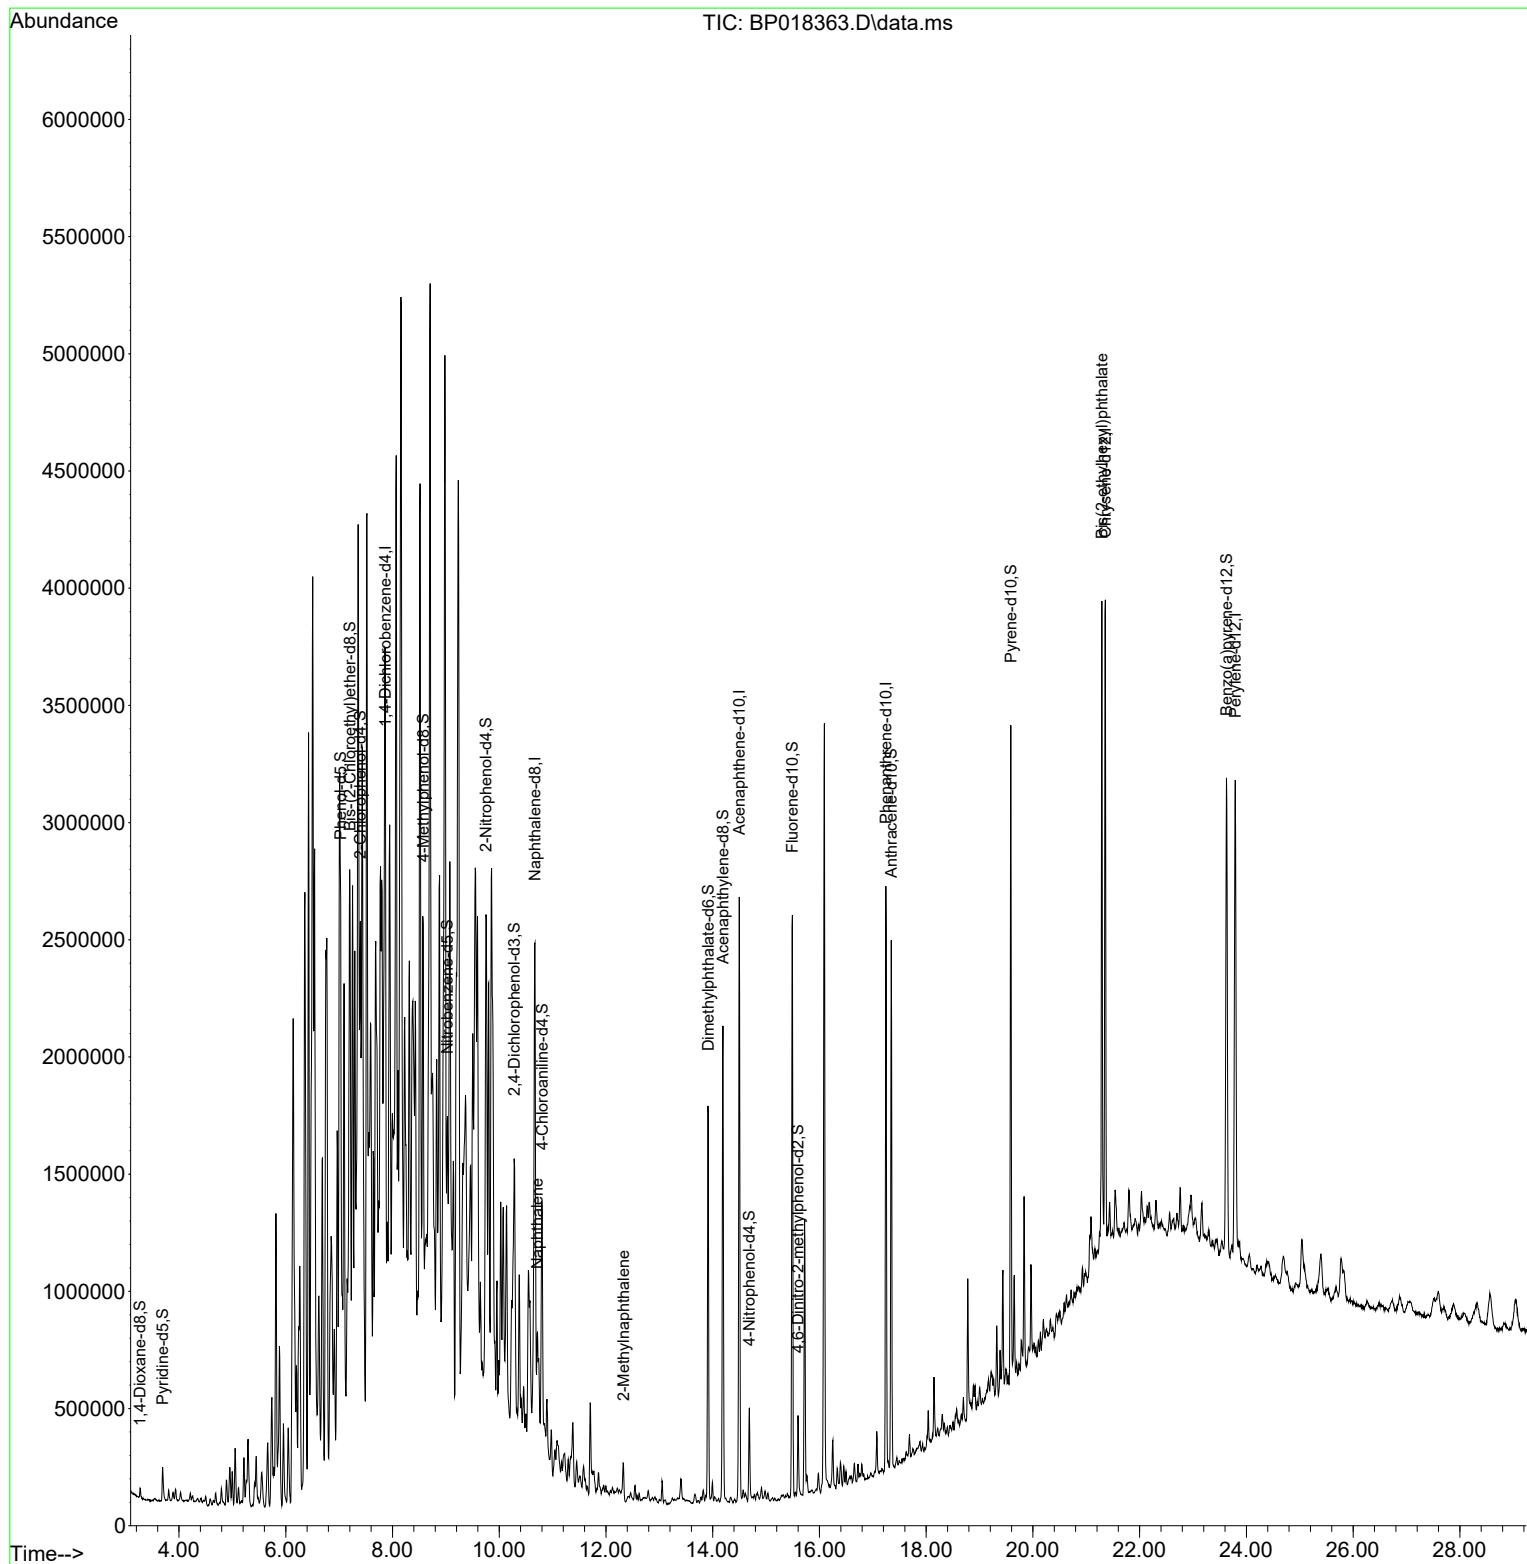


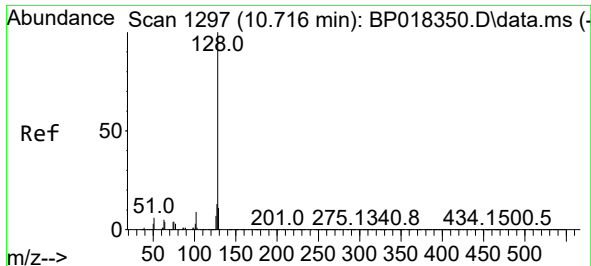

#30
Naphthalene
Concen: 1.010 ng/ul
RT: 10.716 min Scan# 1297
Delta R.T. -0.006 min
Lab File: BP018363.D
Acq: 25 Nov 2023 11:57




Instrument :
BNA_P
ClientSampleId :
DCKR8


Tgt Ion:128 Resp: 93218
Ion Ratio Lower Upper
128 100
129 19.8 8.9 13.3#
127 14.7 10.4 15.6

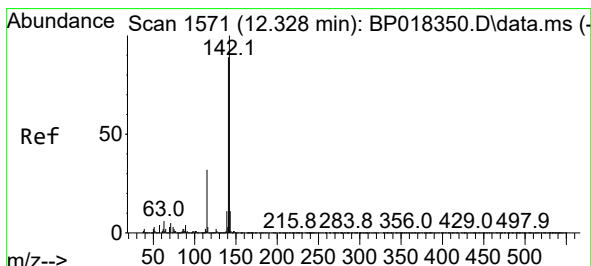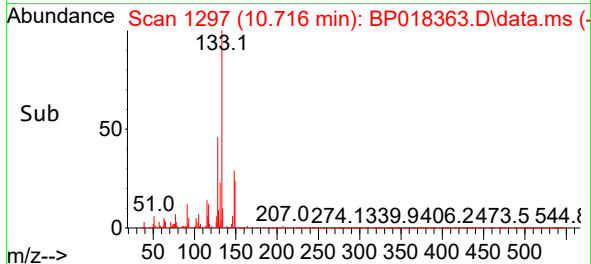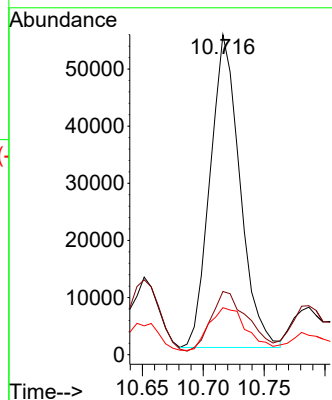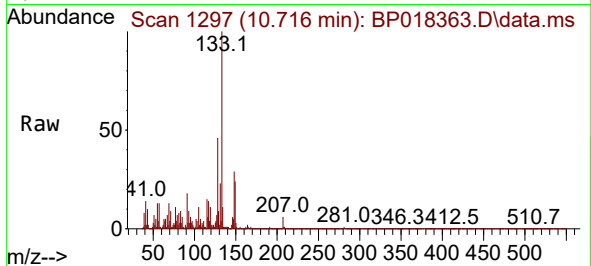

#36
2-Methylnaphthalene
Concen: 1.155 ng/ul
RT: 12.328 min Scan# 1571
Delta R.T. -0.000 min
Lab File: BP018363.D
Acq: 25 Nov 2023 11:57

Tgt Ion:142 Resp: 75414
Ion Ratio Lower Upper
142 100
141 88.7 71.0 106.4

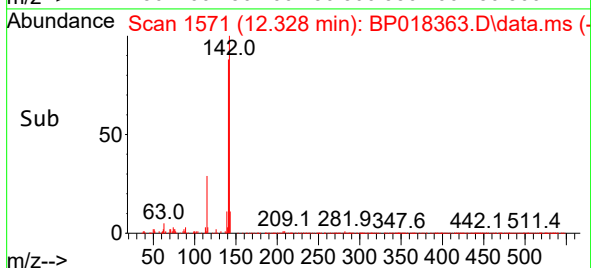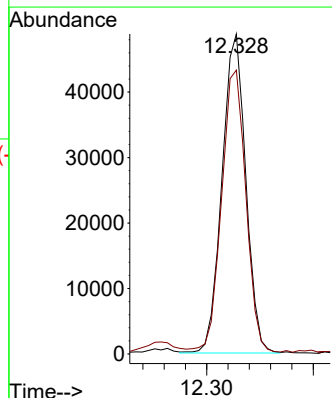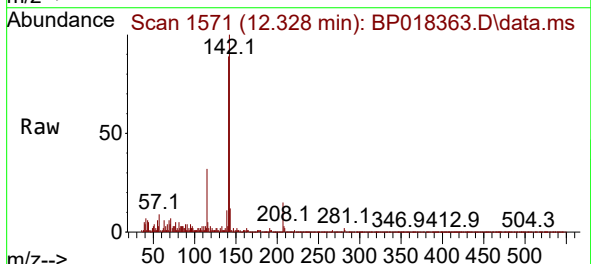

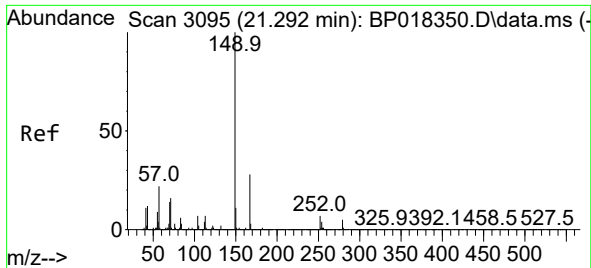

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 15.057 ng/ul
 RT: 21.292 min Scan# 3095
 Delta R.T. -0.000 min
 Lab File: BP018363.D
 Acq: 25 Nov 2023 11:57

Instrument :
 BNA_P
 ClientSampleId :
 DCKR8

Tgt Ion:149 Resp: 1079715
 Ion Ratio Lower Upper
 149 100
 167 28.6 22.1 33.1
 279 4.8 3.4 5.0

