

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018364.D
 Acq On : 25 Nov 2023 12:31
 Operator : MA/JU
 Sample : 05261-16
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKT0

Quant Time: Nov 27 01:21:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	419069	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	1568054	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.498	164	907277	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	1546887	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	1411324	20.000	ng/ul	0.00
88) Perylene-d12	23.798	264	1821605	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	20862	1.865	ng/uL	0.00
4) Pyridine-d5	3.693	84	68169	2.217	ng/ul	0.00
7) Phenol-d5	7.028	99	382685	9.992	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	441776	19.290	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	303395	9.435	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	312407	10.108	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	129478	10.166	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143	118793	10.099	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	292689	10.314	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	243366	6.359	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	940363	11.648	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1053829	11.456	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	91868	8.243	ng/ul	0.00
60) Fluorene-d10	15.492	176	778495	11.529	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	75842	11.517	ng/ul	0.00
73) Anthracene-d10	17.345	188	1027787	12.431	ng/ul	0.00
81) Pyrene-d10	19.586	212	1202783	10.708	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	1280691	12.127	ng/ul	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.298	149	4546546	60.602	ng/ul#	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018364.D
Acq On : 25 Nov 2023 12:31
Operator : MA/JU
Sample : 05261-16
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKT0

Quant Time: Nov 27 01:21:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 24 22:02:00 2023
Response via : Initial Calibration

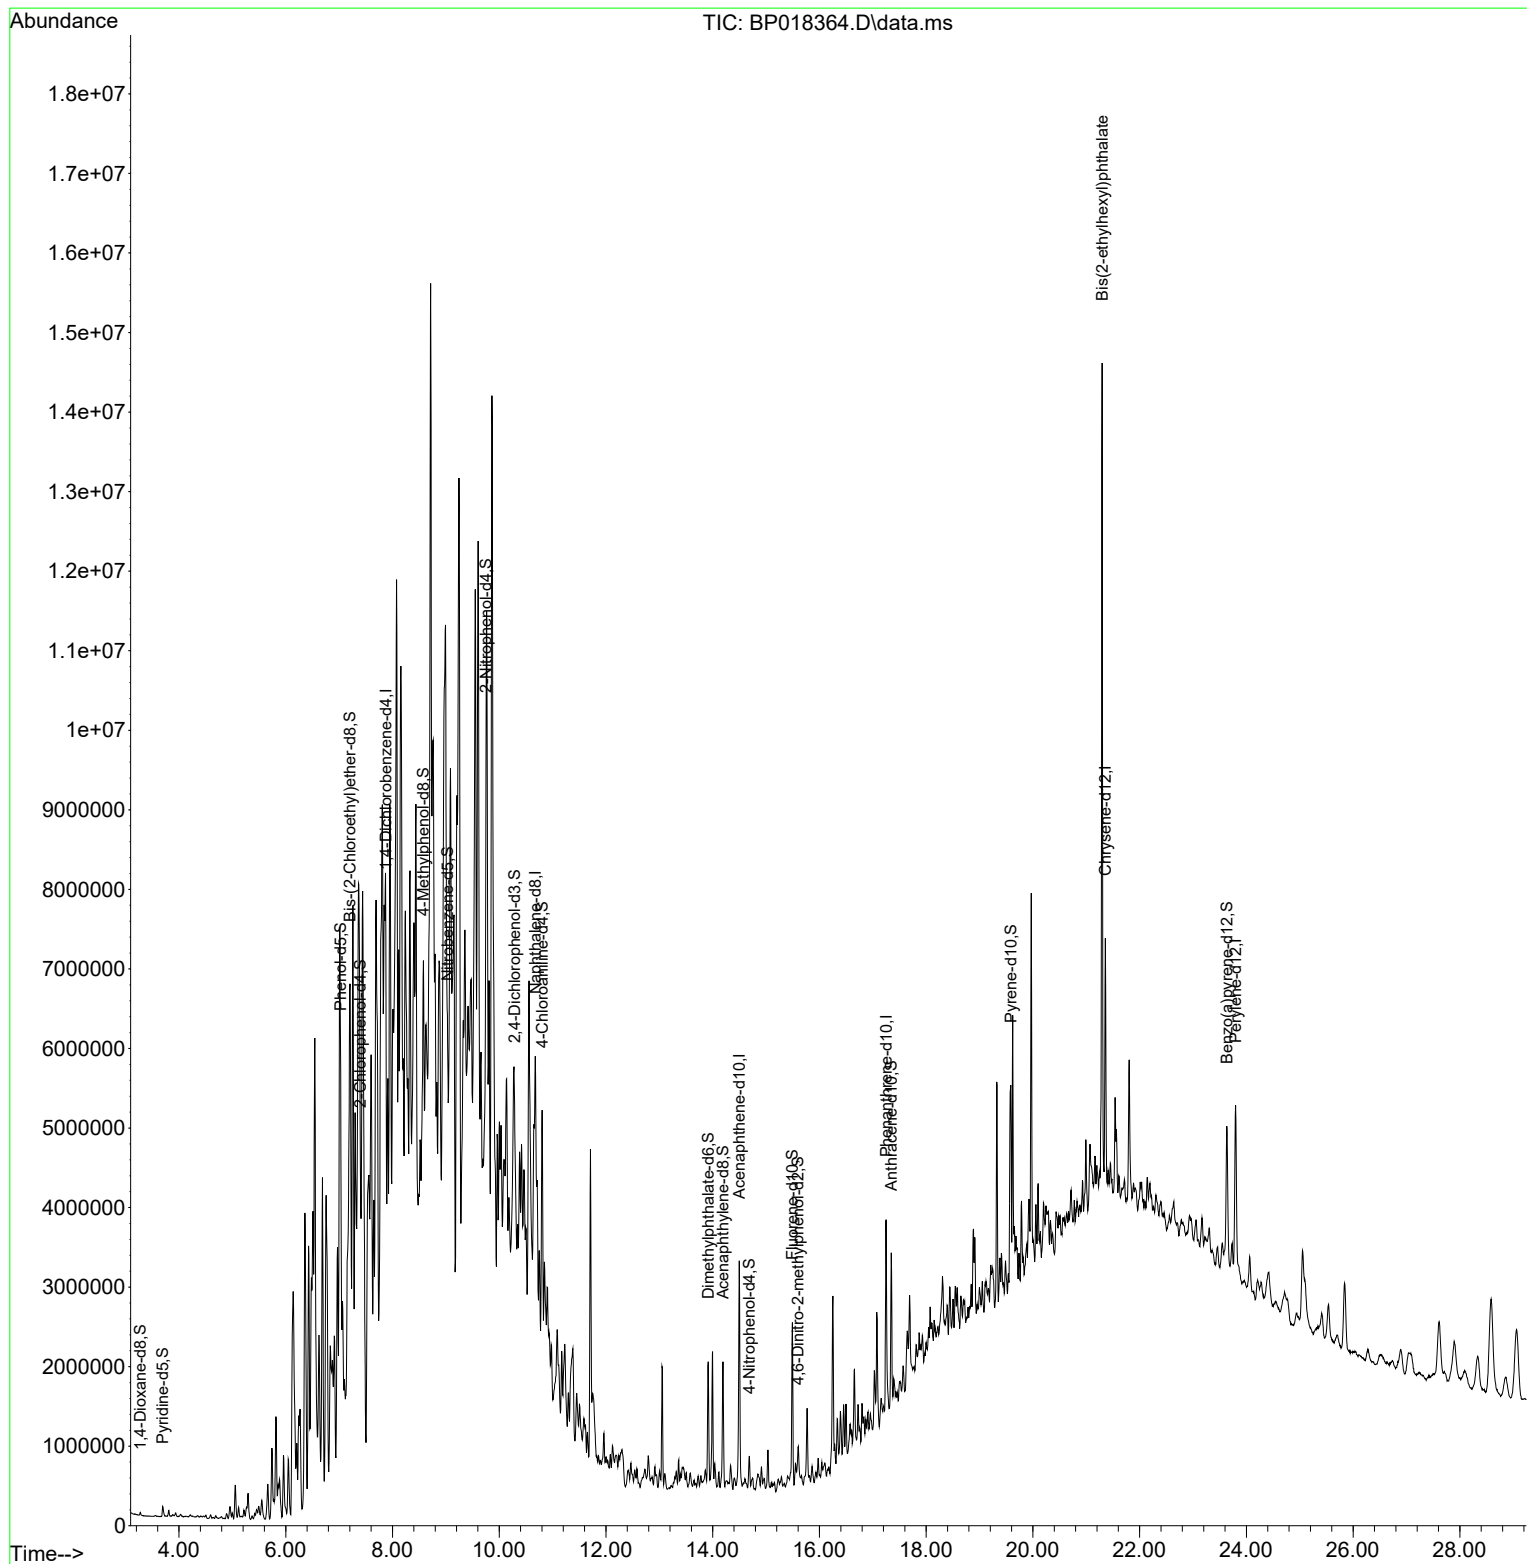

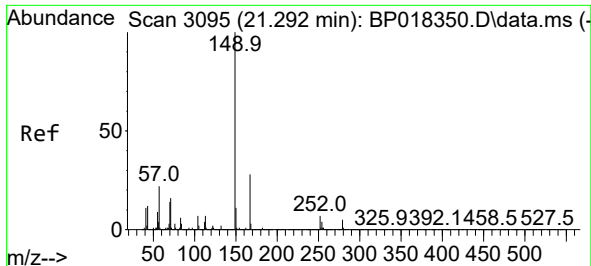

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 60.602 ng/ul
 RT: 21.298 min Scan# 3096
 Delta R.T. 0.006 min
 Lab File: BP018364.D
 Acq: 25 Nov 2023 12:31

Instrument :
 BNA_P
 ClientSampleId :
 DCKT0

Tgt Ion:149 Resp: 4546546
 Ion Ratio Lower Upper
 149 100
 167 29.6 22.1 33.1
 279 6.1 3.4 5.0#

