

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018365.D
 Acq On : 25 Nov 2023 13:05
 Operator : MA/JU
 Sample : 05261-04
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKR5

Quant Time: Nov 27 00:00:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	426404	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	1642138	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	895262	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	1562364	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	1474006	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	1821884	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	34632	3.042	ng/uL	0.00
4) Pyridine-d5	3.693	84	87684	2.803	ng/ul	0.00
7) Phenol-d5	7.028	99	673649	17.287	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	382519	16.415	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	574218	17.550	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	521685	16.588	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	268491	20.130	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	264727	21.491	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	543015	18.272	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	445534	11.116	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	1565130	19.647	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1776068	19.567	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	150973	13.728	ng/ul	0.00
60) Fluorene-d10	15.492	176	1249005	18.745	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	91912	13.819	ng/ul	0.00
73) Anthracene-d10	17.345	188	1648587	19.742	ng/ul	0.00
81) Pyrene-d10	19.586	212	1915365	16.327	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	2180319	20.642	ng/ul	0.01
Target Compounds						
					Qvalue	
8) Phenol	7.057	94	49964	1.307	ng/ul	98
16) Acetophenone	8.693	105	207455	4.311	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018365.D
Acq On : 25 Nov 2023 13:05
Operator : MA/JU
Sample : 05261-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKR5

Quant Time: Nov 27 00:00:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 24 22:02:00 2023
Response via : Initial Calibration




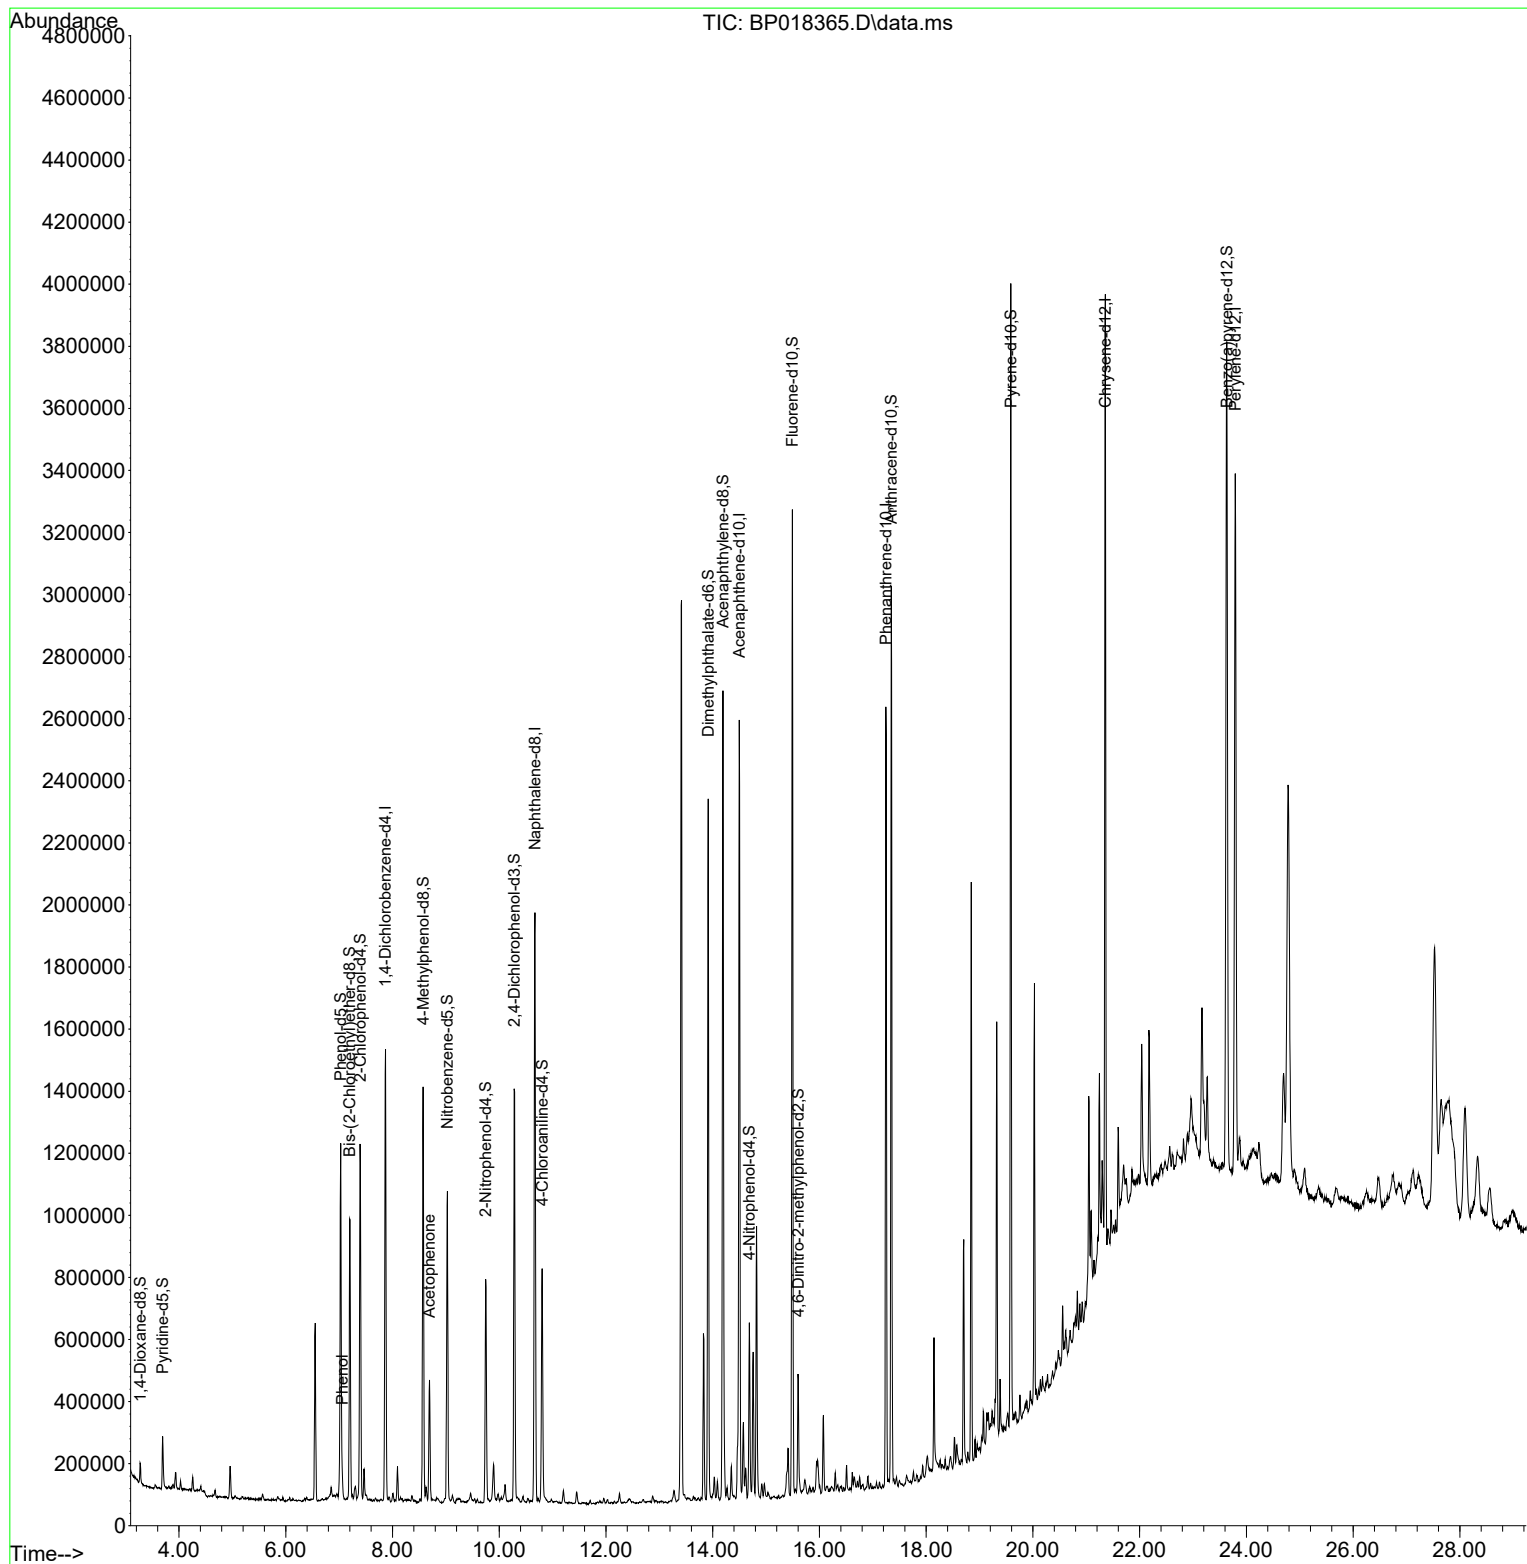


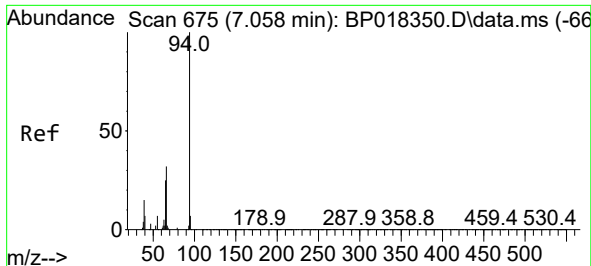

#8
Phenol
Concen: 1.307 ng/ul
RT: 7.057 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP018365.D
Acq: 25 Nov 2023 13:05

Instrument :
BNA_P
ClientSampleId :
DCKR5

Tgt Ion:	94	Resp:	49964
Ion	Ratio	Lower	Upper
94	100		
65	27.2	21.2	31.8
66	33.6	28.0	42.0

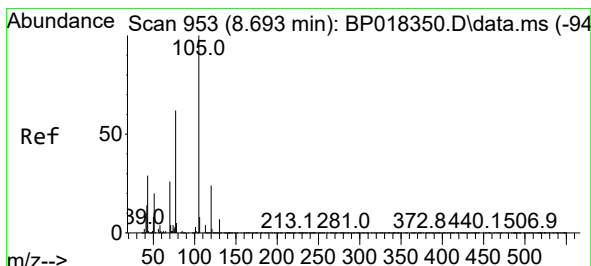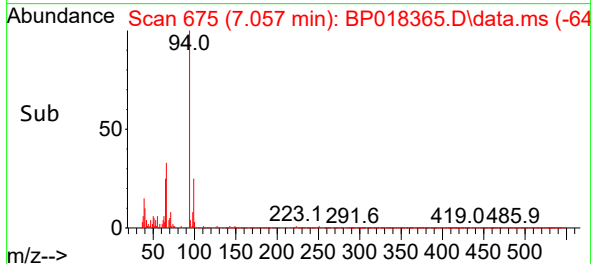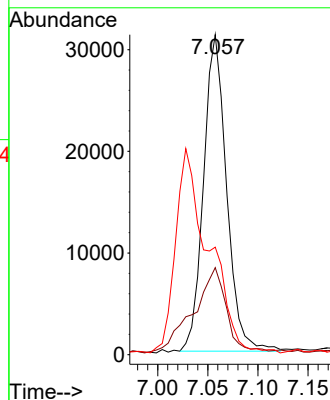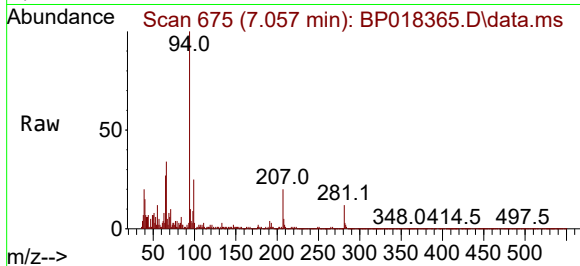

#16
Acetophenone
Concen: 4.311 ng/ul
RT: 8.693 min Scan# 953
Delta R.T. -0.000 min
Lab File: BP018365.D
Acq: 25 Nov 2023 13:05

Tgt Ion:	105	Resp:	207455
Ion	Ratio	Lower	Upper
105	100		
77	69.9	59.5	89.3
51	22.1	20.5	30.7

