

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018380.D
 Acq On : 25 Nov 2023 22:06
 Operator : MA/JU
 Sample : 05261-07
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKQ6

Quant Time: Nov 27 02:03:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 24 22:02:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	392566	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	1403399	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.498	164	713573	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	1328499	20.000	ng/u1	0.00
79) Chrysene-d12	21.357	240	1441278	20.000	ng/u1	0.00
88) Perylene-d12	23.798	264	1737833	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	32859	3.135	ng/uL	0.00
4) Pyridine-d5	3.693	84	55836	1.939	ng/u1	0.00
7) Phenol-d5	7.028	99	593170	16.534	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	373827	17.425	ng/u1	0.00
11) 2-Chlorophenol-d4	7.393	132	526395	17.475	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	300453	10.377	ng/u1	-0.01
21) Nitrobenzene-d5	9.022	128	243486	21.360	ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	231830	22.022	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	446060	17.563	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	83828	2.447	ng/u1	0.00
46) Dimethylphthalate-d6	13.910	166	1201477	18.923	ng/u1	-0.01
49) Acenaphthylene-d8	14.187	160	1387353	19.176	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	139141	15.874	ng/u1	0.00
60) Fluorene-d10	15.487	176	1003851	18.902	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	88187	15.594	ng/u1	0.00
73) Anthracene-d10	17.345	188	1216555	17.133	ng/u1	0.00
81) Pyrene-d10	19.586	212	1768748	15.420	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.633	264	1799432	17.860	ng/u1	0.01
Target Compounds						
					Qvalue	
8) Phenol	7.058	94	63409	1.802	ng/u1	95
16) Acetophenone	8.687	105	241598	5.453	ng/u1	98
72) Phenanthrene	17.286	178	133782	1.656	ng/u1	99
80) Fluoranthene	19.257	202	239869	1.750	ng/u1	99
82) Pyrene	19.616	202	223026	1.616	ng/u1	98
87) Chrysene	21.392	228	123552	1.156	ng/u1	99
90) Benzo(b)fluoranthene	23.051	252	161303	1.278	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018380.D
Acq On : 25 Nov 2023 22:06
Operator : MA/JU
Sample : 05261-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKQ6

Quant Time: Nov 27 02:03:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 24 22:02:00 2023
Response via : Initial Calibration




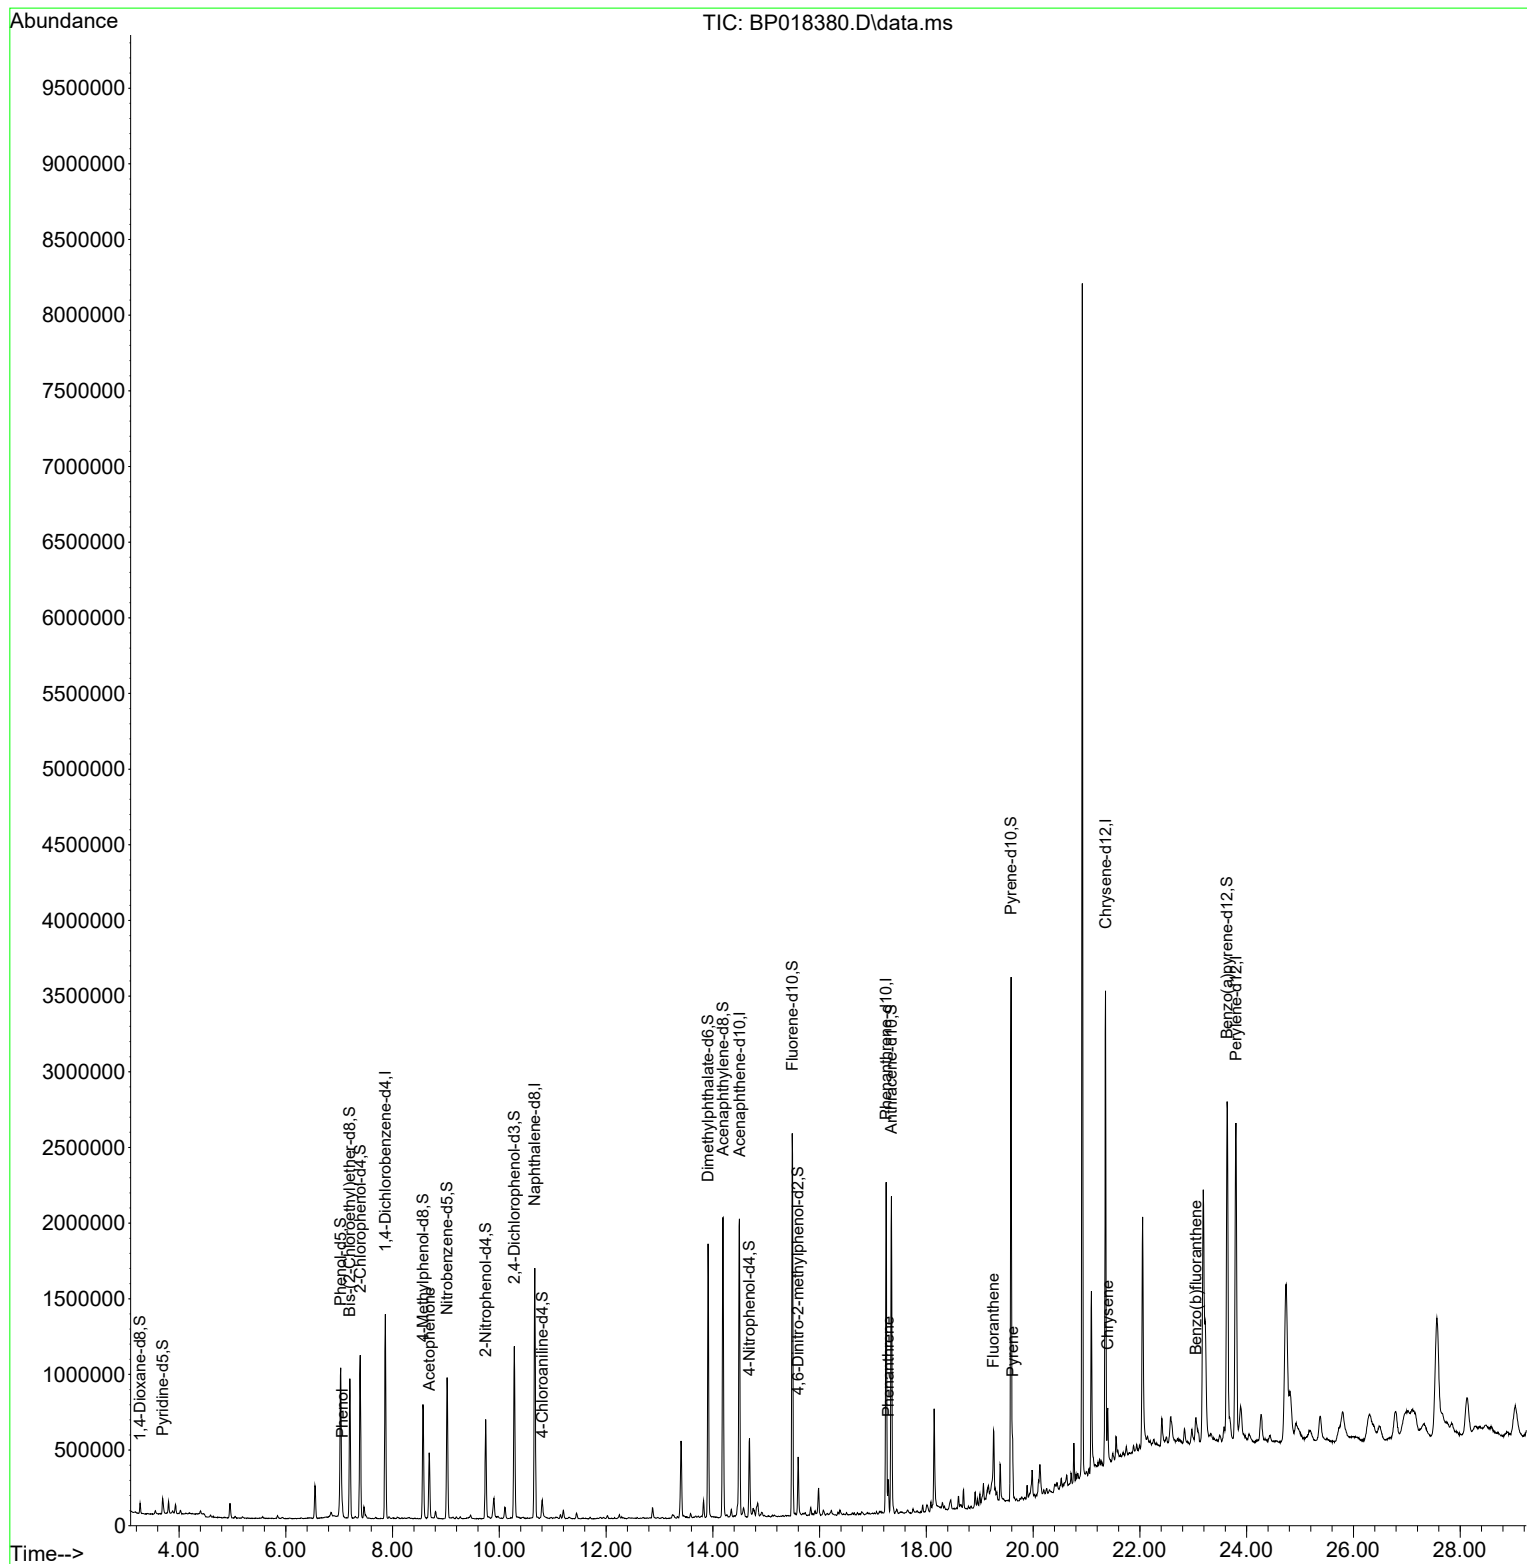


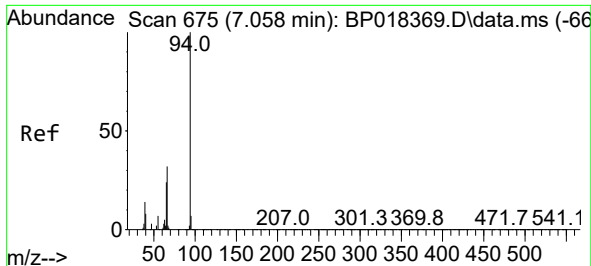

#8
Phenol
Concen: 1.802 ng/ul
RT: 7.058 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP018380.D
Acq: 25 Nov 2023 22:06




Instrument :
BNA_P
ClientSampleId :
DCKQ6


Tgt Ion: 94 Resp: 63409
Ion Ratio Lower Upper
94 100
65 25.1 21.2 31.8
66 31.4 28.0 42.0

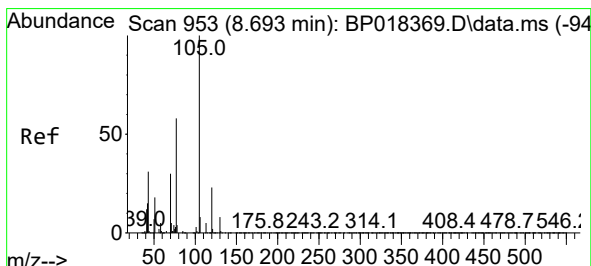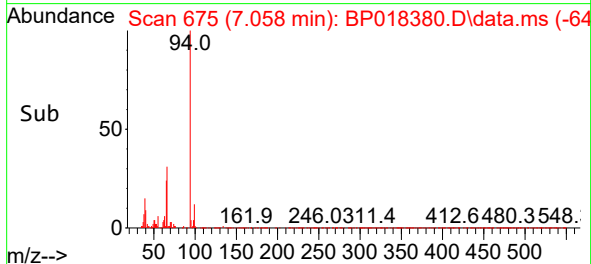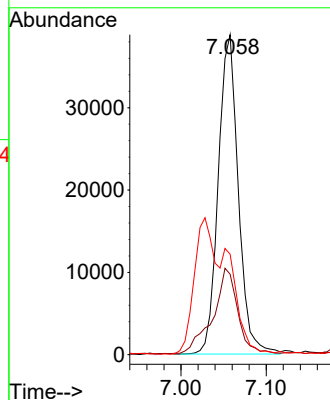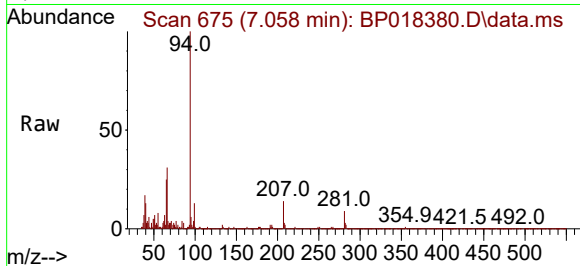

#16
Acetophenone
Concen: 5.453 ng/ul
RT: 8.687 min Scan# 952
Delta R.T. -0.006 min
Lab File: BP018380.D
Acq: 25 Nov 2023 22:06

Tgt Ion: 105 Resp: 241598
Ion Ratio Lower Upper
105 100
77 73.0 59.5 89.3
51 23.5 20.5 30.7


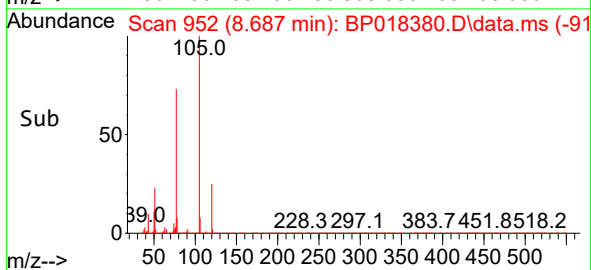
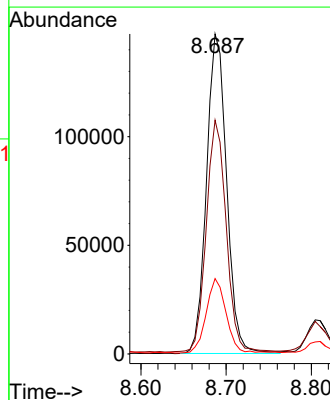
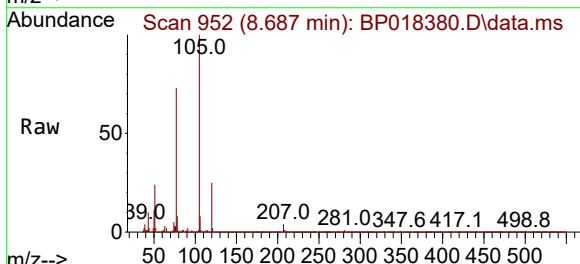


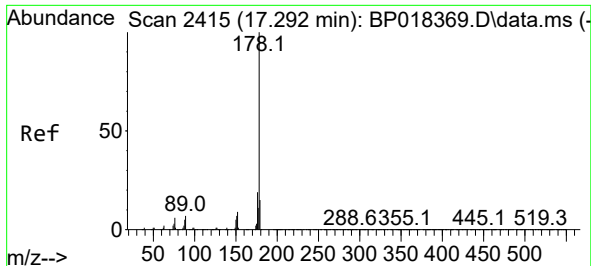

#72
Phenanthrene
Concen: 1.656 ng/ul
RT: 17.286 min Scan# 2415
Delta R.T. -0.006 min
Lab File: BP018380.D
Acq: 25 Nov 2023 22:06




Instrument :
BNA_P
ClientSampleId :
DCKQ6


Tgt Ion:178 Resp: 133782
Ion Ratio Lower Upper
178 100
179 16.1 12.4 18.6
176 19.4 15.1 22.7

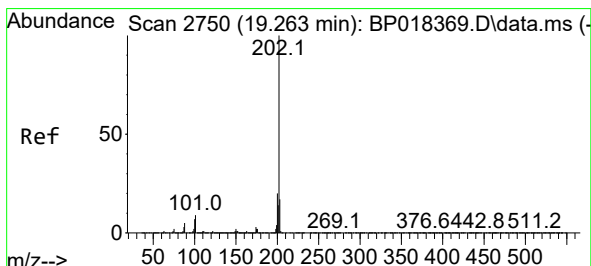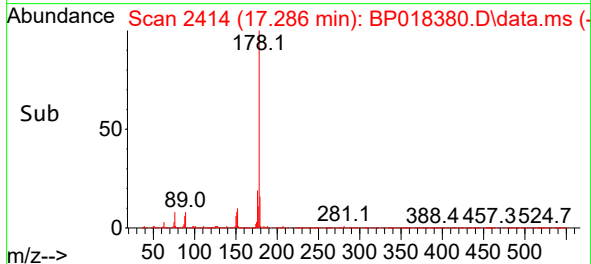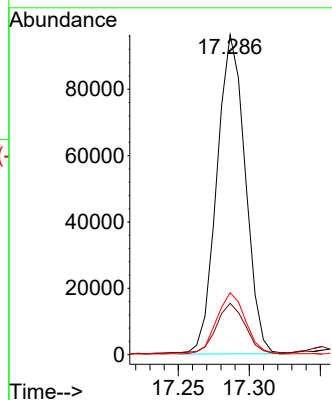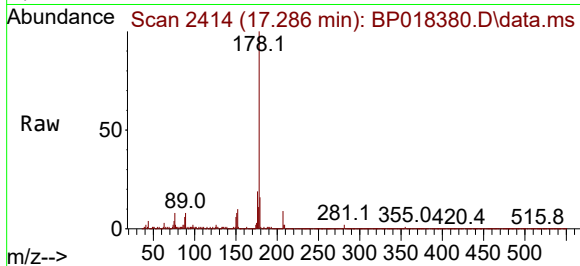

#80
Fluoranthene
Concen: 1.750 ng/ul
RT: 19.257 min Scan# 2749
Delta R.T. -0.006 min
Lab File: BP018380.D
Acq: 25 Nov 2023 22:06

Tgt Ion:202 Resp: 239869
Ion Ratio Lower Upper
202 100
101 11.2 8.6 13.0
100 7.7 6.7 10.1

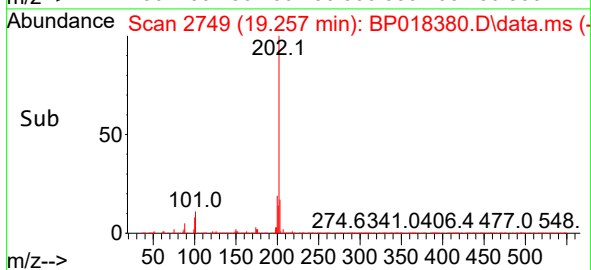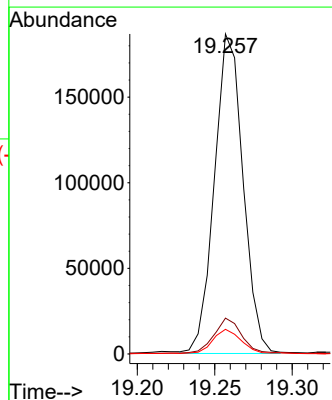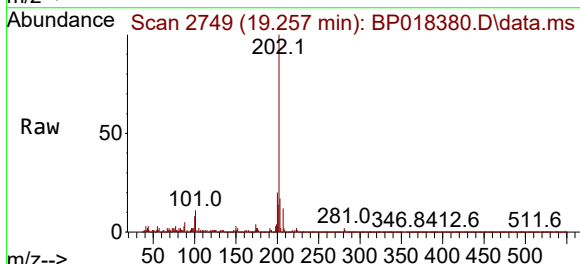

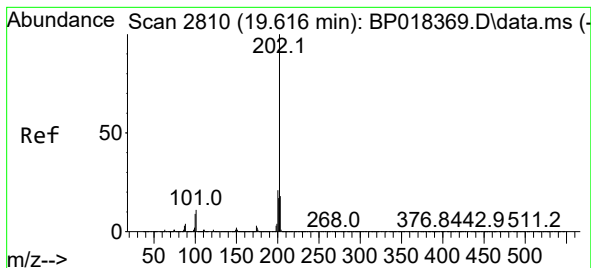

#82

Pyrene

Concen: 1.616 ng/ul

RT: 19.616 min Scan# 2810

Delta R.T. 0.000 min

Lab File: BP018380.D

Acq: 25 Nov 2023 22:06

Instrument :

BNA_P

ClientSampleId :

DCKQ6





Tgt Ion:202 Resp: 223026

Ion Ratio Lower Upper

202 100

101 12.0 10.2 15.4

100 9.8 8.4 12.6

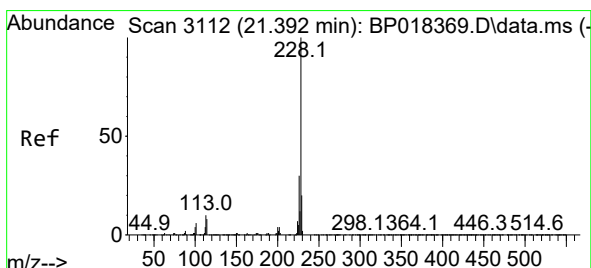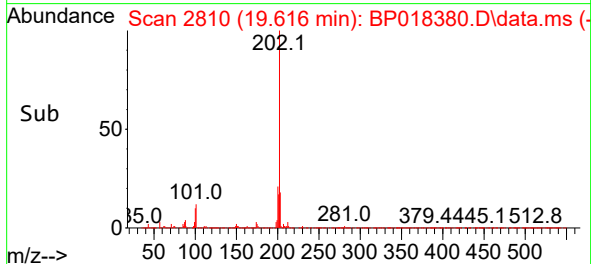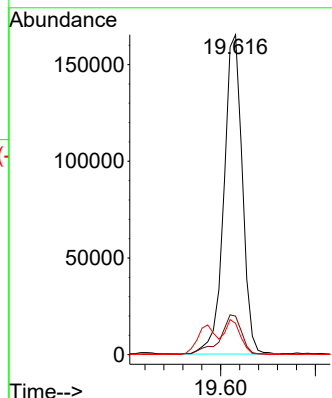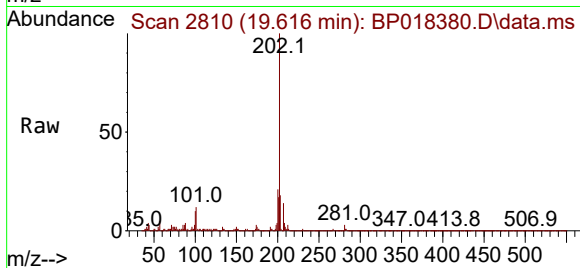

#87

Chrysene

Concen: 1.156 ng/ul

RT: 21.392 min Scan# 3112

Delta R.T. 0.000 min

Lab File: BP018380.D

Acq: 25 Nov 2023 22:06




Tgt Ion:228 Resp: 123552


Ion Ratio Lower Upper

228 100

226 30.0 24.2 36.4


229 21.1 16.1 24.1

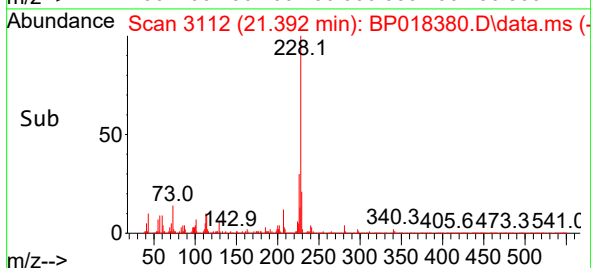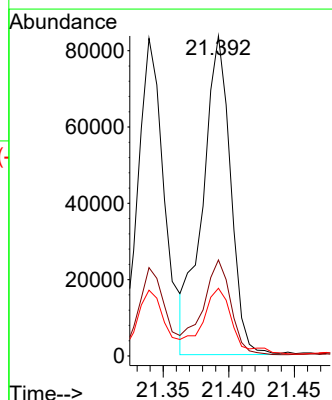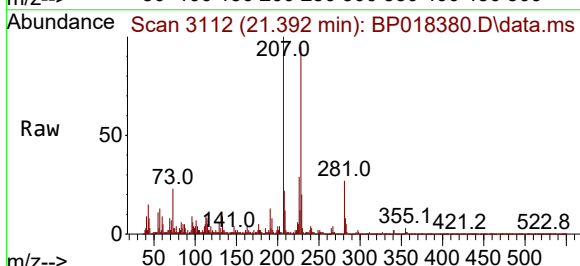

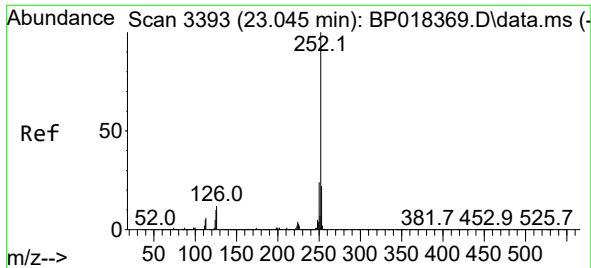

#90
Benzo(b)fluoranthene
Concen: 1.278 ng/ul
RT: 23.051 min Scan# 31
Delta R.T. 0.012 min
Lab File: BP018380.D
Acq: 25 Nov 2023 22:06

Instrument :
BNA_P
ClientSampleId :
DCKQ6

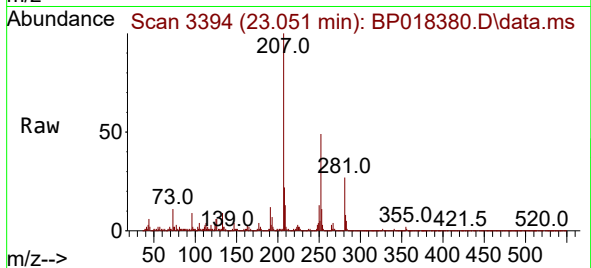

Tgt Ion:252 Resp: 161303
Ion Ratio Lower Upper
252 100
253 23.5 17.7 26.5
125 11.8 8.4 12.6

