

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018321.D
 Acq On : 24 Nov 2023 09:42
 Operator : MA/JU
 Sample : PB157173BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	40	rVB	127600	169000	2.06%	0.184%
2	3.687	97	102	120	rBV	1330628	1972397	24.05%	2.150%
3	4.028	156	160	165	rVB2	23369	35121	0.43%	0.038%
4	7.028	662	670	685	rVB	1744212	2664997	32.49%	2.905%
5	7.205	693	700	711	rVB	1493359	2261999	27.58%	2.466%
6	7.393	725	732	745	rBV	1692687	2705407	32.98%	2.949%
7	7.869	805	813	820	rVB	1376150	2130754	25.98%	2.323%
8	8.575	926	933	944	rBV	2200128	3392308	41.36%	3.698%
9	9.028	1002	1010	1021	rBV	1628200	2573122	31.37%	2.805%
10	9.752	1122	1133	1145	rBV	1120615	1798783	21.93%	1.961%
11	10.287	1216	1224	1233	rBV	2056851	3408838	41.56%	3.716%
12	10.669	1280	1289	1297	rBV	1895148	3128997	38.15%	3.411%
13	10.805	1304	1312	1328	rBV	1748782	2915184	35.54%	3.178%
14	11.952	1501	1507	1508	rBV6	6649	8677	0.11%	0.009%
15	12.257	1554	1559	1568	rBV3	42635	71853	0.88%	0.078%
16	12.693	1628	1633	1637	rBV8	5374	11668	0.14%	0.013%
17	12.893	1662	1667	1672	rBV7	7429	14470	0.18%	0.016%
18	13.416	1750	1756	1761	rBV4	18951	30797	0.38%	0.034%
19	13.481	1761	1767	1770	rVB6	7546	11521	0.14%	0.013%
20	13.922	1835	1842	1855	rBV	3973559	5538674	67.53%	6.038%
21	14.199	1880	1889	1897	rBV	4536955	6688818	81.55%	7.292%
22	14.504	1933	1941	1948	rBV	3102086	4393830	53.57%	4.790%
23	14.687	1966	1972	1986	rBV	1301409	1869054	22.79%	2.038%
24	14.863	1999	2002	2006	rVV6	7894	8273	0.10%	0.009%
25	14.910	2007	2010	2017	rVB9	9136	19723	0.24%	0.022%
26	15.234	2060	2065	2067	rBV6	4746	8608	0.10%	0.009%
27	15.498	2103	2110	2116	rBV	5722991	8202364	100.00%	8.942%
28	15.604	2122	2128	2139	rBV	943718	1292621	15.76%	1.409%
29	15.734	2146	2150	2156	rVB	23568	33106	0.40%	0.036%
30	16.763	2322	2325	2330	rBV6	7524	10249	0.12%	0.011%
31	16.928	2351	2353	2361	rVB9	7625	11679	0.14%	0.013%
32	17.040	2368	2372	2375	rBV4	8768	12905	0.16%	0.014%
33	17.134	2384	2388	2393	rBV7	9221	16970	0.21%	0.018%
34	17.251	2402	2408	2415	rBV	3422296	4776348	58.23%	5.207%
35	17.351	2419	2425	2437	rVV2	5808798	8189539	99.84%	8.928%
36	17.628	2469	2472	2476	rVB5	8846	8360	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018321.D
Acq On : 24 Nov 2023 09:42
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	17.845	2505	2509	2513	rBV7	6937	9627	0.12%	0.010%
38	18.163	2557	2563	2566	rBV8	7209	16808	0.20%	0.018%
39	19.169	2730	2734	2740	rVB2	64157	85397	1.04%	0.093%
40	19.234	2741	2745	2750	rBV	61802	78738	0.96%	0.086%
41	19.592	2800	2806	2813	rBV	6362088	8118304	98.98%	8.850%
42	21.357	3101	3106	3112	rBV	2771373	3413099	41.61%	3.721%
43	23.627	3485	3492	3506	rBV2	3161826	6129613	74.73%	6.682%
44	23.786	3512	3519	3536	rVB	1649207	3492167	42.58%	3.807%




Sum of corrected areas: 91730767

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018321.D
Acq On : 24 Nov 2023 09:42
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

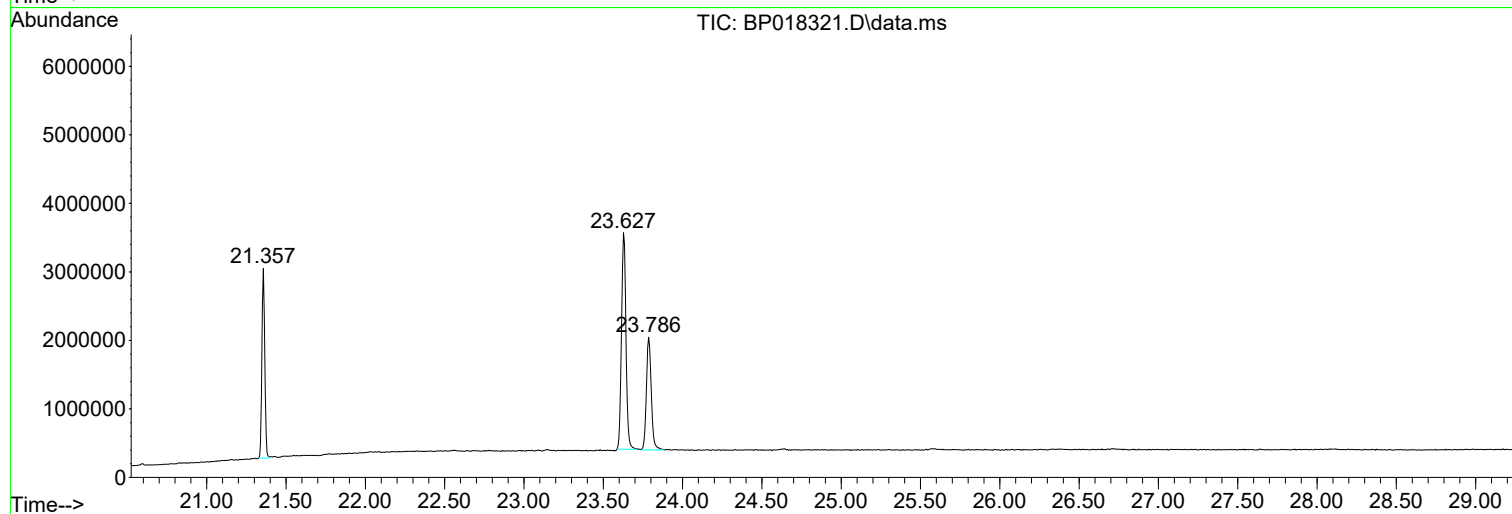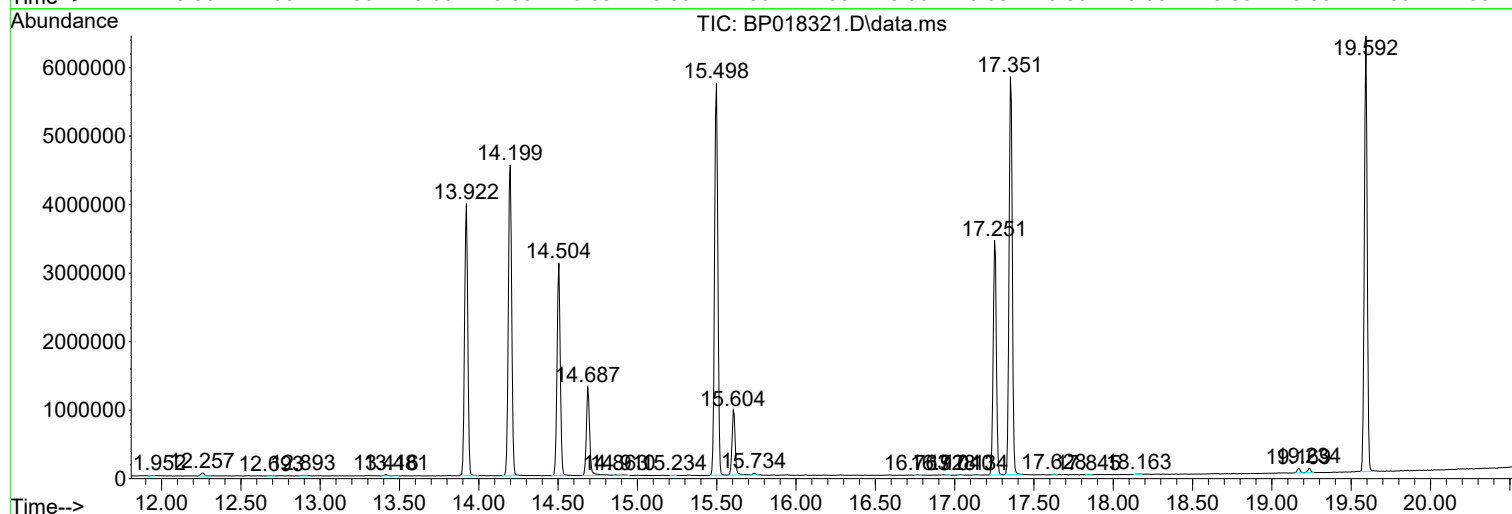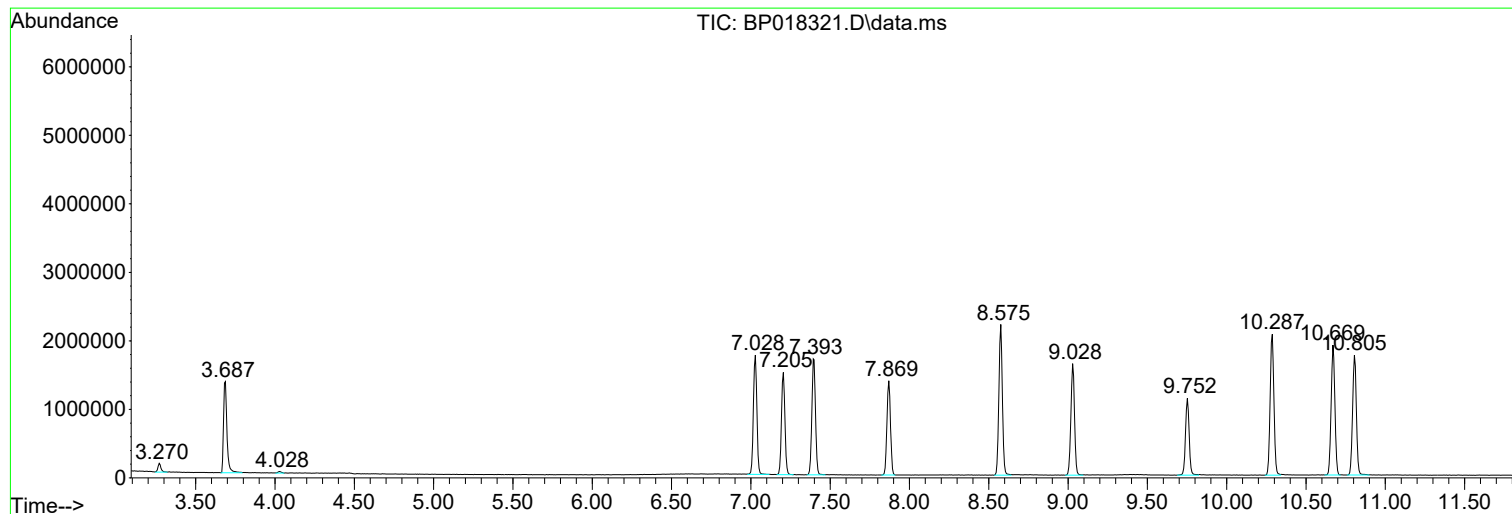

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018321.D
Acq On : 24 Nov 2023 09:42
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018321.D
Acq On : 24 Nov 2023 09:42
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc