

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018325.D
 Acq On : 24 Nov 2023 13:32
 Operator : MA/JU
 Sample : 05261-03DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKV4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	35	rVB3	21318	28282	0.23%	0.013%
2	4.023	156	159	165	rVB	28209	36596	0.30%	0.016%
3	4.558	247	250	256	rBV7	10157	16285	0.13%	0.007%
4	6.234	530	535	537	rBV4	12299	21212	0.18%	0.009%
5	7.046	662	673	687	rVB2	2219340	3952983	32.77%	1.755%
6	7.199	692	699	708	rVV	300753	470126	3.90%	0.209%
7	7.287	708	714	724	rVB	605368	903580	7.49%	0.401%
8	7.422	732	737	747	rVB	1471485	2377948	19.71%	1.056%
9	7.752	786	793	799	rBV	882427	1370303	11.36%	0.608%
10	7.864	804	812	814	rBV	1459627	2220685	18.41%	0.986%
11	7.899	814	818	828	rVB	3456844	5299453	43.93%	2.353%
12	8.099	847	852	857	rBV9	11395	22471	0.19%	0.010%
13	8.216	863	872	880	rBV	2320037	3737950	30.99%	1.659%
14	8.569	926	932	942	rBV	390517	603461	5.00%	0.268%
15	8.675	942	950	957	rBV	1855931	2871437	23.80%	1.275%
16	8.946	988	996	1003	rBV	2045527	3297416	27.33%	1.464%
17	9.022	1003	1009	1012	rVV	320405	517044	4.29%	0.230%
18	9.063	1012	1016	1023	rVB	636261	1002560	8.31%	0.445%
19	9.440	1077	1080	1084	rBV2	11499	15393	0.13%	0.007%
20	9.746	1124	1132	1133	rBV	210550	277379	2.30%	0.123%
21	9.775	1133	1137	1149	rVB	588927	1007139	8.35%	0.447%
22	10.087	1182	1190	1199	rBV	1227339	1926572	15.97%	0.855%
23	10.305	1216	1227	1236	rBV2	1160704	2544109	21.09%	1.129%
24	10.534	1260	1266	1271	rVB9	10186	18413	0.15%	0.008%
25	10.669	1280	1289	1292	rBV	1893508	3198263	26.51%	1.420%
26	10.716	1292	1297	1305	rVV	4641231	7639832	63.33%	3.391%
27	10.799	1305	1311	1324	rVB	254250	443070	3.67%	0.197%
28	10.975	1336	1341	1346	rVB5	9571	16058	0.13%	0.007%
29	11.946	1499	1506	1515	rVV	2072124	3149817	26.11%	1.398%
30	12.252	1553	1558	1567	rVB4	12821	27515	0.23%	0.012%
31	12.657	1623	1627	1633	rBV9	10287	25829	0.21%	0.011%
32	12.752	1639	1643	1649	rVB2	20104	32992	0.27%	0.015%
33	12.869	1657	1663	1667	rBV6	22998	46405	0.38%	0.021%
34	12.934	1667	1674	1679	rVV	1447895	2231189	18.50%	0.990%
35	12.999	1679	1685	1699	rVB	3081413	4699410	38.96%	2.086%
36	13.375	1739	1749	1753	rBV	2332970	3675284	30.47%	1.632%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018325.D
 Acq On : 24 Nov 2023 13:32
 Operator : MA/JU
 Sample : 05261-03DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKV4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	13.416	1753	1756	1764	rVB	1600814	2211502	18.33%	0.982%
38	13.563	1775	1781	1789	rVB2	30182	55055	0.46%	0.024%
39	13.804	1820	1822	1831	rVB7	14152	21244	0.18%	0.009%
40	13.922	1836	1842	1852	rVB	753779	1097510	9.10%	0.487%
41	14.081	1860	1869	1879	rBV	3629445	4987391	41.34%	2.214%
42	14.222	1880	1893	1902	rVB2	5693357	9956598	82.54%	4.420%
43	14.504	1931	1941	1946	rBV	2547157	3852740	31.94%	1.710%
44	14.569	1946	1952	1959	rVB	4897166	7169210	59.43%	3.183%
45	14.640	1959	1964	1967	rBV	52724	63102	0.52%	0.028%
46	14.704	1967	1975	1990	rBV2	1803498	2779634	23.04%	1.234%
47	14.816	1990	1994	1997	rBV	52812	73504	0.61%	0.033%
48	14.863	1997	2002	2008	rVB	1883117	2491014	20.65%	1.106%
49	15.122	2040	2046	2051	rBV3	39745	64373	0.53%	0.029%
50	15.334	2074	2082	2093	rBV	6092618	7920748	65.66%	3.516%
51	15.498	2103	2110	2114	rBV	1160832	1678166	13.91%	0.745%
52	15.551	2114	2119	2125	rVV	6447003	8707610	72.18%	3.865%
53	15.604	2125	2128	2138	rVB	141076	193633	1.61%	0.086%
54	15.734	2145	2150	2157	rBV	7975	14624	0.12%	0.006%
55	15.804	2158	2162	2167	rVB2	26343	36215	0.30%	0.016%
56	15.945	2179	2186	2190	rVB7	13556	25671	0.21%	0.011%
57	16.051	2200	2204	2207	rBV6	10300	16163	0.13%	0.007%
58	16.093	2207	2211	2215	rVB	24343	34447	0.29%	0.015%
59	16.216	2228	2232	2239	rBV6	28109	51807	0.43%	0.023%
60	16.422	2264	2267	2272	rVB	31677	39209	0.33%	0.017%
61	16.557	2279	2290	2300	rBV	6677017	9584134	79.45%	4.255%
62	16.769	2322	2326	2330	rBV6	17745	24136	0.20%	0.011%
63	16.804	2330	2332	2338	rVB6	11477	19532	0.16%	0.009%
64	16.898	2341	2348	2360	rBV	3479107	4858275	40.27%	2.157%
65	16.992	2362	2364	2368	rVV5	17080	20536	0.17%	0.009%
66	17.051	2368	2374	2378	rVV8	25753	49767	0.41%	0.022%
67	17.251	2396	2408	2412	rBV	2475511	3657417	30.32%	1.624%
68	17.298	2412	2416	2421	rVV	2356417	3320881	27.53%	1.474%
69	17.351	2421	2425	2428	rVV	1032359	1583617	13.13%	0.703%
70	17.387	2428	2431	2443	rVB	3154651	4275336	35.44%	1.898%
71	17.657	2473	2477	2480	rBV	22600	26653	0.22%	0.012%
72	17.687	2480	2482	2488	rVB6	15247	24326	0.20%	0.011%
73	17.869	2506	2513	2517	rBV3	44529	77786	0.64%	0.035%
74	17.945	2522	2526	2531	rVB	102692	119526	0.99%	0.053%
75	18.151	2557	2561	2568	rBV2	125750	202341	1.68%	0.090%
76	18.228	2569	2574	2579	rVV	6282672	7293471	60.46%	3.238%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018325.D
 Acq On : 24 Nov 2023 13:32
 Operator : MA/JU
 Sample : 05261-03DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKV4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	18.498	2617	2620	2624	rVV	32249	39337	0.33%	0.017%
78	18.645	2640	2645	2652	rVB	201898	262751	2.18%	0.117%
79	19.004	2704	2706	2711	rBV5	16275	21491	0.18%	0.010%
80	19.057	2711	2715	2716	rBV3	76184	89916	0.75%	0.040%
81	19.081	2716	2719	2723	rVB	158672	183113	1.52%	0.081%
82	19.169	2732	2734	2737	rBV4	17322	19140	0.16%	0.008%
83	19.210	2738	2741	2744	rVV2	54622	59912	0.50%	0.027%
84	19.269	2745	2751	2763	rVB	7621788	9958693	82.55%	4.421%
85	19.392	2769	2772	2779	rBV2	82962	113536	0.94%	0.050%
86	19.504	2788	2791	2795	rBV	56203	64666	0.54%	0.029%
87	19.592	2801	2806	2808	rBV	1442067	1930280	16.00%	0.857%
88	19.622	2808	2811	2820	rVB	3706006	4680143	38.80%	2.078%
89	20.286	2921	2924	2928	rBV3	50951	52443	0.43%	0.023%
90	20.598	2973	2977	2981	rBV	102225	115124	0.95%	0.051%
91	21.092	3058	3061	3066	rBV3	131591	192667	1.60%	0.086%
92	21.233	3083	3085	3091	rVB	81791	87916	0.73%	0.039%
93	21.298	3092	3096	3100	rVV	8874343	10182990	84.41%	4.520%
94	21.351	3100	3105	3110	rVV2	6456146	11287161	93.57%	5.011%
95	21.404	3110	3114	3125	rVB	7747580	10316772	85.52%	4.580%
96	22.310	3265	3268	3274	rVB2	155123	202485	1.68%	0.090%
97	23.104	3395	3403	3410	rBV	6883111	12063439	100.00%	5.355%
98	23.633	3487	3493	3501	rVB	993386	1949295	16.16%	0.865%
99	23.792	3513	3520	3538	rVB2	1999447	4454118	36.92%	1.977%
100	26.404	3953	3964	3978	rVB	2693754	8536088	70.76%	3.789%


Sum of corrected areas: 225266841

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018325.D
Acq On : 24 Nov 2023 13:32
Operator : MA/JU
Sample : 05261-03DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKV4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

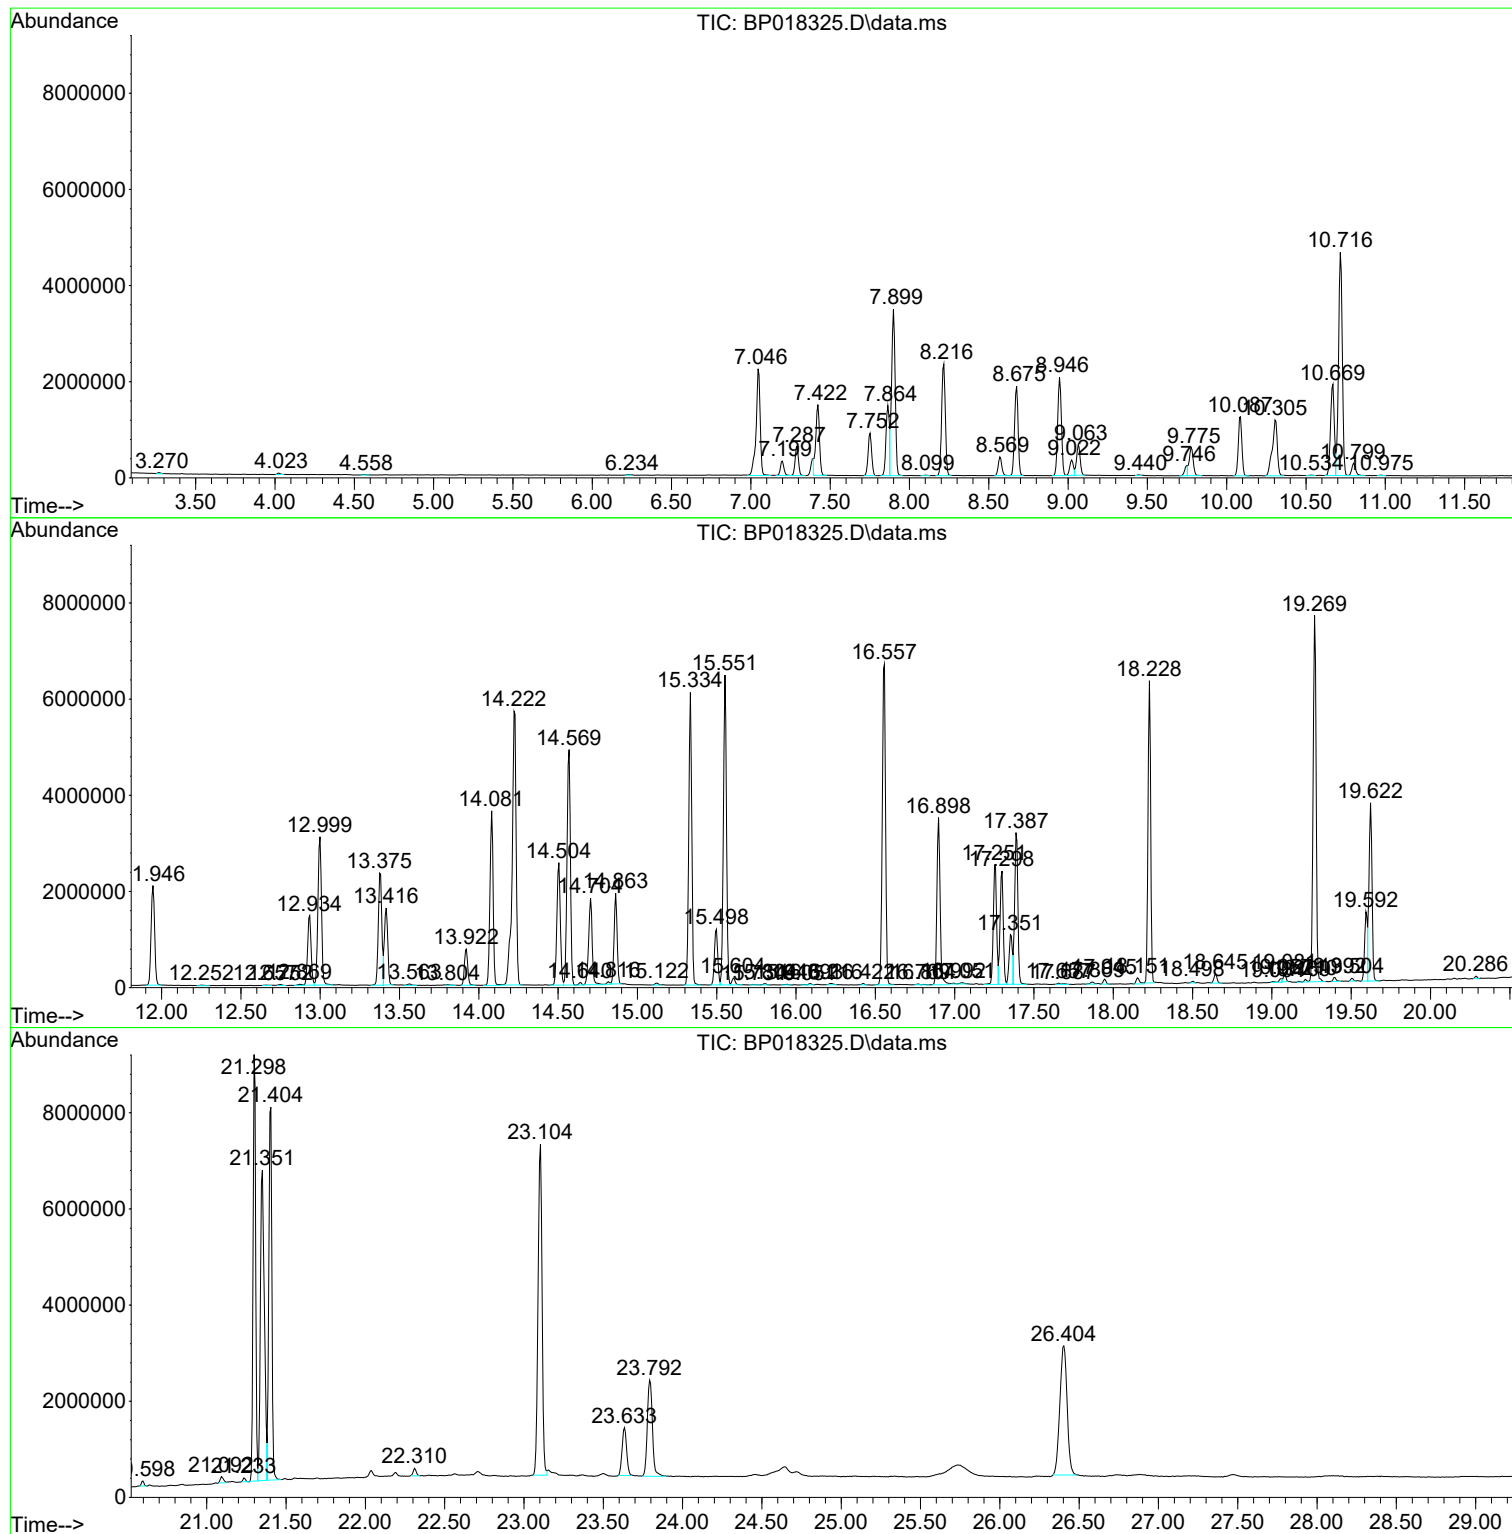

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018325.D
Acq On : 24 Nov 2023 13:32
Operator : MA/JU
Sample : 05261-03DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKV4DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,4-dichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.752	12.34 ng/ul	1370300	1,4-Dichlorobenzene-d4	7.864

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	98
2			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97
3			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97
4			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	97
5			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97

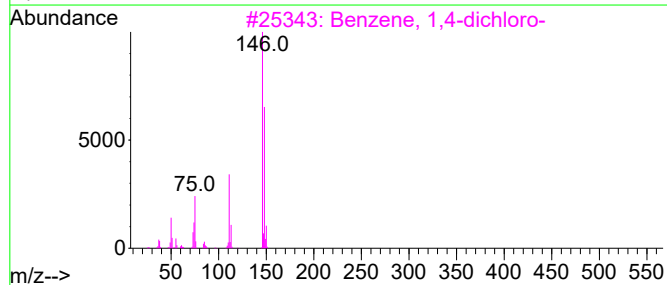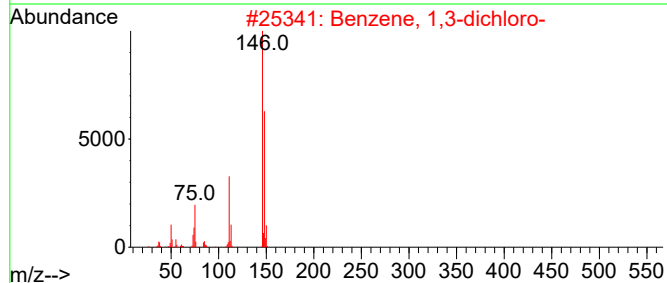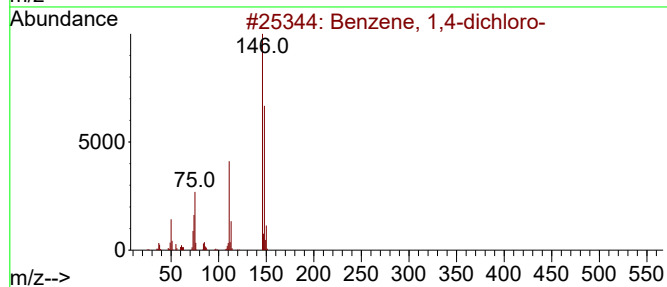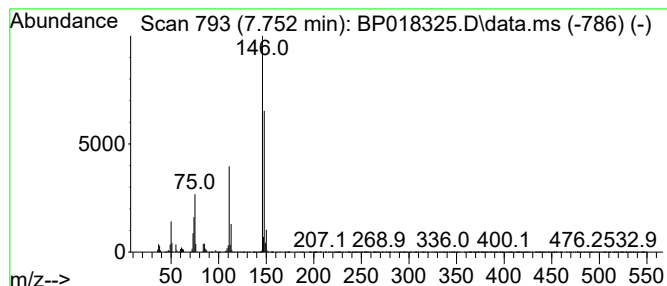

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018325.D
Acq On : 24 Nov 2023 13:32
Operator : MA/JU
Sample : 05261-03DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKV4DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1,2-dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.216	33.66 ng/ul	3737950	1,4-Dichlorobenzene-d4	7.864

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	98
2			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	98
3			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97
4			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97
5			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97

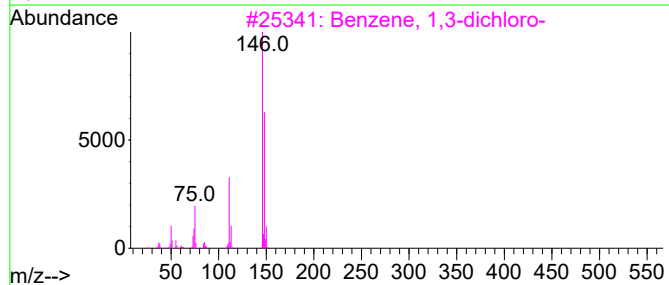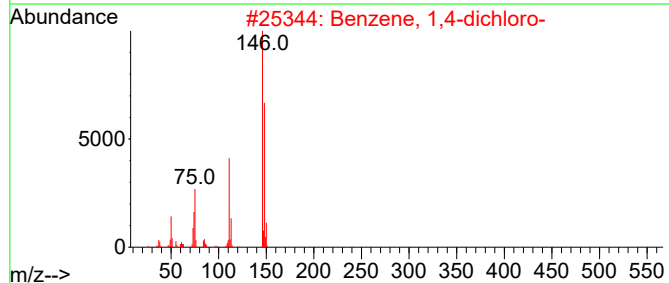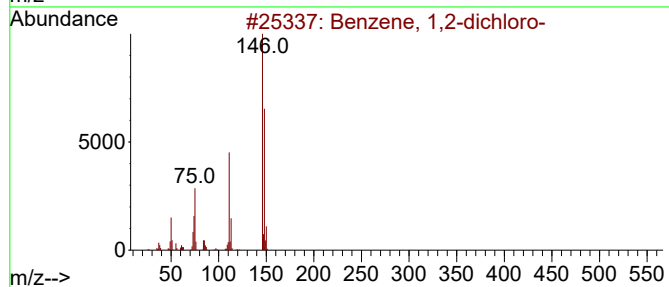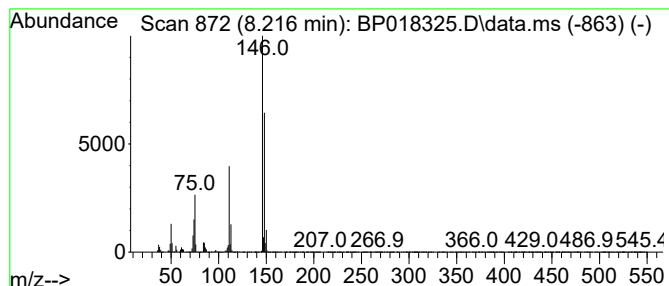

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018325.D
Acq On : 24 Nov 2023 13:32
Operator : MA/JU
Sample : 05261-03DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKV4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,4-di...	7.752	12.3	ng/ul	1370300	1	7.864	2220690	20.0
Benzene, 1,2-di...	8.216	33.7	ng/ul	3737950	1	7.864	2220690	20.0