

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018327.D
 Acq On : 24 Nov 2023 15:02
 Operator : MA/JU
 Sample : 05268-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018327.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rVB	74265	88505	0.93%	0.121%
2	3.693	99	103	113	rBV	224599	316704	3.34%	0.433%
3	3.934	141	144	150	rVB5	20833	35169	0.37%	0.048%
4	4.034	157	161	168	rVB3	22069	34795	0.37%	0.048%
5	7.028	664	670	677	rVB	261820	407309	4.30%	0.557%
6	7.204	693	700	711	rVB	1178648	1788026	18.87%	2.447%
7	7.399	726	733	742	rBV	1019729	1619265	17.09%	2.216%
8	7.499	747	750	755	rVB7	7766	12484	0.13%	0.017%
9	7.869	805	813	820	rVB	1229607	1893821	19.99%	2.592%
10	8.293	882	885	894	rVB2	7748	16177	0.17%	0.022%
11	8.575	926	933	941	rBV	754267	1180312	12.46%	1.615%
12	9.028	1001	1010	1019	rBV	1229849	1968548	20.78%	2.694%
13	9.469	1082	1085	1092	rVB6	14609	25250	0.27%	0.035%
14	9.751	1121	1133	1145	rBV	761294	1248662	13.18%	1.709%
15	10.287	1216	1224	1235	rBV	1333512	2249035	23.74%	3.078%
16	10.669	1275	1289	1298	rVB	1513868	2518976	26.59%	3.448%
17	10.804	1305	1312	1322	rBV	1165972	1923493	20.30%	2.633%
18	11.475	1423	1426	1432	rVB8	5924	11396	0.12%	0.016%
19	11.963	1505	1509	1515	rVB5	11731	21335	0.23%	0.029%
20	12.257	1554	1559	1565	rVB2	29041	49086	0.52%	0.067%
21	12.892	1661	1667	1672	rBV8	8431	20871	0.22%	0.029%
22	13.345	1740	1744	1749	rVB6	10212	14712	0.16%	0.020%
23	13.416	1749	1756	1761	rVB4	20234	31791	0.34%	0.044%
24	13.916	1835	1841	1853	rBV	2695560	3525102	37.21%	4.825%
25	14.192	1880	1888	1900	rBV	2979466	4388320	46.32%	6.006%
26	14.498	1930	1940	1950	rBV	2003796	2977514	31.43%	4.075%
27	14.681	1966	1971	1979	rBV	160640	263647	2.78%	0.361%
28	14.922	2007	2012	2014	rVV6	8744	12831	0.14%	0.018%
29	15.322	2074	2080	2086	rBV6	10038	20416	0.22%	0.028%
30	15.492	2102	2109	2122	rBV	4097673	5656521	59.71%	7.742%
31	15.604	2122	2128	2144	rVV	698664	1002950	10.59%	1.373%
32	15.733	2144	2150	2156	rVB3	19293	36131	0.38%	0.049%
33	16.057	2202	2205	2212	rVB9	5580	10135	0.11%	0.014%
34	16.927	2350	2353	2357	rVB6	7218	10127	0.11%	0.014%
35	17.033	2368	2371	2376	rBV6	7172	12605	0.13%	0.017%
36	17.133	2384	2388	2395	rVB7	12588	19168	0.20%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018327.D
 Acq On : 24 Nov 2023 15:02
 Operator : MA/JU
 Sample : 05268-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.251	2401	2408	2418	rBV	2471083	3466012	36.59%	4.744%
38	17.351	2418	2425	2438	rBV	4694706	6585596	69.52%	9.014%
39	18.145	2556	2560	2571	rBV	90999	153148	1.62%	0.210%
40	18.222	2571	2573	2579	rVB5	8638	11285	0.12%	0.015%
41	19.163	2729	2733	2738	rVB	60403	84728	0.89%	0.116%
42	19.233	2741	2745	2748	rBV	60864	81239	0.86%	0.111%
43	19.386	2767	2771	2776	rBV3	75951	99142	1.05%	0.136%
44	19.592	2800	2806	2812	rBV	6237557	8288630	87.50%	11.345%
45	20.592	2972	2976	2981	rBV	74878	86648	0.91%	0.119%
46	21.357	3100	3106	3112	rBV	3429007	4322225	45.63%	5.916%
47	23.627	3484	3492	3506	rBV2	4651049	9473148	100.00%	12.966%
48	23.786	3511	3519	3535	rVB	2378508	4999180	52.77%	6.842%




Sum of corrected areas: 73062170

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018327.D
Acq On : 24 Nov 2023 15:02
Operator : MA/JU
Sample : 05268-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

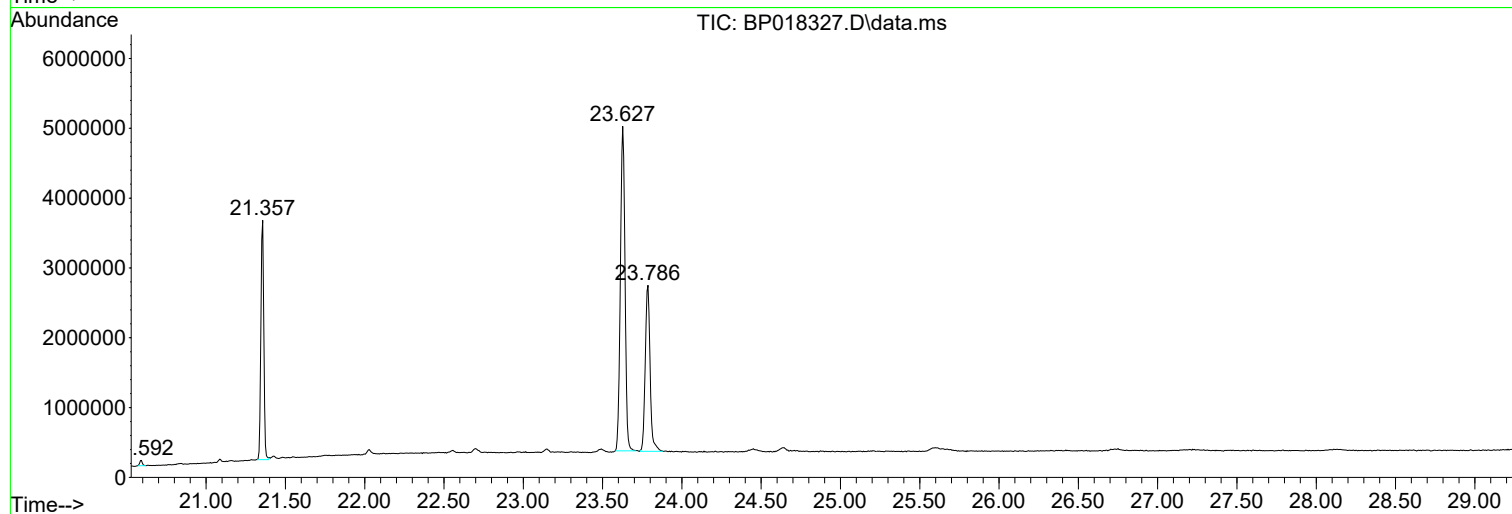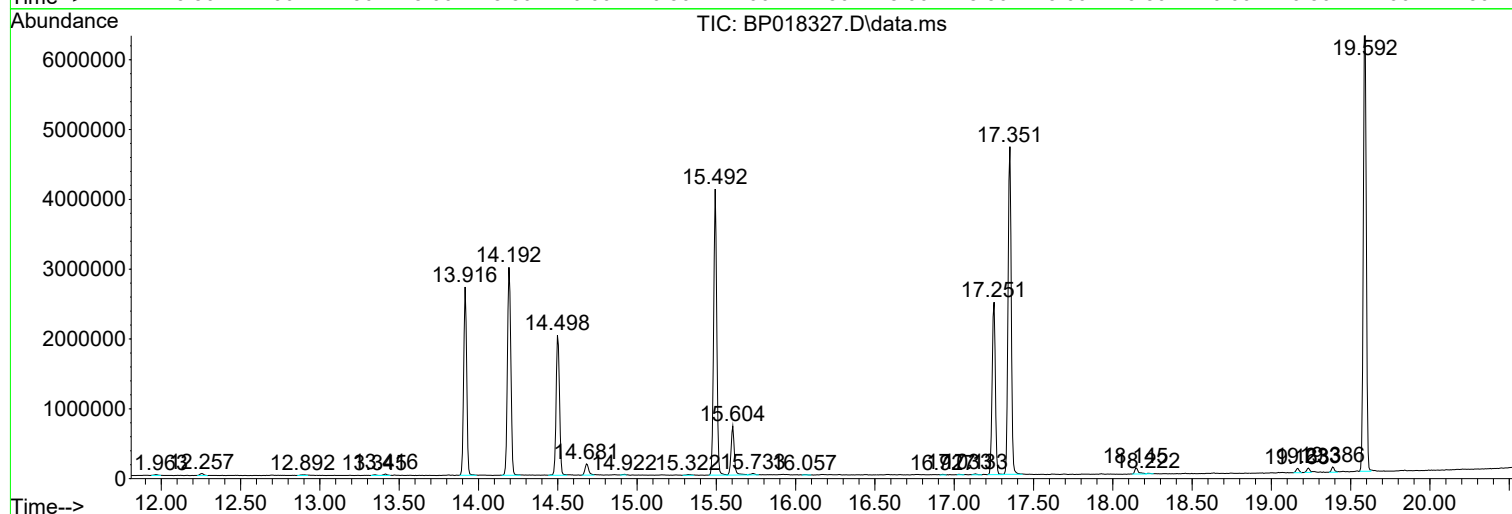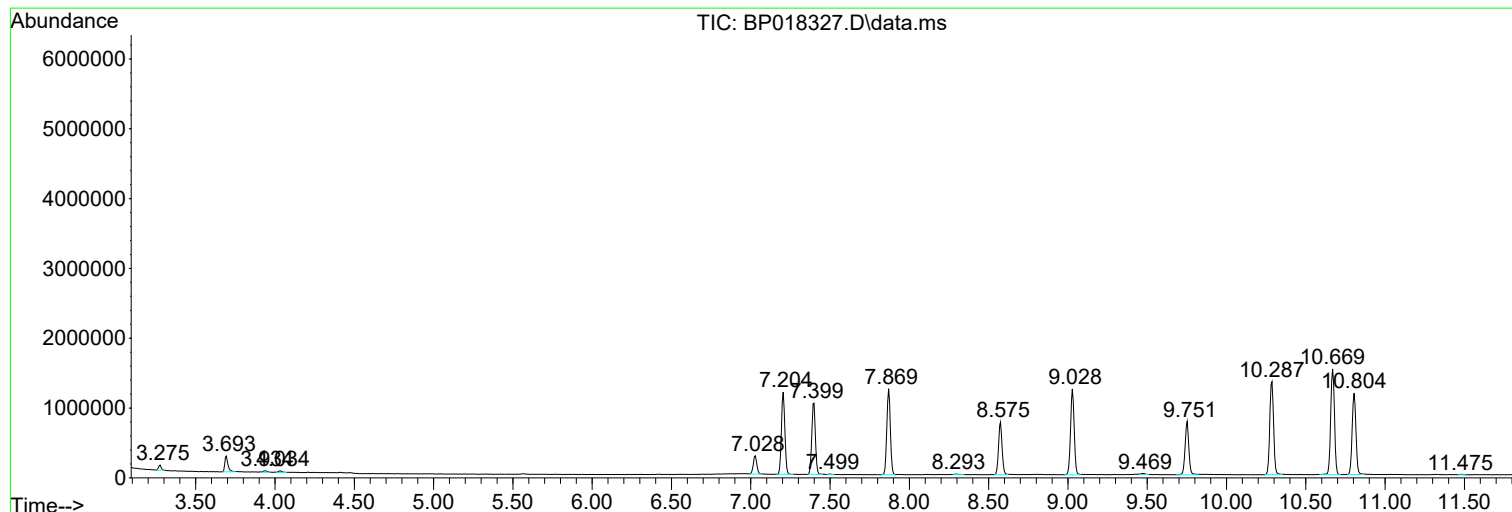

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018327.D
Acq On : 24 Nov 2023 15:02
Operator : MA/JU
Sample : 05268-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018327.D
Acq On : 24 Nov 2023 15:02
Operator : MA/JU
Sample : 05268-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc