

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018331.D
 Acq On : 24 Nov 2023 17:18
 Operator : MA/JU
 Sample : PB157189BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	40	rVB	117340	153708	2.16%	0.181%
2	3.687	98	102	116	rBV	1483868	2050847	28.79%	2.416%
3	4.028	157	160	167	rVB	22107	29519	0.41%	0.035%
4	5.564	418	421	425	rBV6	5662	7535	0.11%	0.009%
5	6.981	658	662	663	rBV4	5359	7845	0.11%	0.009%
6	7.028	663	670	687	rVB	1630793	2467346	34.64%	2.906%
7	7.205	694	700	712	rVB	1383464	2085038	29.27%	2.456%
8	7.399	725	733	747	rBV	1611565	2525057	35.45%	2.974%
9	7.869	805	813	822	rBV	1427275	2183659	30.66%	2.572%
10	8.575	926	933	942	rBV	2033712	3146673	44.18%	3.707%
11	8.869	980	983	990	rVB8	5772	12818	0.18%	0.015%
12	9.028	1002	1010	1021	rBV	1470426	2393019	33.60%	2.819%
13	9.752	1125	1133	1144	rBV	1053523	1660749	23.32%	1.956%
14	10.287	1216	1224	1235	rBV	1956809	3184666	44.71%	3.751%
15	10.669	1279	1289	1300	rVB	1894438	3183376	44.69%	3.750%
16	10.804	1304	1312	1320	rBV	2070690	3400390	47.74%	4.006%
17	11.322	1396	1400	1403	rBV5	5846	9044	0.13%	0.011%
18	11.963	1506	1509	1515	rVB8	5111	8013	0.11%	0.009%
19	12.257	1551	1559	1565	rBV2	38895	67412	0.95%	0.079%
20	12.698	1629	1634	1639	rVV7	6101	12293	0.17%	0.014%
21	12.898	1661	1668	1671	rBV9	7815	16821	0.24%	0.020%
22	13.093	1696	1701	1702	rBV4	6105	7311	0.10%	0.009%
23	13.410	1751	1755	1762	rVB3	24983	39816	0.56%	0.047%
24	13.475	1762	1766	1771	rBV4	5875	11508	0.16%	0.014%
25	13.816	1821	1824	1829	rVB7	7977	11065	0.16%	0.013%
26	13.916	1835	1841	1852	rBV	3477485	4803874	67.44%	5.659%
27	14.192	1881	1888	1896	rBV	4025896	5972799	83.86%	7.036%
28	14.504	1933	1941	1948	rBV	2893789	4261191	59.83%	5.019%
29	14.687	1965	1972	1991	rBV	1101693	1604005	22.52%	1.889%
30	14.916	2006	2011	2016	rVB9	10560	21752	0.31%	0.026%
31	15.151	2047	2051	2055	rBV6	5841	9580	0.13%	0.011%
32	15.328	2075	2081	2085	rBV8	8471	14404	0.20%	0.017%
33	15.492	2102	2109	2117	rBV	5055299	7122689	100.00%	8.390%
34	15.604	2122	2128	2141	rVV	742353	1044787	14.67%	1.231%
35	15.734	2145	2150	2157	rVB3	24882	45601	0.64%	0.054%
36	15.945	2183	2186	2188	rVB4	8042	8288	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018331.D
 Acq On : 24 Nov 2023 17:18
 Operator : MA/JU
 Sample : PB157189BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.275	2239	2242	2246	rBV6	6893	11537	0.16%	0.014%
38	16.586	2291	2295	2299	rVB7	6005	7853	0.11%	0.009%
39	16.757	2321	2324	2329	rBV7	6284	9916	0.14%	0.012%
40	16.928	2349	2353	2356	rVB6	5453	8661	0.12%	0.010%
41	17.133	2383	2388	2392	rBV7	10423	17906	0.25%	0.021%
42	17.251	2401	2408	2414	rBV	3132088	4349666	61.07%	5.124%
43	17.351	2418	2425	2436	rVV	4743281	6680748	93.80%	7.870%
44	18.145	2556	2560	2569	rBV8	32635	62491	0.88%	0.074%
45	19.163	2729	2733	2740	rVB2	52818	73835	1.04%	0.087%
46	19.233	2740	2745	2750	rBV	52403	81702	1.15%	0.096%
47	19.386	2768	2771	2775	rBV3	26490	34462	0.48%	0.041%
48	19.539	2793	2797	2799	rBV4	21288	29437	0.41%	0.035%
49	19.586	2799	2805	2819	rVV	5213275	6466481	90.79%	7.617%
50	20.586	2972	2975	2978	rVB2	63443	71844	1.01%	0.085%
51	21.351	3100	3105	3111	rBV	2714165	3397414	47.70%	4.002%
52	23.621	3484	3491	3507	rVB2	3073671	6084390	85.42%	7.167%
53	23.780	3511	3518	3534	rVB	1830132	3920099	55.04%	4.618%




Sum of corrected areas: 84892940

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018331.D
Acq On : 24 Nov 2023 17:18
Operator : MA/JU
Sample : PB157189BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK189

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

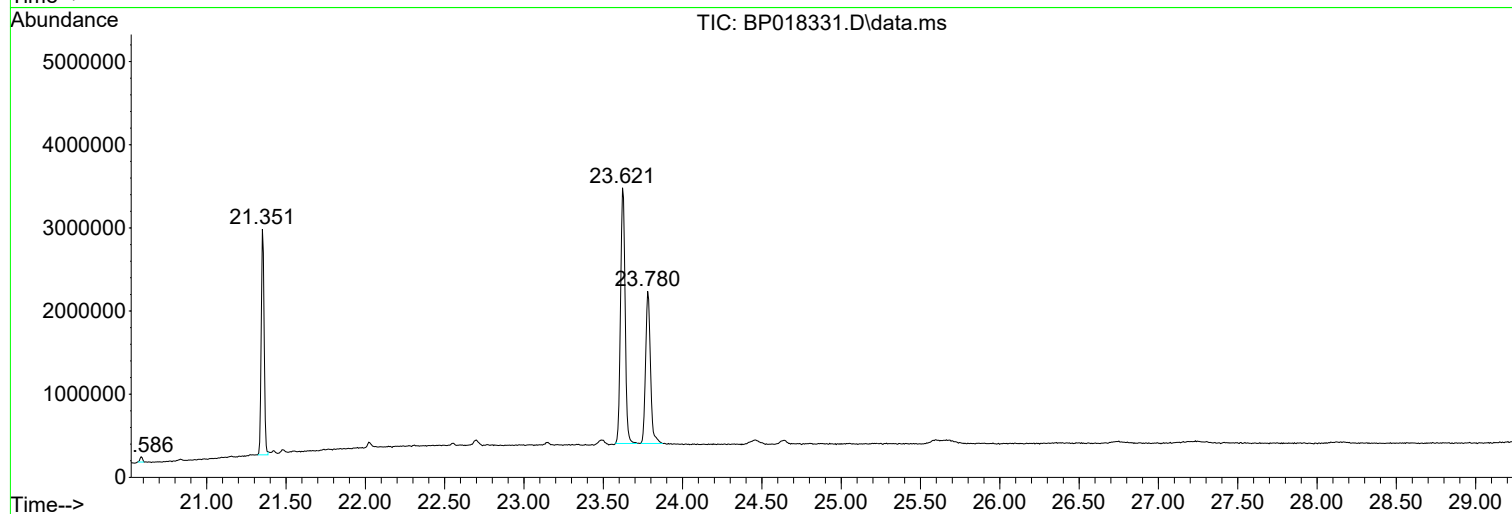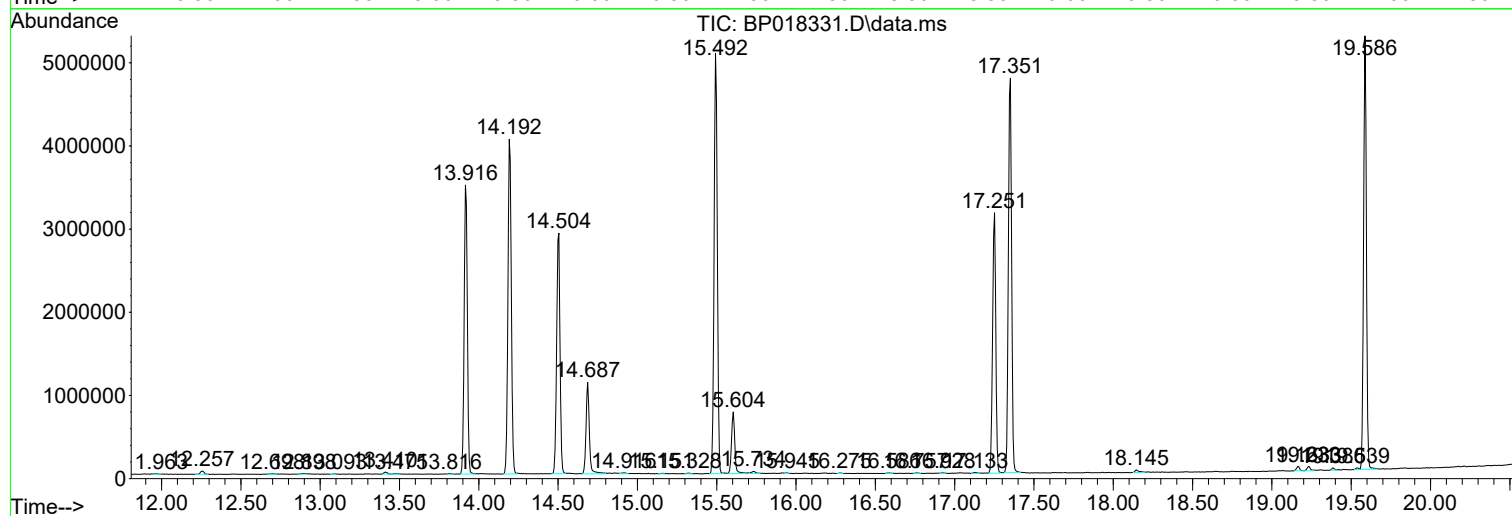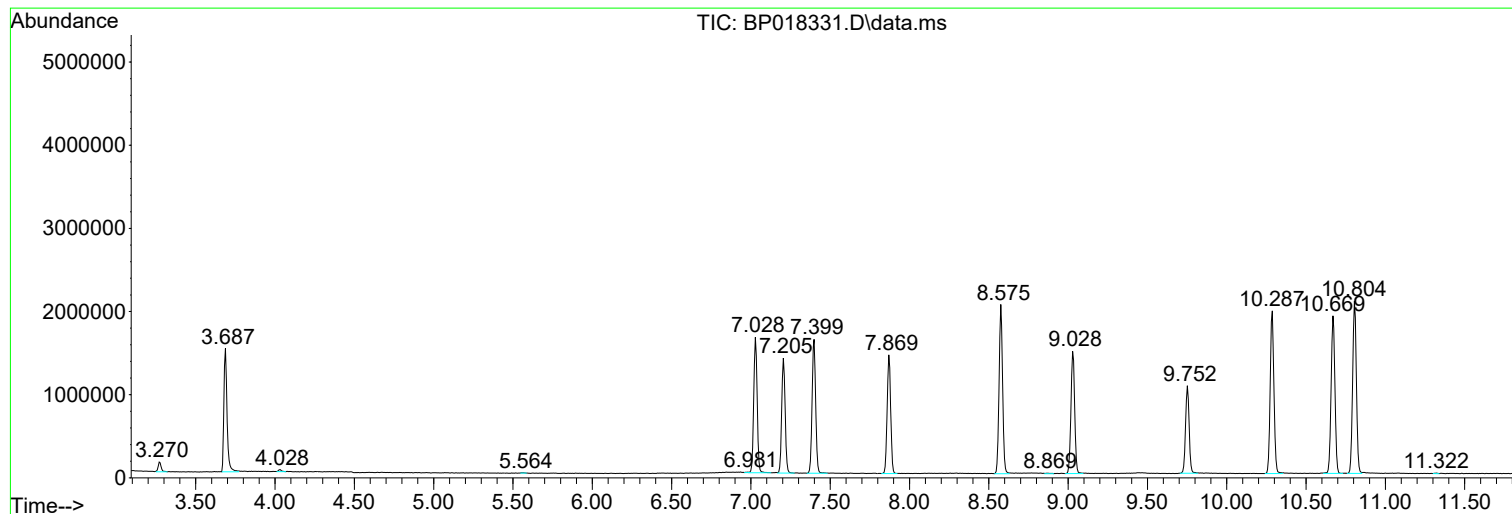

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018331.D
Acq On : 24 Nov 2023 17:18
Operator : MA/JU
Sample : PB157189BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK189

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018331.D
Acq On : 24 Nov 2023 17:18
Operator : MA/JU
Sample : PB157189BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK189

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------