

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018334.D
 Acq On : 24 Nov 2023 19:00
 Operator : MA/JU
 Sample : 05264-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rVB	76031	86617	1.29%	0.132%
2	3.687	99	102	115	rBV	249759	361410	5.40%	0.549%
3	3.934	140	144	149	rVB2	19393	28594	0.43%	0.043%
4	4.028	156	160	166	rBV3	21330	34952	0.52%	0.053%
5	7.028	663	670	679	rVB	347582	533313	7.97%	0.810%
6	7.205	693	700	711	rVB	1209256	1872706	27.97%	2.844%
7	7.399	726	733	742	rBV	1114304	1761052	26.30%	2.675%
8	7.505	748	751	756	rBV7	5378	8330	0.12%	0.013%
9	7.869	805	813	821	rBV	1188686	1812977	27.08%	2.754%
10	8.352	890	895	900	rVB9	3600	7856	0.12%	0.012%
11	8.575	924	933	941	rBV	939005	1459770	21.80%	2.217%
12	9.028	1002	1010	1020	rBV	1299810	2070763	30.93%	3.145%
13	9.463	1074	1084	1091	rVB4	34205	73598	1.10%	0.112%
14	9.752	1123	1133	1145	rBV	821202	1319918	19.71%	2.005%
15	9.975	1166	1171	1179	rVB5	20465	33207	0.50%	0.050%
16	10.287	1216	1224	1238	rBV	1522396	2502582	37.38%	3.801%
17	10.669	1281	1289	1296	rVB	1528197	2505435	37.42%	3.805%
18	10.805	1302	1312	1321	rBV	1448064	2399442	35.84%	3.644%
19	11.457	1418	1423	1426	rBV6	8248	12208	0.18%	0.019%
20	11.599	1444	1447	1455	rVB9	8844	17679	0.26%	0.027%
21	11.963	1502	1509	1515	rBV4	24763	55026	0.82%	0.084%
22	12.257	1551	1559	1564	rBV2	33656	59912	0.89%	0.091%
23	12.693	1631	1633	1637	rVB4	6022	8060	0.12%	0.012%
24	12.887	1663	1666	1670	rBV6	6789	10891	0.16%	0.017%
25	13.128	1702	1707	1710	rVB6	4499	7050	0.11%	0.011%
26	13.410	1750	1755	1761	rBV2	26510	41900	0.63%	0.064%
27	13.475	1762	1766	1771	rVB8	6874	10067	0.15%	0.015%
28	13.775	1812	1817	1819	rBV6	4888	9482	0.14%	0.014%
29	13.810	1819	1823	1827	rVV7	3945	7427	0.11%	0.011%
30	13.916	1834	1841	1853	rBV	2973051	4031928	60.22%	6.124%
31	14.193	1881	1888	1899	rBV	3381751	4858354	72.57%	7.379%
32	14.498	1931	1940	1947	rBV	2112741	3024220	45.17%	4.593%
33	14.681	1965	1971	1983	rBV	152937	249555	3.73%	0.379%
34	14.916	2006	2011	2018	rVB7	13759	23772	0.36%	0.036%
35	15.310	2074	2078	2085	rBV2	17619	30303	0.45%	0.046%
36	15.493	2103	2109	2118	rBV	4210267	5918314	88.40%	8.989%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018334.D
 Acq On : 24 Nov 2023 19:00
 Operator : MA/JU
 Sample : 05264-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.604	2122	2128	2142	rVV	509063	773657	11.56%	1.175%
38	15.734	2146	2150	2158	rVB4	21110	36728	0.55%	0.056%
39	15.910	2174	2180	2181	rBV5	6084	8286	0.12%	0.013%
40	16.757	2321	2324	2328	rBV4	7253	6964	0.10%	0.011%
41	16.928	2349	2353	2356	rBV5	6974	9490	0.14%	0.014%
42	17.128	2384	2387	2392	rVB6	9675	13902	0.21%	0.021%
43	17.245	2401	2407	2414	rBV	2009205	2866425	42.81%	4.353%
44	17.345	2418	2424	2435	rBV	4272891	5982119	89.35%	9.086%
45	17.681	2479	2481	2487	rVB6	5514	7154	0.11%	0.011%
46	17.845	2504	2509	2511	rBV6	6359	10025	0.15%	0.015%
47	18.145	2555	2560	2564	rBV4	35894	54521	0.81%	0.083%
48	19.163	2729	2733	2740	rVB2	51114	62292	0.93%	0.095%
49	19.228	2740	2744	2748	rBV2	47666	68211	1.02%	0.104%
50	19.386	2768	2771	2775	rBV5	27715	35078	0.52%	0.053%
51	19.528	2793	2795	2799	rBV5	10392	13674	0.20%	0.021%
52	19.586	2799	2805	2815	rVV	4778566	6197611	92.57%	9.413%
53	21.351	3100	3105	3115	rBV	2112422	2663049	39.78%	4.045%
54	23.622	3484	3491	3503	rBV2	3451864	6695095	100.00%	10.168%
55	23.780	3511	3518	3535	rVB	1482680	3089068	46.14%	4.692%




Sum of corrected areas: 65842019

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018334.D
Acq On : 24 Nov 2023 19:00
Operator : MA/JU
Sample : 05264-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKP8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

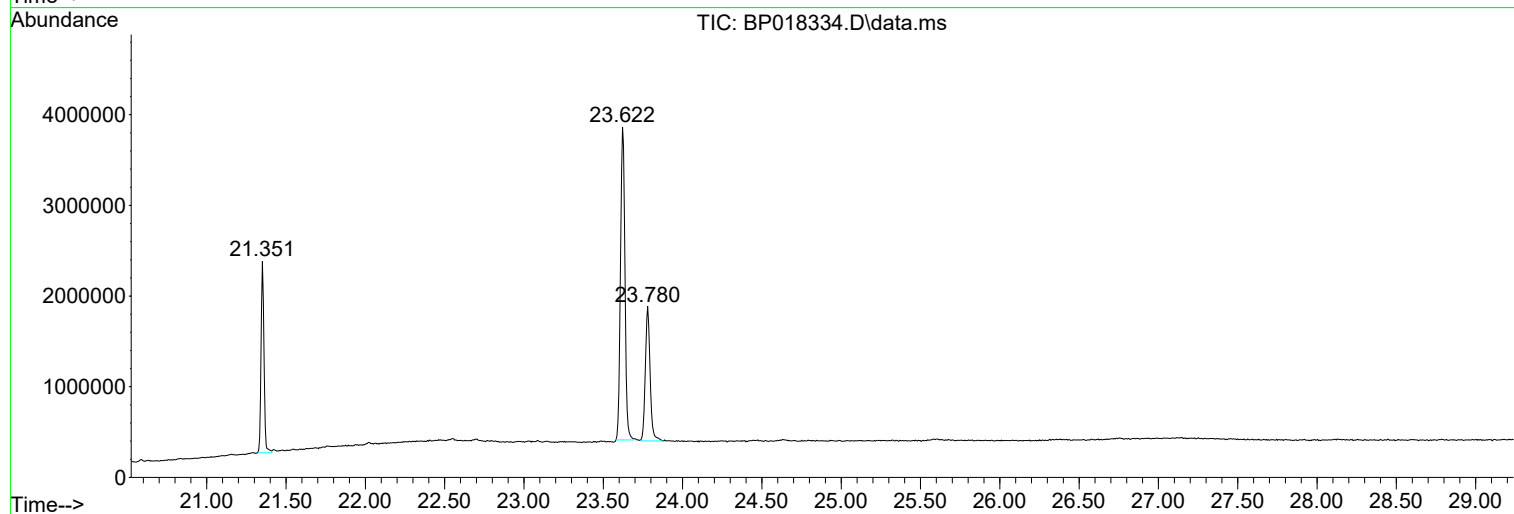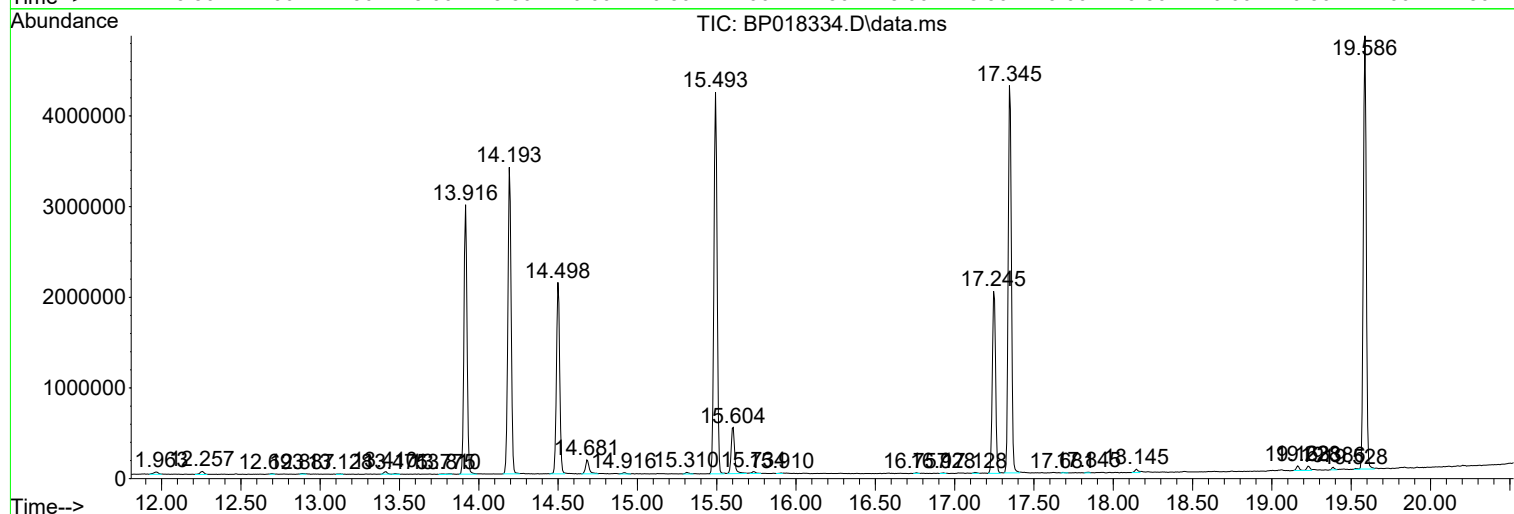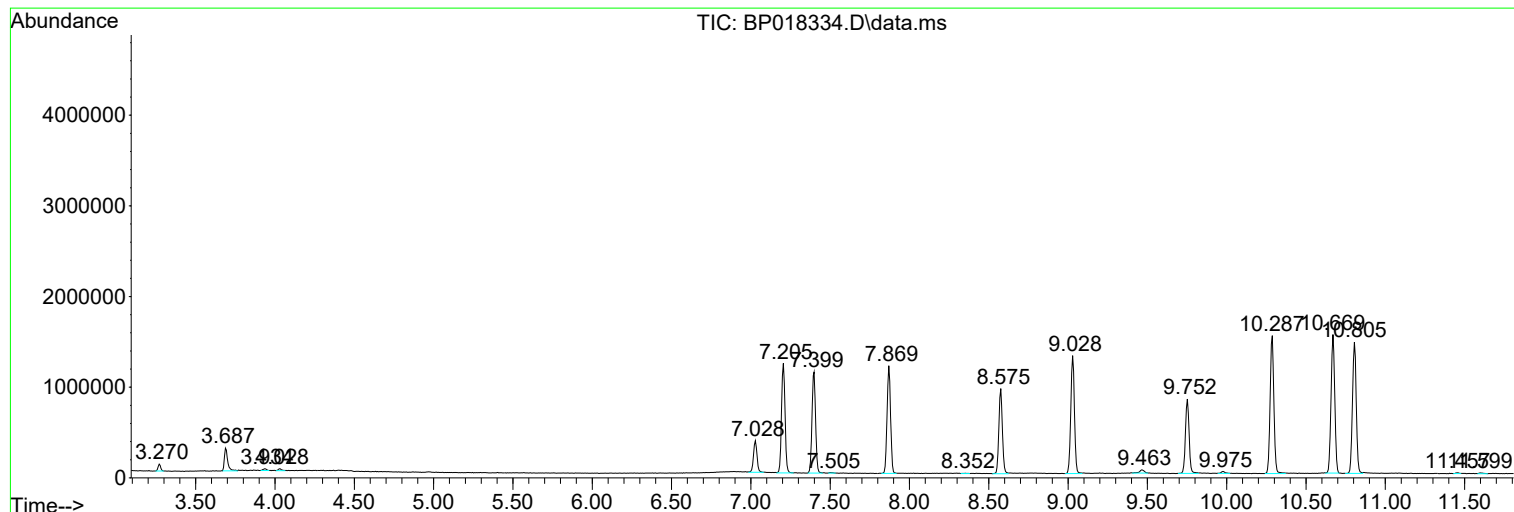

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018334.D
Acq On : 24 Nov 2023 19:00
Operator : MA/JU
Sample : 05264-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKP8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018334.D
Acq On : 24 Nov 2023 19:00
Operator : MA/JU
Sample : 05264-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKP8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc