

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018336.D
 Acq On : 24 Nov 2023 20:08
 Operator : MA/JU
 Sample : 05336-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	38	rVB	84399	108310	1.22%	0.136%
2	3.687	98	102	113	rBV	498717	695237	7.86%	0.871%
3	3.940	141	145	149	rVB2	21467	31867	0.36%	0.040%
4	4.028	157	160	165	rVB2	20431	28081	0.32%	0.035%
5	4.964	316	319	323	rVB6	7641	11665	0.13%	0.015%
6	5.405	389	394	398	rBV7	6044	12764	0.14%	0.016%
7	6.875	634	644	651	rBV4	47325	167068	1.89%	0.209%
8	7.028	664	670	679	rVB	356061	559300	6.32%	0.700%
9	7.205	693	700	708	rVB	1553892	2325152	26.29%	2.912%
10	7.399	725	733	742	rBV	1324354	2108122	23.84%	2.640%
11	7.869	806	813	820	rBV	1341569	2032298	22.98%	2.545%
12	7.940	822	825	832	rVB8	7538	12916	0.15%	0.016%
13	8.216	866	872	878	rVB3	18231	35956	0.41%	0.045%
14	8.575	923	933	944	rBV	1049566	1633897	18.47%	2.046%
15	9.028	1002	1010	1020	rBV	1667593	2628916	29.72%	3.292%
16	9.475	1080	1086	1091	rVB	52860	89015	1.01%	0.111%
17	9.752	1120	1133	1145	rBV	1064660	1728712	19.55%	2.165%
18	10.287	1216	1224	1238	rBV	1885381	3057586	34.57%	3.829%
19	10.669	1282	1289	1297	rVB	1659668	2804133	31.71%	3.512%
20	10.804	1303	1312	1324	rBV	1510644	2508145	28.36%	3.141%
21	11.052	1348	1354	1358	rBV4	12119	21852	0.25%	0.027%
22	11.475	1423	1426	1432	rVB5	14554	25105	0.28%	0.031%
23	11.887	1490	1496	1498	rBV7	6575	12883	0.15%	0.016%
24	11.928	1498	1503	1504	rVV4	9023	15994	0.18%	0.020%
25	11.969	1504	1510	1518	rVB	105987	170187	1.92%	0.213%
26	12.257	1553	1559	1565	rVB2	38309	63534	0.72%	0.080%
27	12.469	1589	1595	1597	rBV7	7166	11664	0.13%	0.015%
28	12.699	1627	1634	1639	rVB7	10356	23994	0.27%	0.030%
29	12.893	1661	1667	1670	rBV8	12428	25725	0.29%	0.032%
30	13.134	1702	1708	1715	rVB7	15486	24394	0.28%	0.031%
31	13.346	1740	1744	1749	rVB8	7680	10952	0.12%	0.014%
32	13.410	1750	1755	1762	rBV2	33312	48527	0.55%	0.061%
33	13.916	1835	1841	1852	rBV	3412534	4676515	52.88%	5.857%
34	14.193	1880	1888	1896	rBV2	4039700	5979148	67.60%	7.488%
35	14.498	1929	1940	1947	rBV	2238502	3327839	37.63%	4.168%
36	14.681	1966	1971	1983	rBV	145195	243128	2.75%	0.304%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018336.D
 Acq On : 24 Nov 2023 20:08
 Operator : MA/JU
 Sample : 05336-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.916	2008	2011	2016	rVB7	12674	18894	0.21%	0.024%
38	15.322	2075	2080	2086	rBV10	8377	16293	0.18%	0.020%
39	15.492	2102	2109	2122	rBV	5105607	7217413	81.60%	9.039%
40	15.604	2122	2128	2140	rVV	705121	1034327	11.69%	1.295%
41	15.734	2146	2150	2156	rVB4	25529	38961	0.44%	0.049%
42	16.098	2209	2212	2218	rBV8	6555	14965	0.17%	0.019%
43	16.257	2234	2239	2247	rVB	30252	55577	0.63%	0.070%
44	16.763	2320	2325	2329	rBV7	11544	22310	0.25%	0.028%
45	16.851	2335	2340	2343	rBV7	12578	18994	0.21%	0.024%
46	16.892	2343	2347	2351	rVV4	23607	34915	0.39%	0.044%
47	17.028	2364	2370	2374	rBV8	8772	15621	0.18%	0.020%
48	17.128	2384	2387	2393	rVB7	17821	22527	0.25%	0.028%
49	17.245	2401	2407	2414	rBV	2244669	3181512	35.97%	3.984%
50	17.345	2418	2424	2442	rVB2	4677520	6761436	76.45%	8.468%
51	18.145	2556	2560	2567	rBV5	68982	100100	1.13%	0.125%
52	19.163	2729	2733	2737	rBV	62173	78529	0.89%	0.098%
53	19.233	2741	2745	2748	rVV	51151	67095	0.76%	0.084%
54	19.386	2767	2771	2777	rBV6	45388	64609	0.73%	0.081%
55	19.586	2799	2805	2811	rBV	5723158	7462265	84.37%	9.345%
56	21.351	3100	3105	3113	rBV	2598653	3367644	38.08%	4.217%
57	23.627	3484	3492	3503	rBV	4508695	8844432	100.00%	11.076%
58	23.780	3511	3518	3538	rVB	1950003	4150558	46.93%	5.198%




Sum of corrected areas: 79849558

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018336.D
Acq On : 24 Nov 2023 20:08
Operator : MA/JU
Sample : 05336-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

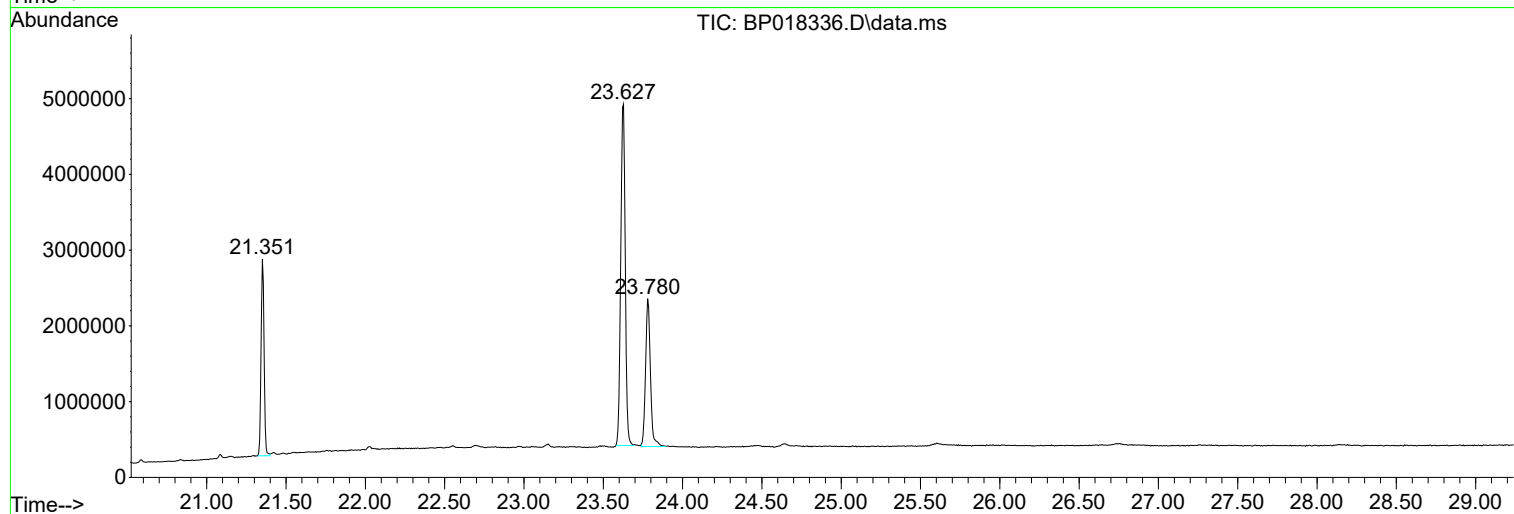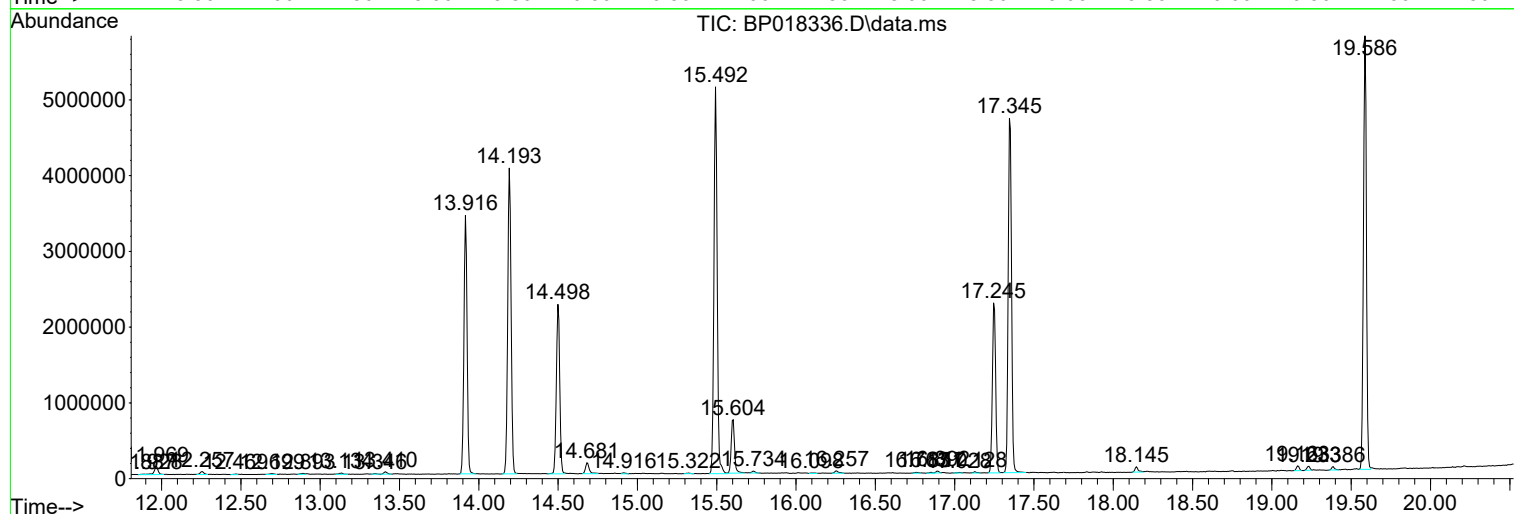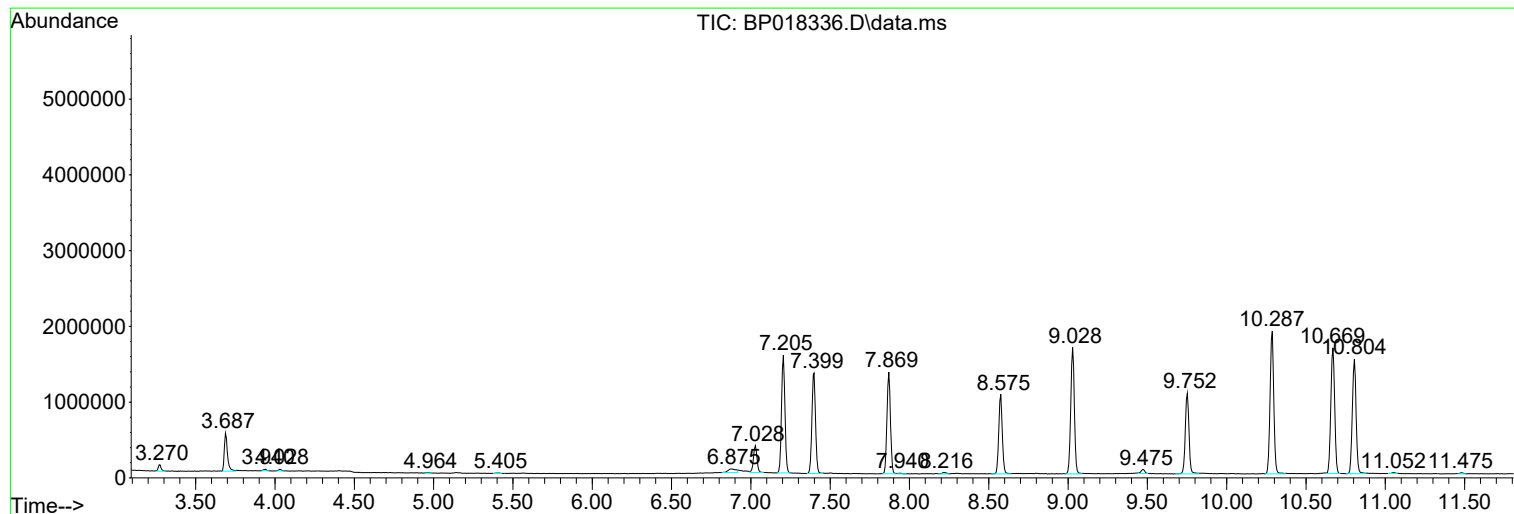

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018336.D
Acq On : 24 Nov 2023 20:08
Operator : MA/JU
Sample : 05336-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018336.D
Acq On : 24 Nov 2023 20:08
Operator : MA/JU
Sample : 05336-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------