

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018337.D
 Acq On : 24 Nov 2023 20:42
 Operator : MA/JU
 Sample : 05336-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	36	rVB	68515	86187	0.82%	0.096%
2	3.693	99	103	112	rBV	281664	405485	3.86%	0.451%
3	4.028	157	160	168	rVB2	24246	33073	0.31%	0.037%
4	4.969	316	320	326	rVB6	13980	21609	0.21%	0.024%
5	5.563	416	421	424	rBV6	8145	14570	0.14%	0.016%
6	7.028	664	670	683	rVB	329524	520099	4.95%	0.578%
7	7.205	693	700	709	rVB	1269129	1923047	18.29%	2.139%
8	7.399	724	733	741	rBV	1162454	1843936	17.54%	2.051%
9	7.499	748	750	758	rVB8	6761	10970	0.10%	0.012%
10	7.869	804	813	828	rBV	1345088	2132262	20.28%	2.371%
11	8.116	850	855	857	rBV6	9490	17202	0.16%	0.019%
12	8.216	869	872	876	rVB2	16404	23954	0.23%	0.027%
13	8.293	881	885	891	rBV5	12443	27523	0.26%	0.031%
14	8.575	925	933	942	rBV	896987	1412481	13.44%	1.571%
15	8.716	951	957	962	rVB	22736	35652	0.34%	0.040%
16	8.975	994	1001	1003	rBV7	12539	20915	0.20%	0.023%
17	9.028	1003	1010	1023	rVB	1369469	2189486	20.83%	2.435%
18	9.469	1076	1085	1097	rVB4	27399	75103	0.71%	0.084%
19	9.751	1126	1133	1148	rBV	871653	1426016	13.56%	1.586%
20	10.069	1183	1187	1194	rVB10	7937	17743	0.17%	0.020%
21	10.287	1216	1224	1232	rBV	1641947	2642524	25.13%	2.939%
22	10.451	1248	1252	1257	rVB8	5815	12532	0.12%	0.014%
23	10.534	1257	1266	1271	rBV	45063	76328	0.73%	0.085%
24	10.616	1271	1280	1281	rBV9	12047	21488	0.20%	0.024%
25	10.669	1282	1289	1297	rVB	1687623	2783192	26.47%	3.095%
26	10.804	1305	1312	1321	rBV	875915	1454116	13.83%	1.617%
27	11.045	1344	1353	1361	rVB6	19401	49405	0.47%	0.055%
28	11.322	1394	1400	1404	rBV6	9952	21886	0.21%	0.024%
29	11.892	1490	1497	1499	rBV8	6708	11017	0.10%	0.012%
30	11.963	1504	1509	1517	rVB2	24890	45357	0.43%	0.050%
31	12.257	1553	1559	1567	rVB2	32864	56561	0.54%	0.063%
32	12.657	1621	1627	1628	rBV5	8343	11857	0.11%	0.013%
33	12.692	1628	1633	1640	rVB2	85445	139050	1.32%	0.155%
34	12.892	1664	1667	1674	rBV8	11503	19689	0.19%	0.022%
35	12.998	1679	1685	1689	rVB8	10774	14956	0.14%	0.017%
36	13.128	1703	1707	1711	rBV6	11706	18464	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018337.D
 Acq On : 24 Nov 2023 20:42
 Operator : MA/JU
 Sample : 05336-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	13.198	1714	1719	1726	rVB5	26711	42833	0.41%	0.048%
38	13.298	1731	1736	1740	rBV3	26186	44058	0.42%	0.049%
39	13.339	1740	1743	1747	rVV5	8425	13066	0.12%	0.015%
40	13.410	1750	1755	1761	rVB3	29197	48294	0.46%	0.054%
41	13.475	1761	1766	1770	rBV7	7328	15921	0.15%	0.018%
42	13.810	1816	1823	1826	rBV9	9339	20943	0.20%	0.023%
43	13.916	1835	1841	1852	rVV	3150278	4238714	40.32%	4.714%
44	14.039	1855	1862	1866	rVB10	14159	28813	0.27%	0.032%
45	14.192	1877	1888	1902	rBV2	3695819	5373735	51.11%	5.976%
46	14.498	1930	1940	1956	rBV	2483604	3620668	34.44%	4.027%
47	14.628	1956	1962	1966	rBV	28377	49015	0.47%	0.055%
48	14.686	1966	1972	1981	rBV	194020	296309	2.82%	0.330%
49	14.816	1989	1994	2002	rBV2	46549	93859	0.89%	0.104%
50	14.898	2002	2008	2016	rVB	623266	897422	8.54%	0.998%
51	15.039	2027	2032	2040	rBV3	66879	104498	0.99%	0.116%
52	15.122	2042	2046	2049	rVB6	12874	16953	0.16%	0.019%
53	15.322	2075	2080	2082	rBV6	13700	18743	0.18%	0.021%
54	15.492	2103	2109	2114	rBV	4887221	6820407	64.87%	7.585%
55	15.545	2114	2118	2123	rVV	319031	545045	5.18%	0.606%
56	15.604	2123	2128	2138	rVB	808449	1203656	11.45%	1.339%
57	15.733	2146	2150	2156	rVB4	20401	34168	0.32%	0.038%
58	15.839	2163	2168	2175	rVB4	29060	46552	0.44%	0.052%
59	15.916	2177	2181	2184	rBV6	10668	15863	0.15%	0.018%
60	15.986	2190	2193	2197	rVB2	17381	21523	0.20%	0.024%
61	16.075	2202	2208	2211	rBV8	9476	22046	0.21%	0.025%
62	16.110	2211	2214	2218	rVB5	10282	13630	0.13%	0.015%
63	16.169	2218	2224	2228	rBV7	14092	28147	0.27%	0.031%
64	16.428	2265	2268	2273	rVB4	12071	14138	0.13%	0.016%
65	16.522	2279	2284	2290	rBV3	18310	32091	0.31%	0.036%
66	16.580	2290	2294	2296	rBV5	9878	14887	0.14%	0.017%
67	16.757	2322	2324	2329	rVB6	12081	19275	0.18%	0.021%
68	16.851	2336	2340	2343	rBV3	13873	23310	0.22%	0.026%
69	16.892	2343	2347	2351	rVV4	47261	68360	0.65%	0.076%
70	17.063	2374	2376	2382	rVB3	13700	17627	0.17%	0.020%
71	17.128	2383	2387	2395	rVB4	24118	37798	0.36%	0.042%
72	17.251	2401	2408	2414	rVV	2992965	4331584	41.20%	4.817%
73	17.345	2418	2424	2435	rBV2	5060609	7577420	72.07%	8.427%
74	17.627	2467	2472	2473	rBV4	11770	18014	0.17%	0.020%
75	17.651	2473	2476	2481	rVB	38648	53380	0.51%	0.059%
76	17.839	2504	2508	2510	rBV5	10724	16576	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018337.D
 Acq On : 24 Nov 2023 20:42
 Operator : MA/JU
 Sample : 05336-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.922	2520	2522	2526	rBV5	7090	11743	0.11%	0.013%
78	18.145	2556	2560	2564	rBV3	89568	133201	1.27%	0.148%
79	18.216	2569	2572	2578	rVB7	17746	32360	0.31%	0.036%
80	18.304	2584	2587	2592	rVB2	24222	34661	0.33%	0.039%
81	18.404	2601	2604	2609	rVB6	16457	27120	0.26%	0.030%
82	18.633	2641	2643	2648	rVB4	22817	26826	0.26%	0.030%
83	19.163	2729	2733	2737	rVB2	78636	101056	0.96%	0.112%
84	19.233	2740	2745	2749	rBV	72918	109501	1.04%	0.122%
85	19.386	2767	2771	2777	rBV2	98763	131350	1.25%	0.146%
86	19.539	2792	2797	2799	rBV5	26427	45155	0.43%	0.050%
87	19.586	2799	2805	2812	rBV	7231835	9648516	91.77%	10.730%
88	20.586	2971	2975	2980	rBV	265565	291884	2.78%	0.325%
89	21.351	3100	3105	3113	rBV	4021276	5185201	49.32%	5.767%
90	21.421	3114	3117	3122	rVB	172477	229680	2.18%	0.255%
91	22.027	3215	3220	3231	rBV	309893	511455	4.86%	0.569%
92	22.704	3330	3335	3344	rVB	344045	683471	6.50%	0.760%
93	23.498	3464	3470	3481	rVB2	305269	815936	7.76%	0.907%
94	23.627	3484	3492	3506	rVV2	5426474	10513359	100.00%	11.692%
95	23.786	3511	3519	3537	rVB	2790547	5871066	55.84%	6.529%




Sum of corrected areas: 89918617

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018337.D
Acq On : 24 Nov 2023 20:42
Operator : MA/JU
Sample : 05336-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

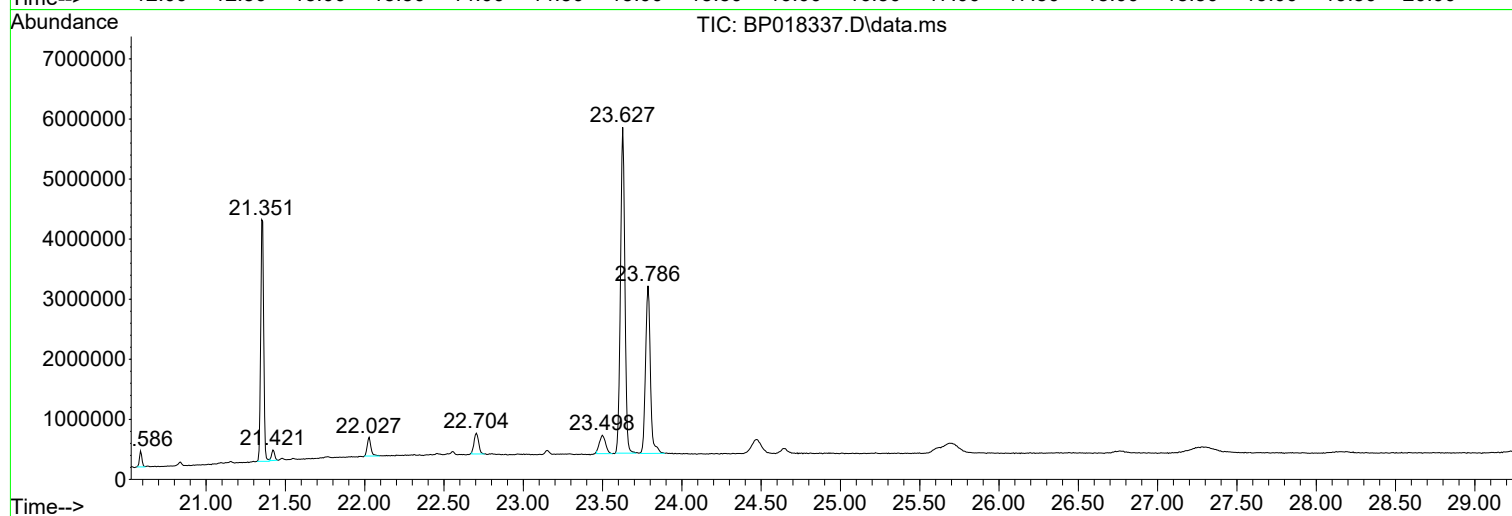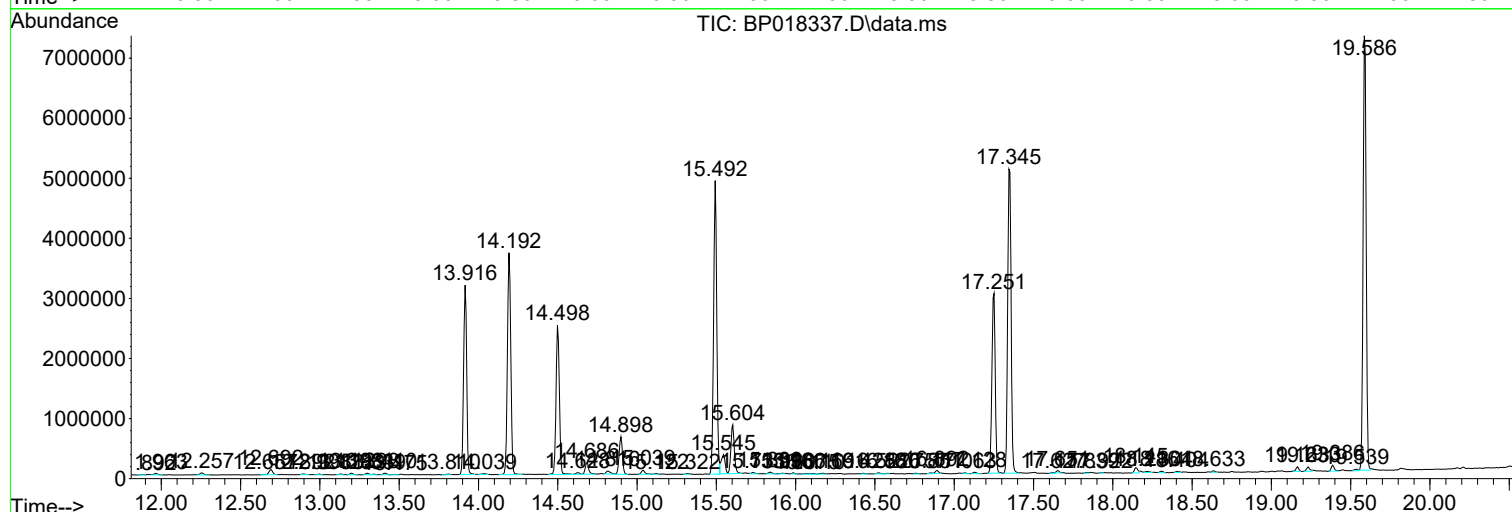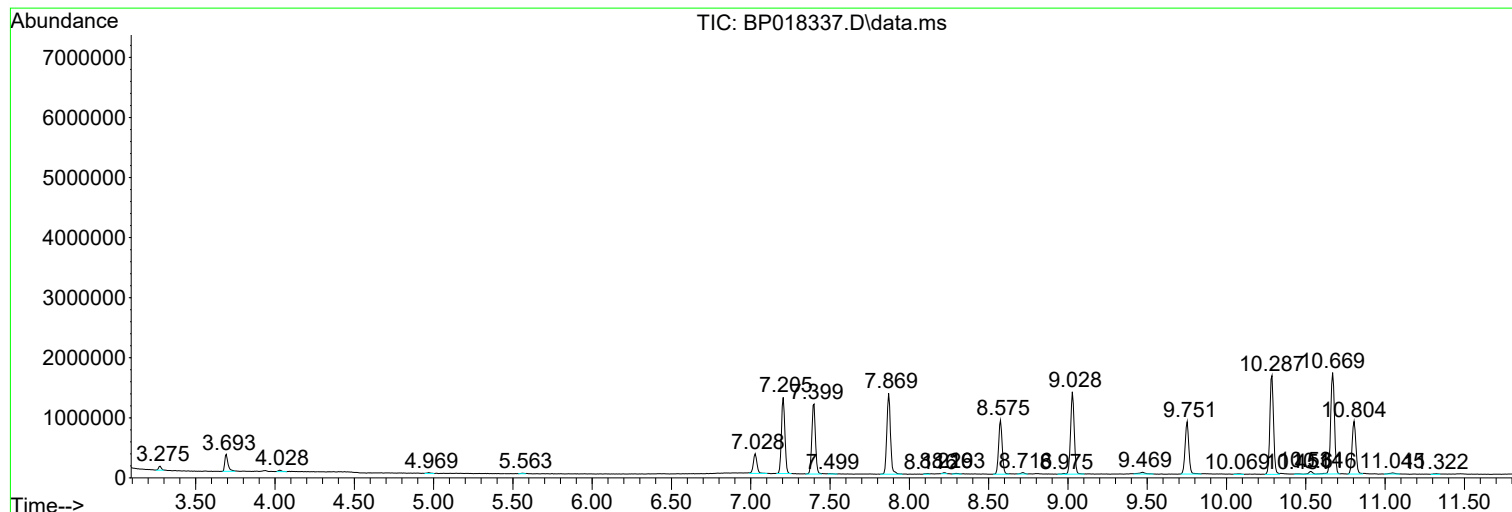

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018337.D
Acq On : 24 Nov 2023 20:42
Operator : MA/JU
Sample : 05336-05
Misc :
ALS Vial : 18 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
DCKC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexasiloxane, tetradecamethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
22.704	2.33 ng/ul	683471	Perylene-d12	23.786	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexasiloxane, tetradecamethyl-	458	C14H42O5Si6	000107-52-8	76
2	Cyclononasiloxane, octadecamethyl-	666	C18H54O9Si9	000556-71-8	72
3	Mercaptoacetic acid, 2TMS deriva...	236	C8H20O2SSi2	006398-62-5	32
4	Cyclodecasiloxane, eicosamethyl-	740	C20H60O10Si10	018772-36-6	27
5	Pentasiloxane, dodecamethyl-	384	C12H36O4Si5	000141-63-9	25

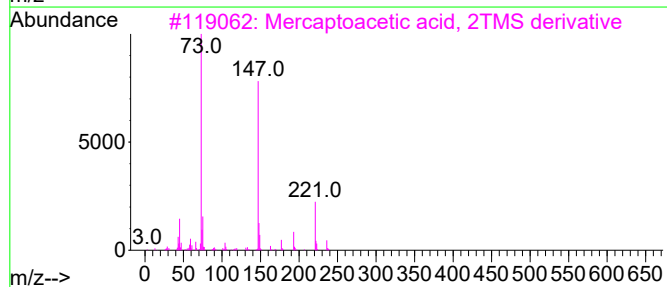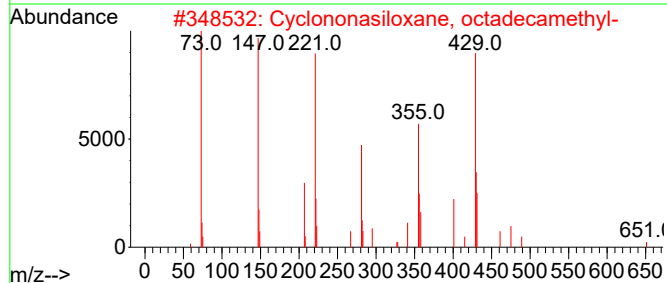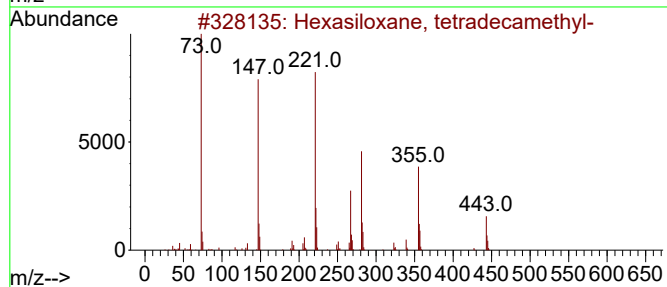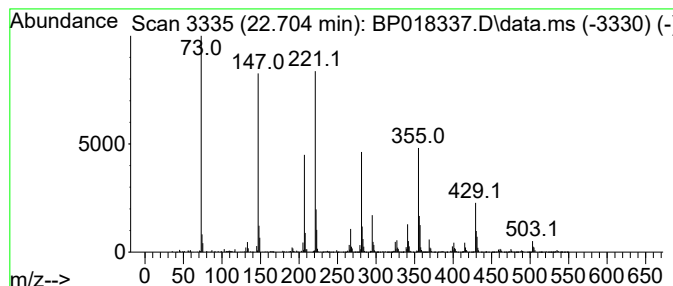

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018337.D
Acq On : 24 Nov 2023 20:42
Operator : MA/JU
Sample : 05336-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.498	2.78 ng/ul	815936	Perylene-d12	23.786

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexasiloxane, tetradecamethyl-	458	C14H42O5Si6	000107-52-8	70
2			3,6-Dioxa-2,4,5,7-tetrasilaoctan...	294	C10H30O2Si4	004342-25-0	43
3			1,1,1,5,7,7,7-Heptamethyl-3,3-bi...	444	C13H40O5Si6	038147-00-1	42
4			Cyclononasiloxane, octadecamethyl-	666	C18H54O9Si9	000556-71-8	40
5			Heptasiloxane, hexadecamethyl-	532	C16H48O6Si7	000541-01-5	16

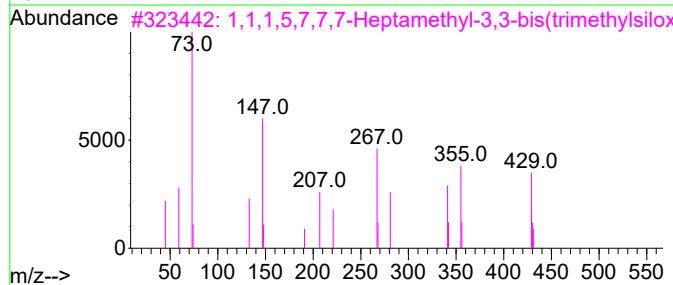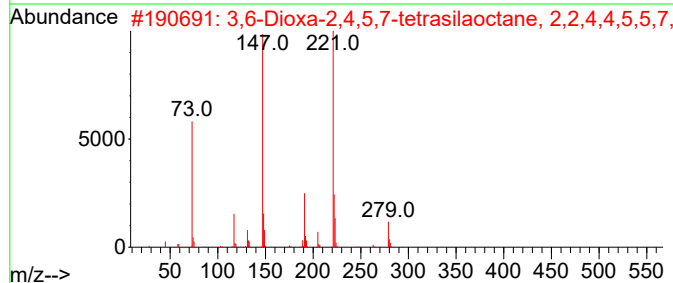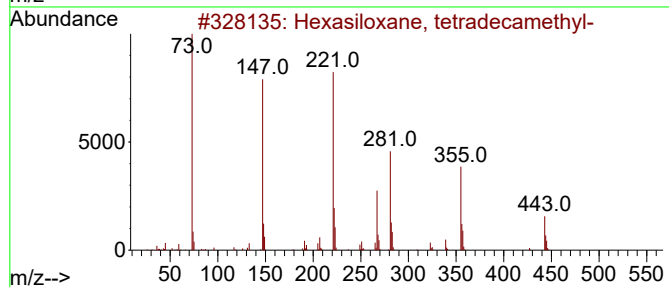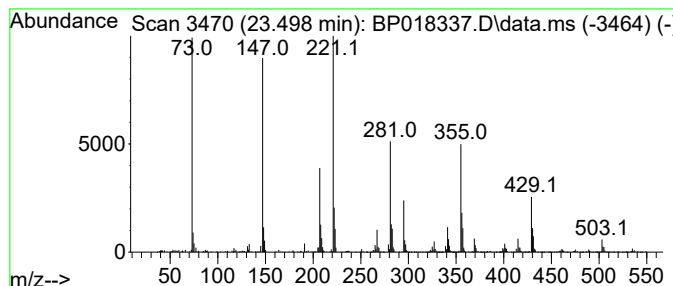

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018337.D
Acq On : 24 Nov 2023 20:42
Operator : MA/JU
Sample : 05336-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexasiloxane, t...	22.704	2.3	ng/ul	683471	6	23.786	5871070	20.0
unknown-01	23.498	2.8	ng/ul	815936	6	23.786	5871070	20.0