

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018338.D
 Acq On : 24 Nov 2023 21:16
 Operator : MA/JU
 Sample : 05336-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rVB	82177	108917	1.57%	0.144%
2	3.687	98	102	112	rBV	728404	1010694	14.61%	1.336%
3	3.934	141	144	152	rVB2	24802	42211	0.61%	0.056%
4	4.028	157	160	165	rVB	20940	30796	0.45%	0.041%
5	5.140	345	349	353	rBV4	12611	19677	0.28%	0.026%
6	7.028	664	670	676	rVB	262286	404267	5.84%	0.534%
7	7.205	693	700	710	rVB	1183206	1833623	26.51%	2.423%
8	7.393	726	732	746	rBV	988909	1568503	22.67%	2.073%
9	7.505	747	751	755	rVB7	7018	10523	0.15%	0.014%
10	7.681	776	781	786	rVB9	3526	8619	0.12%	0.011%
11	7.869	805	813	823	rBV	1463586	2258230	32.65%	2.985%
12	7.940	823	825	830	rVB6	6413	8907	0.13%	0.012%
13	8.222	864	873	877	rBV3	19312	37637	0.54%	0.050%
14	8.575	926	933	944	rVV	802943	1283995	18.56%	1.697%
15	8.716	953	957	962	rVB7	10660	14708	0.21%	0.019%
16	9.028	1003	1010	1021	rVB	1263732	2013619	29.11%	2.661%
17	9.416	1073	1076	1077	rBV3	5989	7268	0.11%	0.010%
18	9.469	1082	1085	1092	rVB6	16908	33655	0.49%	0.044%
19	9.752	1123	1133	1143	rBV	738324	1228099	17.75%	1.623%
20	10.287	1216	1224	1233	rBV	1408374	2373346	34.31%	3.137%
21	10.528	1262	1265	1269	rVB6	7714	10692	0.15%	0.014%
22	10.610	1272	1279	1282	rVV9	7927	18313	0.26%	0.024%
23	10.669	1282	1289	1298	rVB	1985739	3295275	47.64%	4.355%
24	10.804	1305	1312	1327	rBV	2095253	3414662	49.36%	4.513%
25	11.051	1351	1354	1357	rVB4	8989	10183	0.15%	0.013%
26	11.481	1420	1427	1432	rVB5	18973	35166	0.51%	0.046%
27	11.963	1502	1509	1520	rVB5	19600	47649	0.69%	0.063%
28	12.251	1552	1558	1567	rVB3	31679	60224	0.87%	0.080%
29	12.687	1627	1632	1633	rVV4	8996	13002	0.19%	0.017%
30	12.698	1633	1634	1637	rVB3	11171	8211	0.12%	0.011%
31	12.887	1659	1666	1671	rBV9	11401	24365	0.35%	0.032%
32	13.293	1731	1735	1740	rBV8	9030	15436	0.22%	0.020%
33	13.345	1740	1744	1746	rVV5	7590	9106	0.13%	0.012%
34	13.410	1749	1755	1761	rVV2	41106	67185	0.97%	0.089%
35	13.475	1764	1766	1771	rVB6	7006	9063	0.13%	0.012%
36	13.816	1820	1824	1828	rBV6	5585	8179	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018338.D
 Acq On : 24 Nov 2023 21:16
 Operator : MA/JU
 Sample : 05336-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	13.916	1835	1841	1847	rBV	3363565	4573347	66.11%	6.044%
38	14.192	1878	1888	1899	rBV	3677753	5335332	77.13%	7.051%
39	14.498	1930	1940	1949	rBV	3028009	4512320	65.23%	5.964%
40	14.628	1958	1962	1966	rVB2	11644	17544	0.25%	0.023%
41	14.681	1966	1971	1978	rBV	114000	174321	2.52%	0.230%
42	14.810	1989	1993	1995	rBV5	9580	13687	0.20%	0.018%
43	14.898	2004	2008	2016	rVB	21832	43848	0.63%	0.058%
44	15.322	2075	2080	2086	rBV4	16326	28430	0.41%	0.038%
45	15.492	2102	2109	2114	rBV	4875372	6917471	100.00%	9.142%
46	15.528	2114	2115	2122	rVV	373862	349879	5.06%	0.462%
47	15.604	2122	2128	2138	rVV	518771	742682	10.74%	0.982%
48	15.681	2138	2141	2145	rVB5	7263	10395	0.15%	0.014%
49	15.734	2146	2150	2153	rVV2	18079	21026	0.30%	0.028%
50	15.851	2169	2170	2175	rVB5	7630	7658	0.11%	0.010%
51	15.910	2175	2180	2183	rBV7	9382	17771	0.26%	0.023%
52	15.986	2191	2193	2196	rVB4	8291	8574	0.12%	0.011%
53	16.281	2238	2243	2249	rVB10	8040	15644	0.23%	0.021%
54	16.757	2321	2324	2327	rBV5	7592	11307	0.16%	0.015%
55	16.922	2350	2352	2358	rVB7	7917	10659	0.15%	0.014%
56	17.034	2368	2371	2374	rVB4	9386	11753	0.17%	0.016%
57	17.128	2382	2387	2392	rBV7	16213	27567	0.40%	0.036%
58	17.251	2401	2408	2414	rBV	3361447	4693303	67.85%	6.203%
59	17.345	2418	2424	2437	rVV	4623876	6617892	95.67%	8.747%
60	17.439	2437	2440	2445	rVB7	12577	21188	0.31%	0.028%
61	17.828	2503	2506	2511	rBV7	6185	11529	0.17%	0.015%
62	18.145	2556	2560	2568	rBV8	36113	71089	1.03%	0.094%
63	18.633	2641	2643	2646	rBV3	6979	9033	0.13%	0.012%
64	19.163	2729	2733	2739	rVB3	56145	80852	1.17%	0.107%
65	19.233	2741	2745	2749	rBV	51777	72633	1.05%	0.096%
66	19.386	2768	2771	2777	rBV6	26050	31230	0.45%	0.041%
67	19.586	2799	2805	2812	rBV	5007022	6461286	93.41%	8.540%
68	19.816	2841	2844	2855	rVB2	40186	75591	1.09%	0.100%
69	20.586	2973	2975	2980	rVB2	42129	43838	0.63%	0.058%
70	21.351	3100	3105	3113	rBV	2678473	3518759	50.87%	4.651%
71	23.627	3484	3492	3505	rBV	2954389	5800446	83.85%	7.666%
72	23.786	3512	3519	3535	rVB	1893226	3959323	57.24%	5.233%




Sum of corrected areas: 75663212

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018338.D
Acq On : 24 Nov 2023 21:16
Operator : MA/JU
Sample : 05336-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

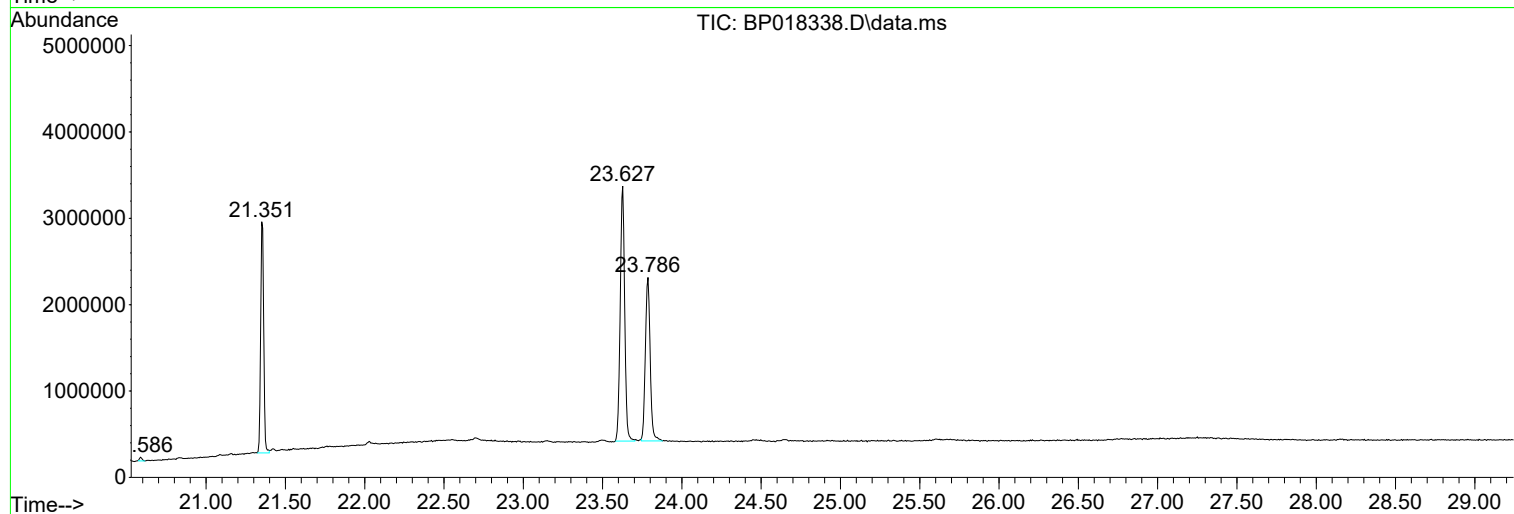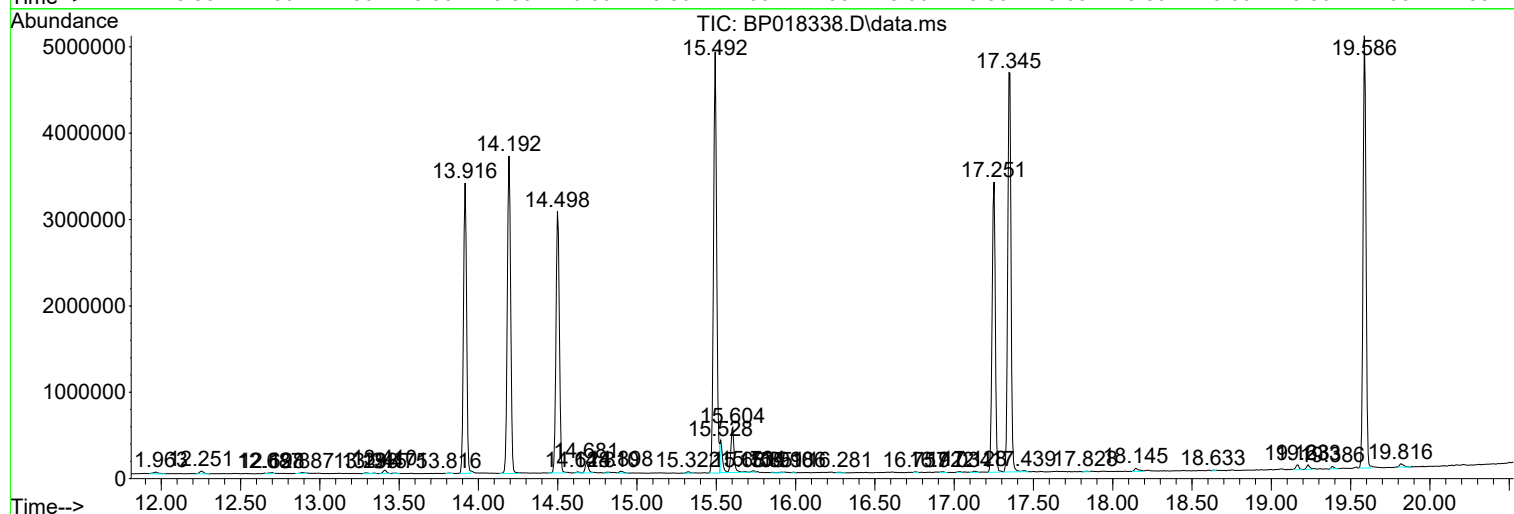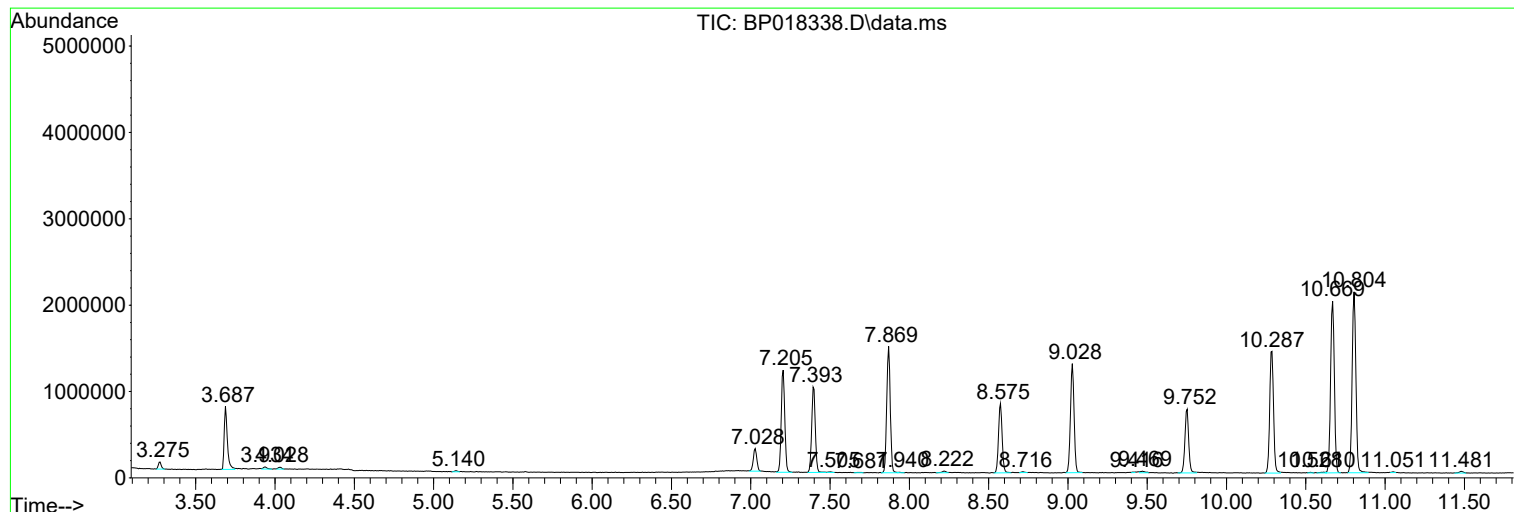

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018338.D
Acq On : 24 Nov 2023 21:16
Operator : MA/JU
Sample : 05336-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018338.D
Acq On : 24 Nov 2023 21:16
Operator : MA/JU
Sample : 05336-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc