

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018344.D
 Acq On : 25 Nov 2023 00:40
 Operator : MA/JU
 Sample : 05336-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rBV	78071	104043	1.44%	0.136%
2	3.558	76	80	86	rBV6	12814	28361	0.39%	0.037%
3	3.687	99	102	116	rBV	344070	513107	7.12%	0.672%
4	3.934	140	144	154	rBV2	23713	42001	0.58%	0.055%
5	4.028	156	160	166	rVB2	24426	38303	0.53%	0.050%
6	5.528	410	415	420	rBV8	7461	15226	0.21%	0.020%
7	5.575	420	423	429	rVB8	5458	10700	0.15%	0.014%
8	6.881	641	645	651	rVB4	10787	18069	0.25%	0.024%
9	7.028	664	670	678	rVB	301337	466500	6.48%	0.611%
10	7.204	693	700	709	rVB	1300594	2042158	28.35%	2.675%
11	7.393	726	732	742	rBV	1329533	2069031	28.73%	2.710%
12	7.499	747	750	754	rVB6	7580	11363	0.16%	0.015%
13	7.810	796	803	807	rBV2	32914	53933	0.75%	0.071%
14	7.869	807	813	821	rVV	1302412	2053350	28.51%	2.690%
15	7.946	821	826	829	rVB7	11215	20079	0.28%	0.026%
16	8.287	880	884	889	rVB6	4518	7991	0.11%	0.010%
17	8.575	926	933	944	rBV	779053	1226321	17.03%	1.606%
18	9.028	1002	1010	1019	rBV	1470482	2342965	32.53%	3.069%
19	9.469	1079	1085	1093	rVB2	27679	60223	0.84%	0.079%
20	9.751	1123	1133	1146	rBV	974310	1593430	22.12%	2.087%
21	10.028	1176	1180	1185	rBV6	6939	10705	0.15%	0.014%
22	10.287	1216	1224	1234	rBV	1645505	2761224	38.33%	3.617%
23	10.669	1282	1289	1299	rVB	1799744	2974442	41.30%	3.896%
24	10.804	1304	1312	1321	rBV	1223440	2003827	27.82%	2.625%
25	11.069	1352	1357	1365	rVB9	8816	21909	0.30%	0.029%
26	11.481	1423	1427	1432	rVB8	6046	11977	0.17%	0.016%
27	11.963	1503	1509	1519	rVB3	19015	43461	0.60%	0.057%
28	12.251	1549	1558	1566	rVB3	36877	71690	1.00%	0.094%
29	12.687	1630	1632	1638	rVB6	7093	8523	0.12%	0.011%
30	12.863	1657	1662	1663	rBV5	6961	8720	0.12%	0.011%
31	12.892	1663	1667	1671	rVV6	6671	11645	0.16%	0.015%
32	13.128	1704	1707	1713	rVB8	8145	12034	0.17%	0.016%
33	13.339	1739	1743	1747	rVB6	8338	10502	0.15%	0.014%
34	13.410	1750	1755	1761	rVB2	42181	67720	0.94%	0.089%
35	13.469	1761	1765	1766	rBV4	6735	8546	0.12%	0.011%
36	13.681	1799	1801	1806	rVB6	5276	9049	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018344.D
 Acq On : 25 Nov 2023 00:40
 Operator : MA/JU
 Sample : 05336-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	13.816	1820	1824	1827	rBV5	5562	9628	0.13%	0.013%
38	13.916	1834	1841	1853	rBV	3591261	4708174	65.37%	6.167%
39	14.192	1880	1888	1899	rBV	3953121	5661273	78.60%	7.416%
40	14.498	1933	1940	1947	rBV	2698798	3900726	54.16%	5.110%
41	14.563	1947	1951	1957	rVB	29016	48631	0.68%	0.064%
42	14.628	1958	1962	1966	rVB	15134	17796	0.25%	0.023%
43	14.681	1966	1971	1985	rBV	137589	233023	3.24%	0.305%
44	14.857	1997	2001	2005	rBV7	5107	10344	0.14%	0.014%
45	14.910	2005	2010	2017	rVB4	17600	40366	0.56%	0.053%
46	15.157	2049	2052	2057	rVB7	5531	7667	0.11%	0.010%
47	15.239	2063	2066	2074	rBV2	15137	29048	0.40%	0.038%
48	15.316	2074	2079	2085	rBV8	11429	21803	0.30%	0.029%
49	15.492	2102	2109	2116	rBV	5012364	7063648	98.07%	9.253%
50	15.604	2122	2128	2139	rBV	793156	1095040	15.20%	1.434%
51	15.733	2146	2150	2158	rVB3	23789	39297	0.55%	0.051%
52	15.839	2165	2168	2170	rBV3	6622	7317	0.10%	0.010%
53	15.922	2177	2182	2183	rBV4	8109	9477	0.13%	0.012%
54	16.180	2221	2226	2229	rBV7	7033	12053	0.17%	0.016%
55	16.275	2237	2242	2250	rBV7	9056	19579	0.27%	0.026%
56	16.757	2321	2324	2327	rBV5	7033	8509	0.12%	0.011%
57	16.792	2327	2330	2335	rVB3	13778	17844	0.25%	0.023%
58	16.892	2344	2347	2351	rVB5	12262	14411	0.20%	0.019%
59	17.039	2365	2372	2375	rBV6	7678	15725	0.22%	0.021%
60	17.063	2375	2376	2381	rVB5	5930	7925	0.11%	0.010%
61	17.122	2382	2386	2392	rVV7	16429	24391	0.34%	0.032%
62	17.245	2400	2407	2414	rBV	2610618	3875077	53.80%	5.076%
63	17.345	2418	2424	2438	rVV2	4890261	7034246	97.66%	9.215%
64	17.651	2473	2476	2480	rVB2	19270	26126	0.36%	0.034%
65	17.927	2520	2523	2528	rVB6	10782	14143	0.20%	0.019%
66	18.145	2556	2560	2570	rBV2	117243	183182	2.54%	0.240%
67	18.604	2634	2638	2641	rBV4	11893	19358	0.27%	0.025%
68	19.163	2730	2733	2740	rVB2	59947	76014	1.06%	0.100%
69	19.227	2740	2744	2749	rBV	54394	89339	1.24%	0.117%
70	19.386	2767	2771	2777	rBV2	97119	126287	1.75%	0.165%
71	19.586	2799	2805	2812	rBV	5398259	6960420	96.63%	9.118%
72	20.586	2972	2975	2979	rBV3	50008	54862	0.76%	0.072%
73	21.351	3100	3105	3111	rBV	2476112	3125845	43.40%	4.095%
74	23.627	3484	3492	3506	rBV2	3661320	7202883	100.00%	9.435%
75	23.786	3512	3519	3535	rVB	1799841	3773976	52.40%	4.944%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018344.D
Acq On : 25 Nov 2023 00:40
Operator : MA/JU
Sample : 05336-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 76338581

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018344.D
Acq On : 25 Nov 2023 00:40
Operator : MA/JU
Sample : 05336-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

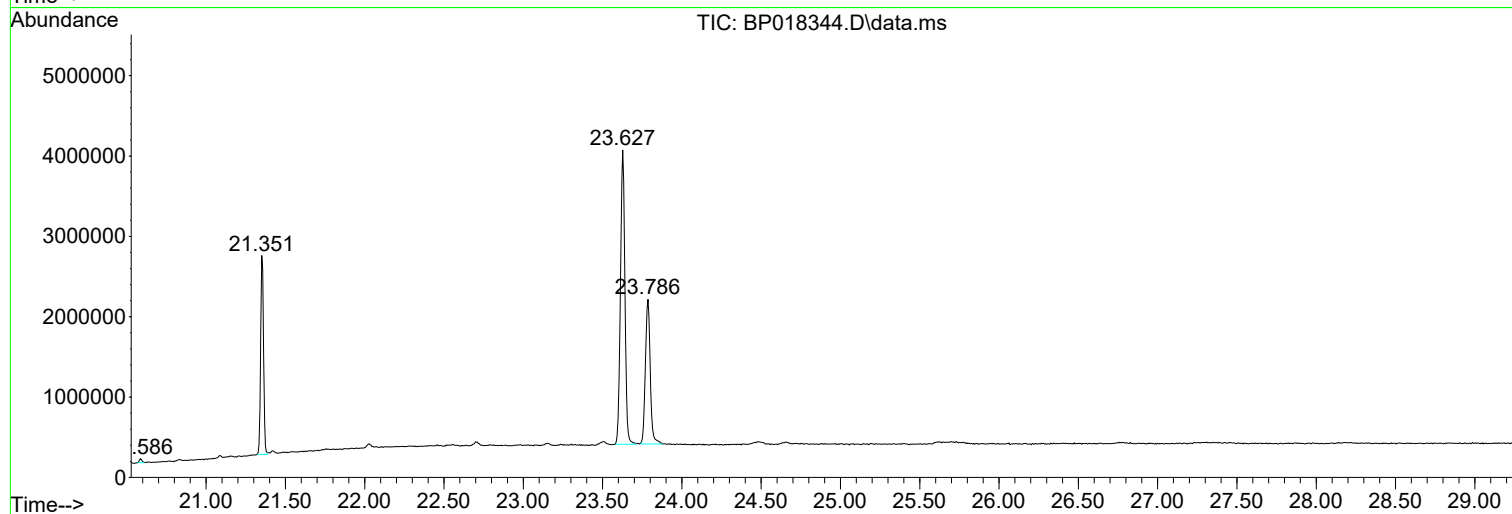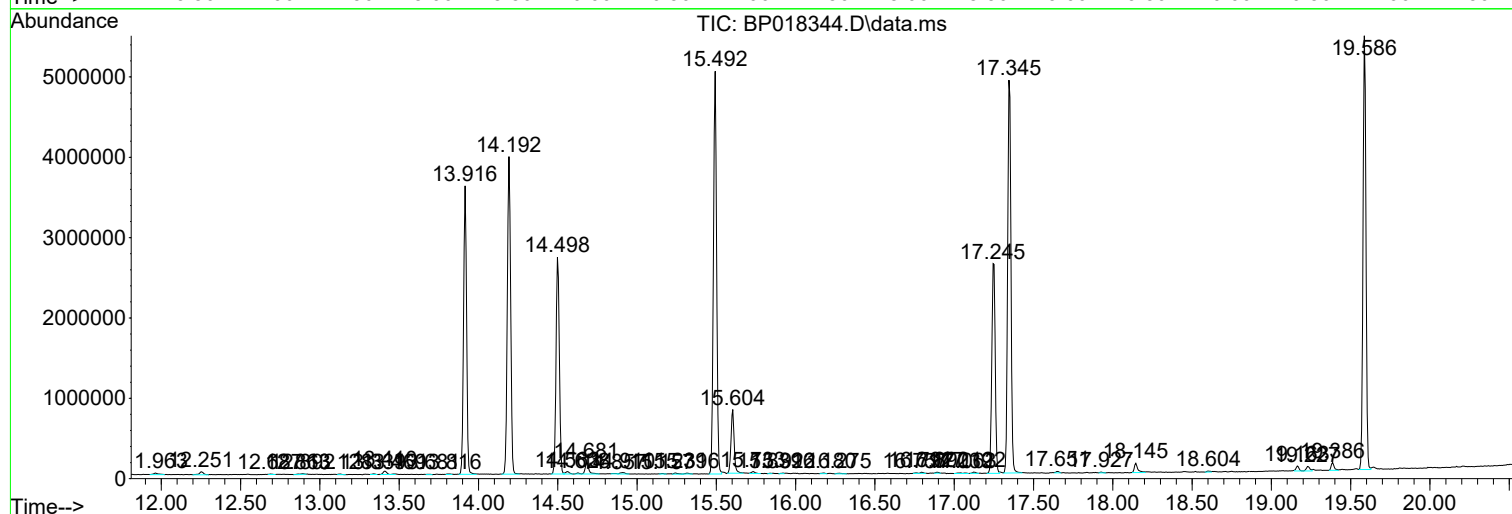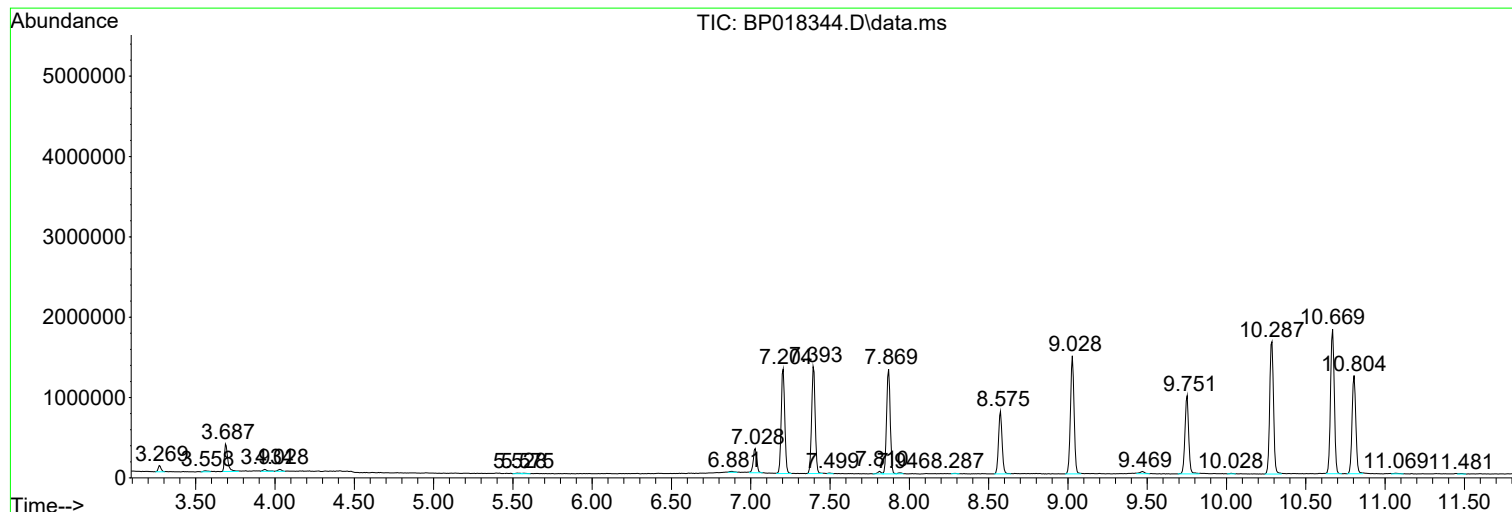

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018344.D
Acq On : 25 Nov 2023 00:40
Operator : MA/JU
Sample : 05336-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018344.D
Acq On : 25 Nov 2023 00:40
Operator : MA/JU
Sample : 05336-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc