

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018345.D
 Acq On : 25 Nov 2023 01:14
 Operator : MA/JU
 Sample : 05336-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rVB	79798	105173	1.46%	0.144%
2	3.558	77	80	81	rBV3	10494	11694	0.16%	0.016%
3	3.687	98	102	114	rBV	309205	460426	6.40%	0.632%
4	3.940	141	145	150	rVB2	23173	34159	0.47%	0.047%
5	4.028	157	160	164	rVB	25067	32141	0.45%	0.044%
6	4.963	315	319	324	rBV8	7079	13858	0.19%	0.019%
7	5.140	346	349	354	rBV5	8185	11515	0.16%	0.016%
8	7.028	663	670	677	rVB	276613	430196	5.98%	0.590%
9	7.204	693	700	707	rVB	1242629	1887993	26.25%	2.590%
10	7.393	724	732	740	rBV	1077485	1699462	23.63%	2.331%
11	7.499	746	750	756	rVB8	6445	14068	0.20%	0.019%
12	7.869	804	813	821	rBV	1361728	2114313	29.40%	2.900%
13	7.940	821	825	829	rVV7	10660	16581	0.23%	0.023%
14	8.246	874	877	881	rVB6	5733	8217	0.11%	0.011%
15	8.575	924	933	943	rBV	868026	1326580	18.45%	1.820%
16	8.716	951	957	964	rVB2	33891	57684	0.80%	0.079%
17	8.975	997	1001	1003	rBV5	6030	8560	0.12%	0.012%
18	9.028	1003	1010	1020	rVB	1338786	2135101	29.69%	2.929%
19	9.293	1050	1055	1058	rBV7	5522	10005	0.14%	0.014%
20	9.340	1058	1063	1068	rVV9	3904	7616	0.11%	0.010%
21	9.469	1078	1085	1091	rVB2	28989	56806	0.79%	0.078%
22	9.751	1125	1133	1139	rBV	840309	1364211	18.97%	1.871%
23	10.069	1184	1187	1194	rBV9	7097	14424	0.20%	0.020%
24	10.287	1216	1224	1235	rBV	1498064	2497839	34.73%	3.426%
25	10.669	1281	1289	1297	rVB	1767870	2967375	41.26%	4.070%
26	10.804	1304	1312	1323	rBV	1356867	2287185	31.80%	3.137%
27	11.022	1343	1349	1355	rBV10	12998	31293	0.44%	0.043%
28	11.275	1385	1392	1396	rVB8	7189	19337	0.27%	0.027%
29	11.692	1461	1463	1472	rVB10	7309	10532	0.15%	0.014%
30	11.781	1475	1478	1487	rVB9	8896	15626	0.22%	0.021%
31	11.963	1503	1509	1514	rBV6	9307	17535	0.24%	0.024%
32	12.051	1521	1524	1528	rVB6	9001	9912	0.14%	0.014%
33	12.257	1549	1559	1565	rBV2	30119	65475	0.91%	0.090%
34	12.545	1598	1608	1615	rVB2	31338	55810	0.78%	0.077%
35	12.692	1629	1633	1638	rVB8	4963	9583	0.13%	0.013%
36	12.981	1675	1682	1684	rBV8	5128	9851	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018345.D
 Acq On : 25 Nov 2023 01:14
 Operator : MA/JU
 Sample : 05336-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	13.028	1687	1690	1693	rVB4	5637	7777	0.11%	0.011%
38	13.128	1704	1707	1711	rVB5	6994	9134	0.13%	0.013%
39	13.181	1711	1716	1718	rBV6	7961	13209	0.18%	0.018%
40	13.292	1731	1735	1739	rBV7	6328	10279	0.14%	0.014%

41	13.339	1739	1743	1749	rVB6	17341	29197	0.41%	0.040%
42	13.410	1749	1755	1759	rBV3	28020	46470	0.65%	0.064%
43	13.475	1762	1766	1769	rBV5	7716	12468	0.17%	0.017%
44	13.669	1796	1799	1808	rVB5	12995	28672	0.40%	0.039%
45	13.822	1818	1825	1829	rBV7	18984	35308	0.49%	0.048%

46	13.916	1835	1841	1851	rVB	2938830	4021684	55.92%	5.517%
47	14.192	1878	1888	1903	rBV	3497337	4976037	69.19%	6.826%
48	14.422	1923	1927	1930	rBV5	7224	9437	0.13%	0.013%
49	14.498	1930	1940	1946	rVV	2527517	3688030	51.28%	5.059%
50	14.563	1946	1951	1956	rVV	395633	580081	8.07%	0.796%

51	14.628	1958	1962	1966	rVV	43124	62959	0.88%	0.086%
52	14.680	1966	1971	1984	rVV	130334	210719	2.93%	0.289%
53	14.816	1989	1994	1996	rBV6	7974	12258	0.17%	0.017%
54	14.898	2002	2008	2015	rVB	151717	238403	3.31%	0.327%
55	15.039	2027	2032	2034	rBV6	13597	18442	0.26%	0.025%

56	15.116	2042	2045	2050	rBV6	7783	12276	0.17%	0.017%
57	15.322	2075	2080	2085	rVB9	10859	18706	0.26%	0.026%
58	15.416	2091	2096	2102	rBV3	31602	50026	0.70%	0.069%
59	15.492	2102	2109	2115	rVV	4327897	6097032	84.78%	8.363%
60	15.545	2115	2118	2122	rVV	88730	125864	1.75%	0.173%

61	15.604	2122	2128	2136	rVV	602311	879079	12.22%	1.206%
62	15.669	2136	2139	2144	rVV7	18221	34853	0.48%	0.048%
63	15.733	2147	2150	2154	rVB3	17360	23975	0.33%	0.033%
64	15.839	2164	2168	2176	rVB6	11711	22615	0.31%	0.031%
65	15.916	2176	2181	2184	rVV7	9211	18706	0.26%	0.026%

66	15.980	2187	2192	2201	rVB7	19641	42080	0.59%	0.058%
67	16.216	2227	2232	2237	rVB5	25565	41839	0.58%	0.057%
68	16.275	2240	2242	2246	rVB3	7496	7445	0.10%	0.010%
69	16.504	2276	2281	2288	rBV3	32786	60215	0.84%	0.083%
70	16.757	2320	2324	2331	rVB8	11935	18561	0.26%	0.025%

71	16.892	2337	2347	2352	rBV5	60849	124662	1.73%	0.171%
72	17.033	2367	2371	2373	rBV3	9692	11196	0.16%	0.015%
73	17.063	2374	2376	2382	rVB4	11128	13734	0.19%	0.019%
74	17.133	2382	2388	2389	rBV6	10720	17338	0.24%	0.024%
75	17.192	2395	2398	2401	rBV5	7446	12323	0.17%	0.017%

76	17.245	2401	2407	2413	rBV	2448813	3504317	48.73%	4.807%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018345.D
 Acq On : 25 Nov 2023 01:14
 Operator : MA/JU
 Sample : 05336-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.345	2418	2424	2436	rVB	4286555	6051384	84.14%	8.301%
78	17.651	2469	2476	2481	rBV	234909	328464	4.57%	0.451%
79	17.804	2498	2502	2510	rBV2	25599	51261	0.71%	0.070%
80	18.145	2556	2560	2570	rBV2	102208	174149	2.42%	0.239%
81	18.592	2634	2636	2640	rBV5	6930	9171	0.13%	0.013%
82	18.739	2659	2661	2668	rVB7	10062	17370	0.24%	0.024%
83	19.163	2729	2733	2739	rVB2	53114	72954	1.01%	0.100%
84	19.233	2740	2745	2748	rBV	48070	71476	0.99%	0.098%
85	19.386	2767	2771	2778	rVB3	70035	92628	1.29%	0.127%
86	19.586	2799	2805	2816	rBV	4958517	6373727	88.63%	8.743%
87	21.086	3057	3060	3065	rBV3	57104	73476	1.02%	0.101%
88	21.351	3100	3105	3114	rBV	2714687	3359348	46.71%	4.608%
89	23.627	3484	3492	3507	rBV2	3593220	7191757	100.00%	9.865%
90	23.786	3512	3519	3535	rVB	1950808	4068236	56.57%	5.580%




Sum of corrected areas: 72900943

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018345.D
Acq On : 25 Nov 2023 01:14
Operator : MA/JU
Sample : 05336-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

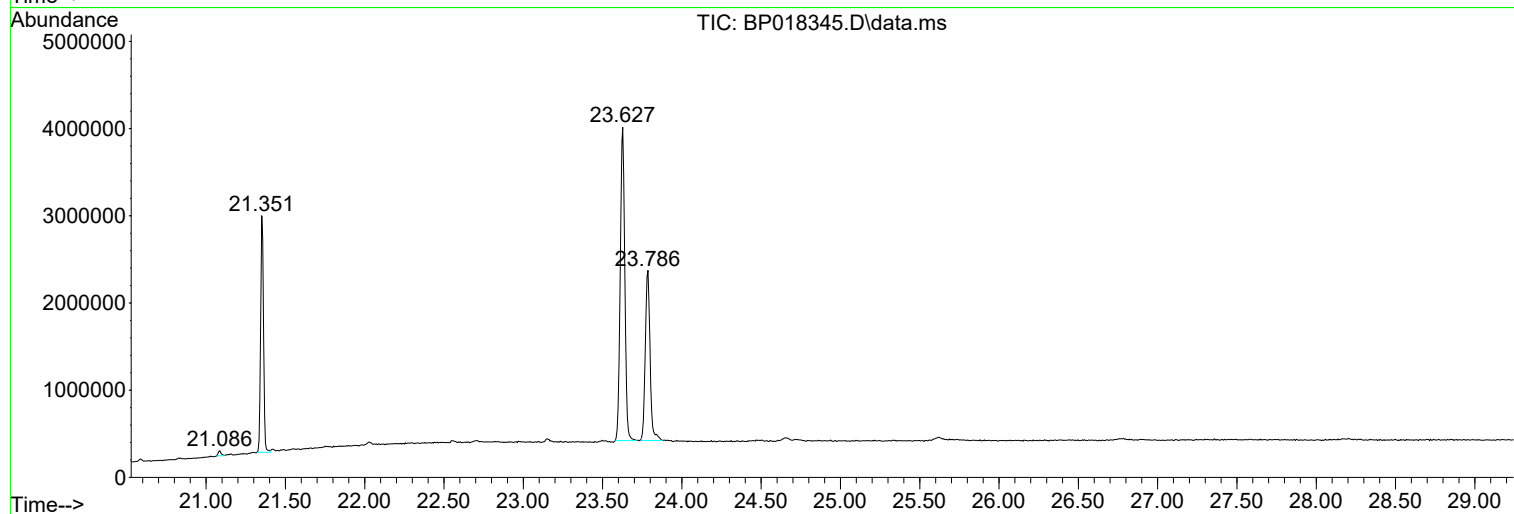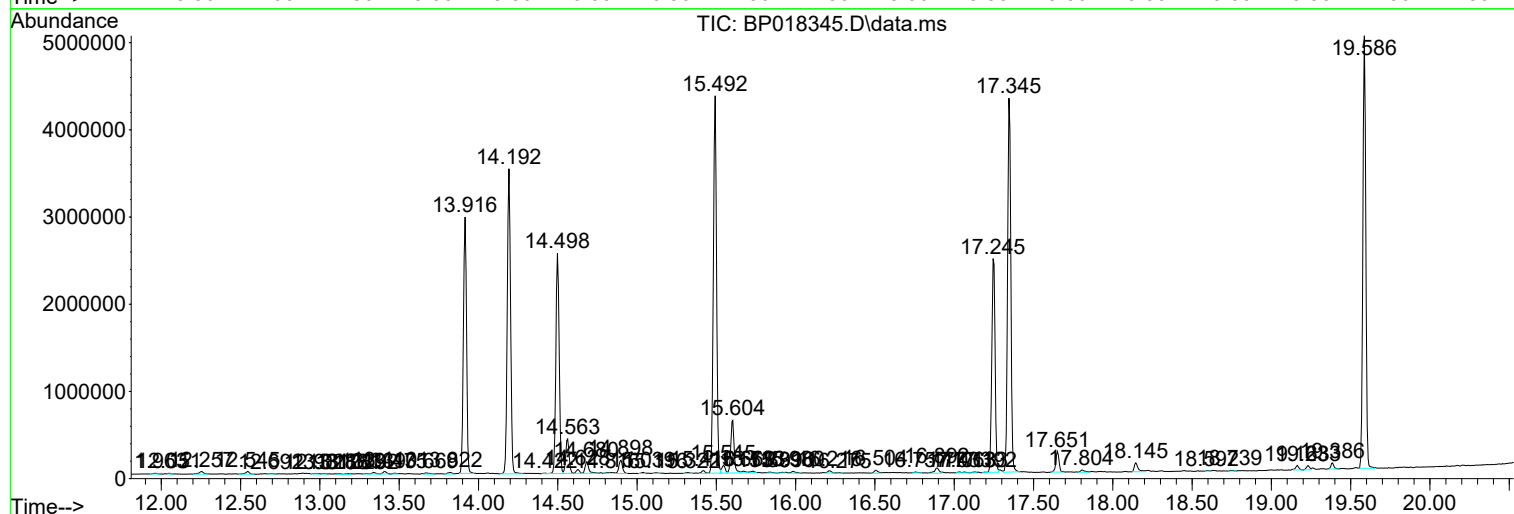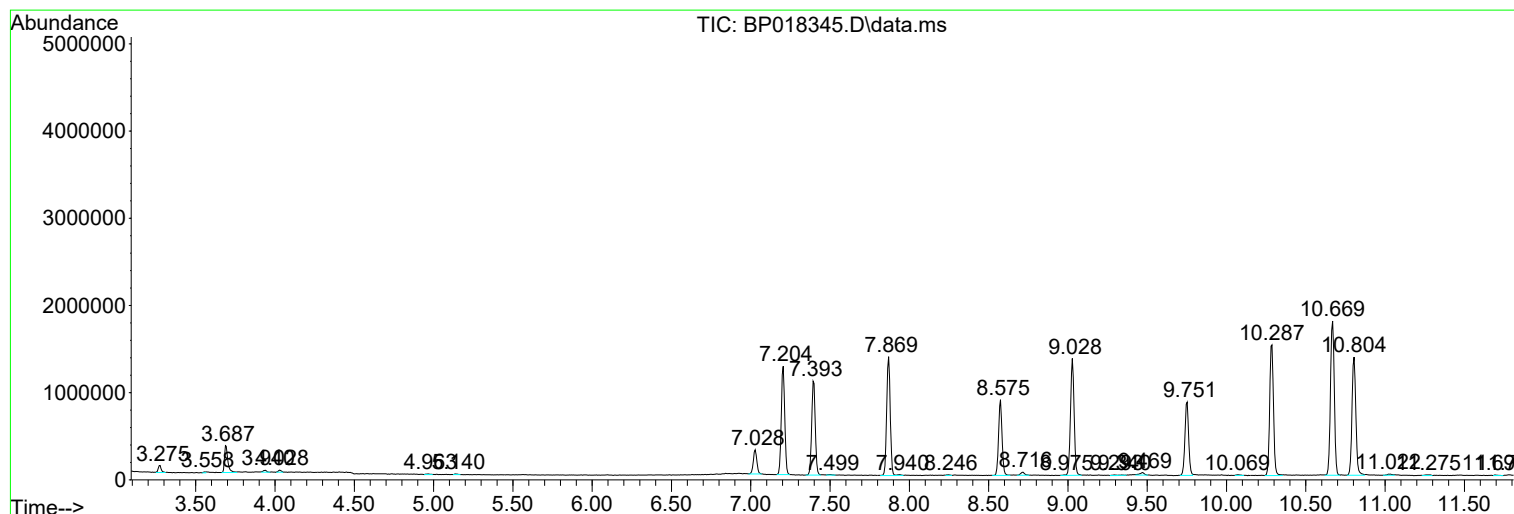

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018345.D
Acq On : 25 Nov 2023 01:14
Operator : MA/JU
Sample : 05336-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018345.D
Acq On : 25 Nov 2023 01:14
Operator : MA/JU
Sample : 05336-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc