

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018351.D
 Acq On : 25 Nov 2023 05:12
 Operator : MA/JU
 Sample : PB157273BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK273

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rBV	119451	149858	1.97%	0.201%
2	3.687	98	102	113	rBV	1266175	1732228	22.78%	2.320%
3	4.028	157	160	166	rVB	23826	27682	0.36%	0.037%
4	7.028	663	670	684	rVB	1563716	2379097	31.29%	3.187%
5	7.204	693	700	711	rVB	1326383	2019583	26.56%	2.705%
6	7.393	726	732	740	rBV	1577602	2493683	32.80%	3.340%
7	7.869	806	813	819	rBV	1292140	2016443	26.52%	2.701%
8	8.299	883	886	892	rVB7	5005	8939	0.12%	0.012%
9	8.575	924	933	945	rBV	1815027	2854423	37.54%	3.824%
10	9.028	1001	1010	1019	rBV	1336244	2163734	28.46%	2.898%
11	9.428	1068	1078	1079	rBV8	6768	15625	0.21%	0.021%
12	9.457	1081	1083	1091	rVB9	9068	18020	0.24%	0.024%
13	9.751	1124	1133	1145	rBV	886473	1463198	19.24%	1.960%
14	10.281	1215	1223	1231	rBV	1655878	2774597	36.49%	3.717%
15	10.604	1272	1278	1280	rBV7	5098	8564	0.11%	0.011%
16	10.669	1280	1289	1296	rVB	1549929	2623387	34.50%	3.514%
17	10.804	1304	1312	1323	rBV	1462704	2450466	32.23%	3.282%
18	11.892	1491	1497	1499	rVV7	3791	8492	0.11%	0.011%
19	11.957	1504	1508	1516	rVB10	8553	20152	0.27%	0.027%
20	12.251	1553	1558	1566	rVB2	32848	52530	0.69%	0.070%
21	12.692	1629	1633	1638	rBV8	5454	10724	0.14%	0.014%
22	12.887	1660	1666	1671	rBV10	7794	15743	0.21%	0.021%
23	13.404	1749	1754	1762	rVV4	24419	44750	0.59%	0.060%
24	13.475	1762	1766	1773	rVB9	8231	17538	0.23%	0.023%
25	13.916	1834	1841	1852	rBV	2482630	3477855	45.74%	4.659%
26	14.192	1880	1888	1896	rBV	3112972	4531106	59.59%	6.070%
27	14.498	1933	1940	1952	rVV	2081705	2984939	39.26%	3.998%
28	14.686	1965	1972	1983	rBV	861286	1325142	17.43%	1.775%
29	15.492	2101	2109	2115	rBV	3708782	5328288	70.08%	7.137%
30	15.598	2122	2127	2141	rBV	561623	806174	10.60%	1.080%
31	15.733	2146	2150	2159	rVB4	16954	30183	0.40%	0.040%
32	16.275	2238	2242	2247	rBV8	6156	11642	0.15%	0.016%
33	16.580	2290	2294	2298	rVB7	6132	9919	0.13%	0.013%
34	17.127	2383	2387	2391	rBV7	7517	13027	0.17%	0.017%
35	17.245	2401	2407	2414	rBV	2213463	3057896	40.22%	4.096%
36	17.345	2418	2424	2438	rBV	3822215	5360902	70.50%	7.181%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018351.D
Acq On : 25 Nov 2023 05:12
Operator : MA/JU
Sample : PB157273BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK273

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	17.927	2519	2523	2526	rBV6	7594	10921	0.14%	0.015%
38	18.151	2554	2561	2563	rBV8	12635	25851	0.34%	0.035%
39	19.163	2729	2733	2739	rVB2	51274	63761	0.84%	0.085%
40	19.227	2740	2744	2749	rBV	47471	61546	0.81%	0.082%
41	19.586	2799	2805	2811	rBV	5210374	6480817	85.23%	8.681%
42	21.351	3100	3105	3115	rBV	3044125	3757794	49.42%	5.034%
43	23.627	3484	3492	3510	rBV2	3720778	7603649	100.00%	10.185%
44	23.786	3512	3519	3538	rVB	2030383	4342063	57.10%	5.816%




Sum of corrected areas: 74652931

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018351.D
Acq On : 25 Nov 2023 05:12
Operator : MA/JU
Sample : PB157273BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK273

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

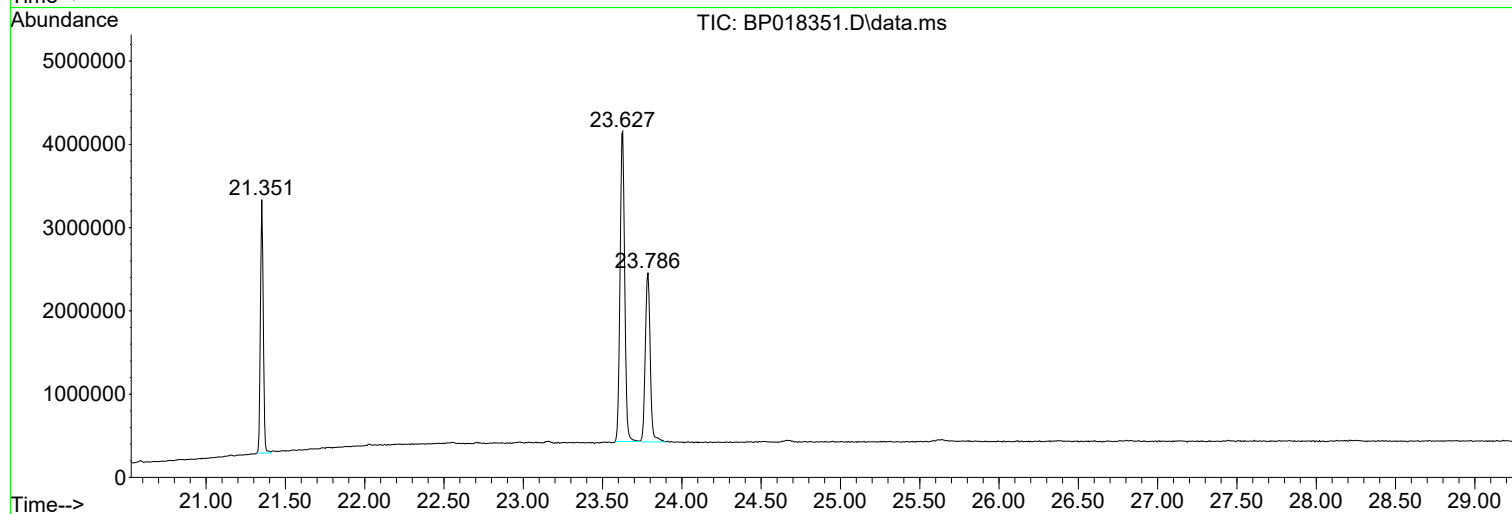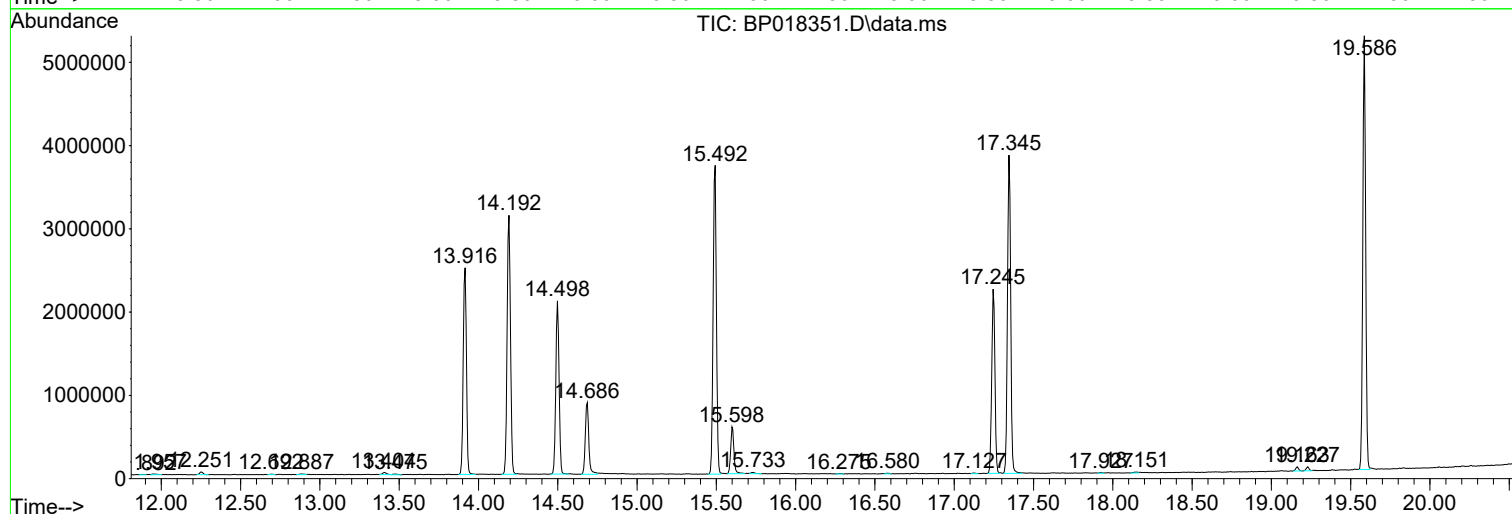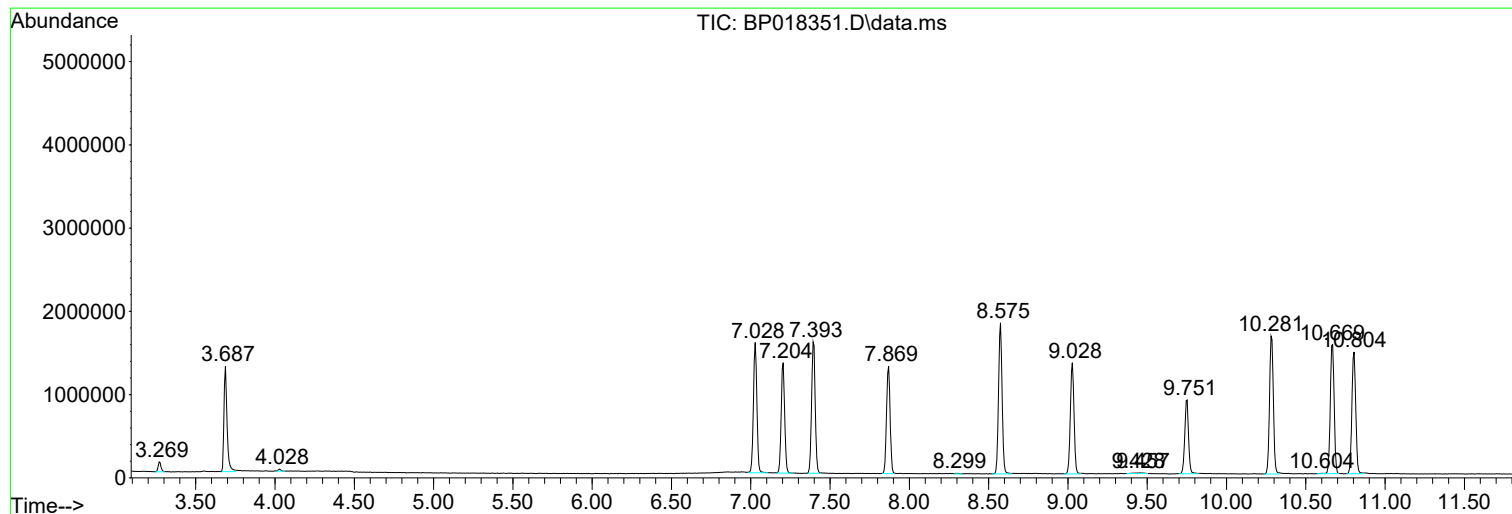

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018351.D
Acq On : 25 Nov 2023 05:12
Operator : MA/JU
Sample : PB157273BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK273

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018351.D
Acq On : 25 Nov 2023 05:12
Operator : MA/JU
Sample : PB157273BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK273

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------