

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018352.D
 Acq On : 25 Nov 2023 05:45
 Operator : MA/JU
 Sample : PB157098BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	37	rVB	130455	156983	2.01%	0.200%
2	3.687	98	102	115	rBV	1348622	1858502	23.75%	2.367%
3	4.028	156	160	165	rVB2	29649	44301	0.57%	0.056%
4	7.028	663	670	680	rVB	1670485	2534681	32.39%	3.228%
5	7.205	693	700	707	rVB	1403519	2161168	27.62%	2.753%
6	7.393	725	732	742	rBV	1721917	2687269	34.34%	3.423%
7	7.869	805	813	820	rVB	1500372	2314180	29.57%	2.948%
8	8.575	926	933	942	rBV	1951860	3016296	38.54%	3.842%
9	9.028	1001	1010	1020	rBV	1449773	2285275	29.20%	2.911%
10	9.752	1123	1133	1140	rBV	919058	1514781	19.36%	1.929%
11	10.281	1216	1223	1233	rBV	1761132	2899849	37.06%	3.694%
12	10.669	1281	1289	1299	rVB	1780157	2999974	38.34%	3.821%
13	10.805	1304	1312	1320	rBV	1509998	2550197	32.59%	3.248%
14	11.957	1503	1508	1513	rVB7	7183	13332	0.17%	0.017%
15	12.257	1552	1559	1563	rBV2	33669	56915	0.73%	0.072%
16	13.404	1750	1754	1759	rVV3	20522	35636	0.46%	0.045%
17	13.475	1762	1766	1770	rVB7	7018	10724	0.14%	0.014%
18	13.804	1815	1822	1826	rBV10	4567	9698	0.12%	0.012%
19	13.916	1835	1841	1853	rBV	2591423	3523014	45.02%	4.487%
20	14.193	1880	1888	1900	rBV	3276871	4648174	59.40%	5.920%
21	14.498	1933	1940	1951	rBV	2330804	3312135	42.33%	4.219%
22	14.687	1966	1972	1987	rVV	919000	1339557	17.12%	1.706%
23	15.322	2075	2080	2084	rVB8	5128	9967	0.13%	0.013%
24	15.493	2102	2109	2117	rBV	3858770	5438190	69.49%	6.927%
25	15.598	2122	2127	2137	rBV	548527	808114	10.33%	1.029%
26	15.728	2145	2149	2156	rVB5	18278	33850	0.43%	0.043%
27	16.575	2290	2293	2299	rBV8	5754	7894	0.10%	0.010%
28	16.757	2318	2324	2328	rBV9	8334	15642	0.20%	0.020%
29	16.916	2349	2351	2357	rBV7	6177	9274	0.12%	0.012%
30	17.122	2383	2386	2394	rBV9	6956	11829	0.15%	0.015%
31	17.245	2400	2407	2418	rBV	2352956	3367317	43.03%	4.289%
32	17.345	2418	2424	2439	rVV	3963991	5416999	69.22%	6.900%
33	17.834	2503	2507	2514	rBV10	5628	11411	0.15%	0.015%
34	18.145	2557	2560	2564	rBV6	9552	15780	0.20%	0.020%
35	19.163	2729	2733	2737	rBV2	48908	62779	0.80%	0.080%
36	19.233	2740	2745	2751	rVV	45578	65368	0.84%	0.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018352.D
Acq On : 25 Nov 2023 05:45
Operator : MA/JU
Sample : PB157098BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.381	2768	2770	2772	rBV2	11100	9867	0.13%	0.013%
38	19.586	2799	2805	2812	rBV	4925878	6538797	83.56%	8.328%
39	21.351	3100	3105	3112	rBV	3235033	4087712	52.24%	5.207%
40	23.627	3484	3492	3509	rBV	3993105	7825410	100.00%	9.967%
41	23.786	3512	3519	3539	rVB	2279025	4802457	61.37%	6.117%




Sum of corrected areas: 78511298

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018352.D
Acq On : 25 Nov 2023 05:45
Operator : MA/JU
Sample : PB157098BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

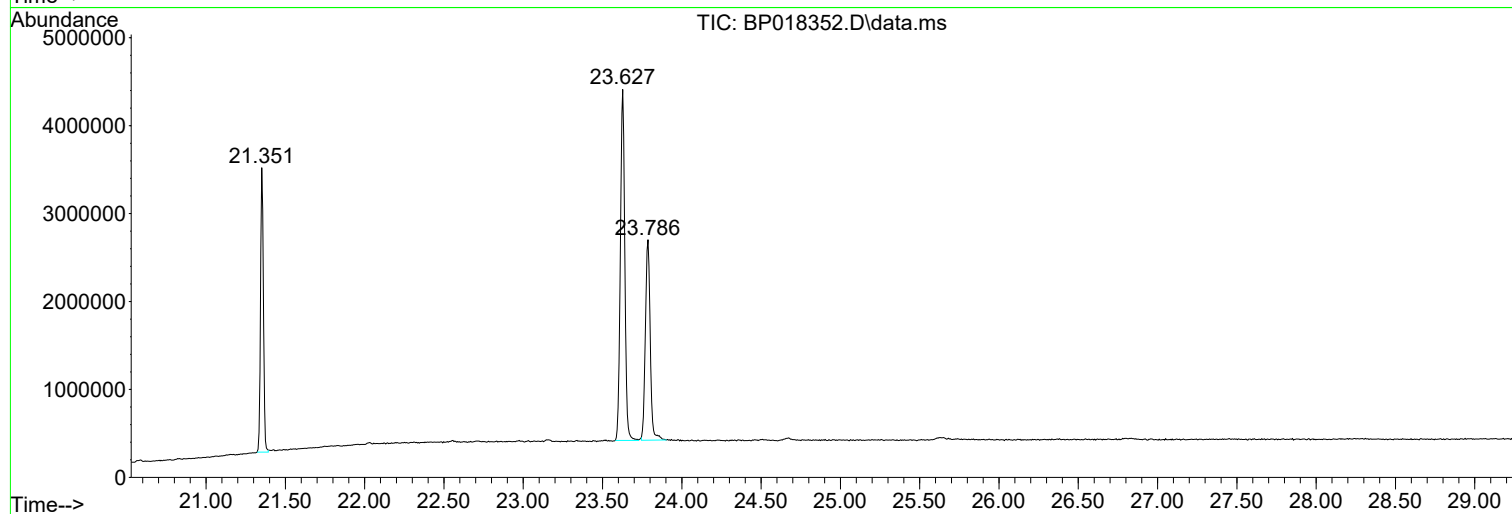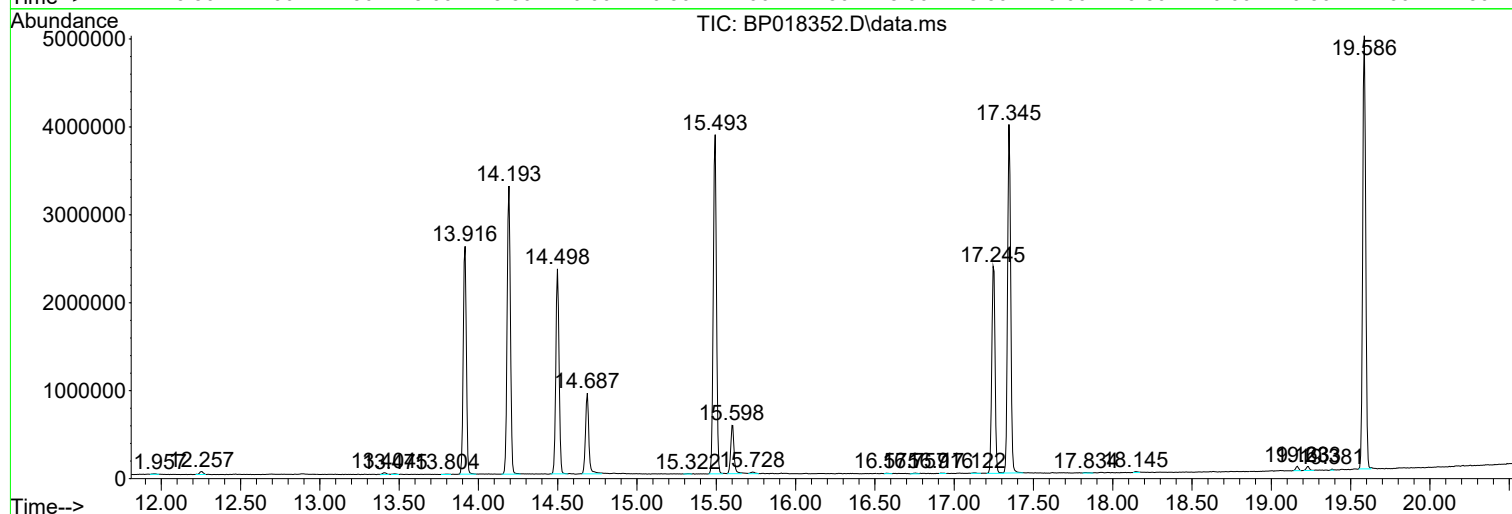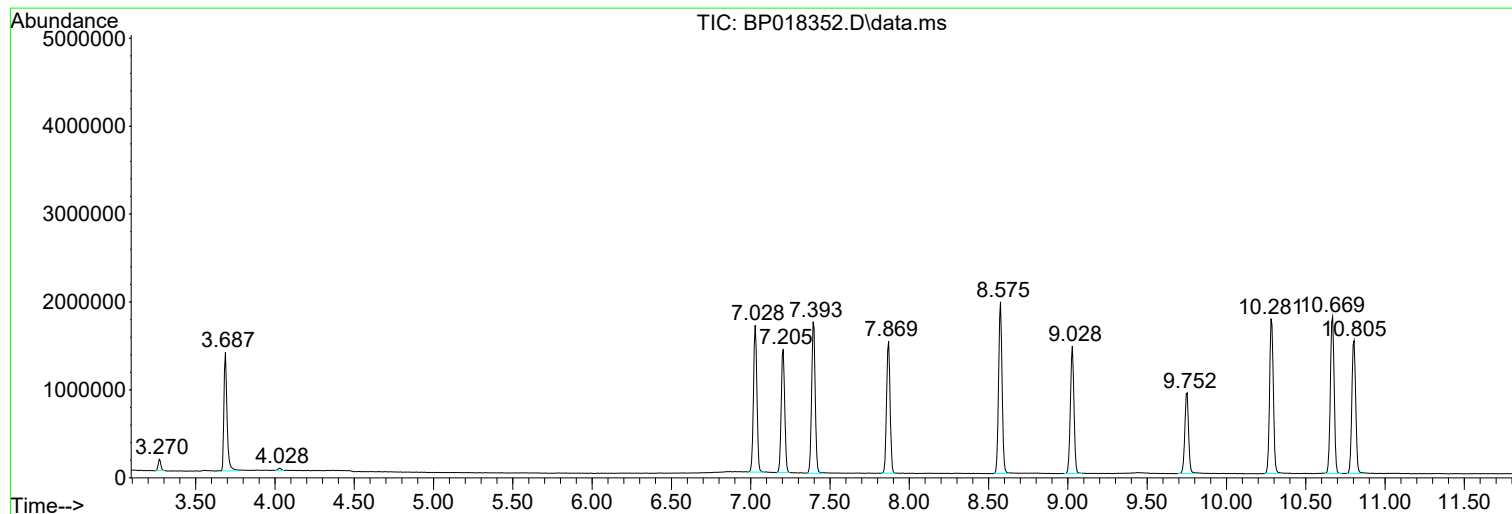

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018352.D
Acq On : 25 Nov 2023 05:45
Operator : MA/JU
Sample : PB157098BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018352.D
Acq On : 25 Nov 2023 05:45
Operator : MA/JU
Sample : PB157098BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc