

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018354.D
 Acq On : 25 Nov 2023 06:53
 Operator : MA/JU
 Sample : PB157121BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rVB	145465	183366	2.17%	0.185%
2	3.687	98	102	120	rBV	1511225	2186829	25.85%	2.206%
3	4.028	157	160	165	rVB	27739	36304	0.43%	0.037%
4	7.028	663	670	679	rVB	2065270	3148710	37.23%	3.177%
5	7.205	693	700	709	rVB	1724712	2643674	31.26%	2.667%
6	7.393	725	732	740	rBV	2055349	3242355	38.33%	3.271%
7	7.869	806	813	820	rBV	1478957	2317535	27.40%	2.338%
8	8.575	923	933	944	rBV	2574200	4063524	48.04%	4.099%
9	9.028	1001	1010	1019	rBV	1863921	2972761	35.15%	2.999%
10	9.752	1122	1133	1147	rBV	1288834	2157553	25.51%	2.177%
11	10.281	1214	1223	1235	rBV	2423251	4067050	48.08%	4.103%
12	10.669	1281	1289	1296	rVB	1989840	3368439	39.82%	3.398%
13	10.805	1301	1312	1325	rBV	2209866	3641588	43.05%	3.674%
14	12.251	1551	1558	1565	rBV	49946	84513	1.00%	0.085%
15	13.410	1749	1755	1760	rBV2	29169	45586	0.54%	0.046%
16	13.475	1762	1766	1771	rVB7	8481	14300	0.17%	0.014%
17	13.916	1834	1841	1856	rBV	4187097	5687311	67.24%	5.738%
18	14.193	1881	1888	1902	rBV	4895842	7182761	84.92%	7.246%
19	14.498	1933	1940	1948	rBV	3019270	4288103	50.70%	4.326%
20	14.687	1965	1972	1983	rBV	1258795	1795623	21.23%	1.812%
21	14.910	2007	2010	2015	rVB6	9583	14009	0.17%	0.014%
22	15.493	2102	2109	2116	rBV	5873833	8458316	100.00%	8.533%
23	15.598	2122	2127	2136	rBV	871382	1232212	14.57%	1.243%
24	15.728	2145	2149	2156	rVB	28661	48472	0.57%	0.049%
25	16.051	2202	2204	2210	rVB7	6371	11122	0.13%	0.011%
26	16.275	2239	2242	2246	rVB4	6858	9856	0.12%	0.010%
27	16.928	2350	2353	2357	rVB6	7098	9730	0.12%	0.010%
28	17.034	2367	2371	2373	rBV5	8716	13407	0.16%	0.014%
29	17.245	2400	2407	2417	rBV	2984877	4224041	49.94%	4.261%
30	17.345	2417	2424	2439	rVV	5677013	7960773	94.12%	8.031%
31	18.151	2556	2561	2563	rBV5	11128	19785	0.23%	0.020%
32	18.745	2658	2662	2668	rBV9	7838	19868	0.23%	0.020%
33	19.163	2729	2733	2737	rVB2	66616	83694	0.99%	0.084%
34	19.228	2740	2744	2749	rBV	58325	77024	0.91%	0.078%
35	19.586	2799	2805	2812	rBV	6043736	7808698	92.32%	7.878%
36	21.351	3100	3105	3115	rBV	2884990	3664057	43.32%	3.696%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018354.D
Acq On : 25 Nov 2023 06:53
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	23.627	3484	3492	3510	rBV2	4090226	8217990	97.16%	8.291%
38	23.786	3512	3519	3533	rVB	1967554	4122120	48.73%	4.159%




Sum of corrected areas: 99123059

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018354.D
Acq On : 25 Nov 2023 06:53
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

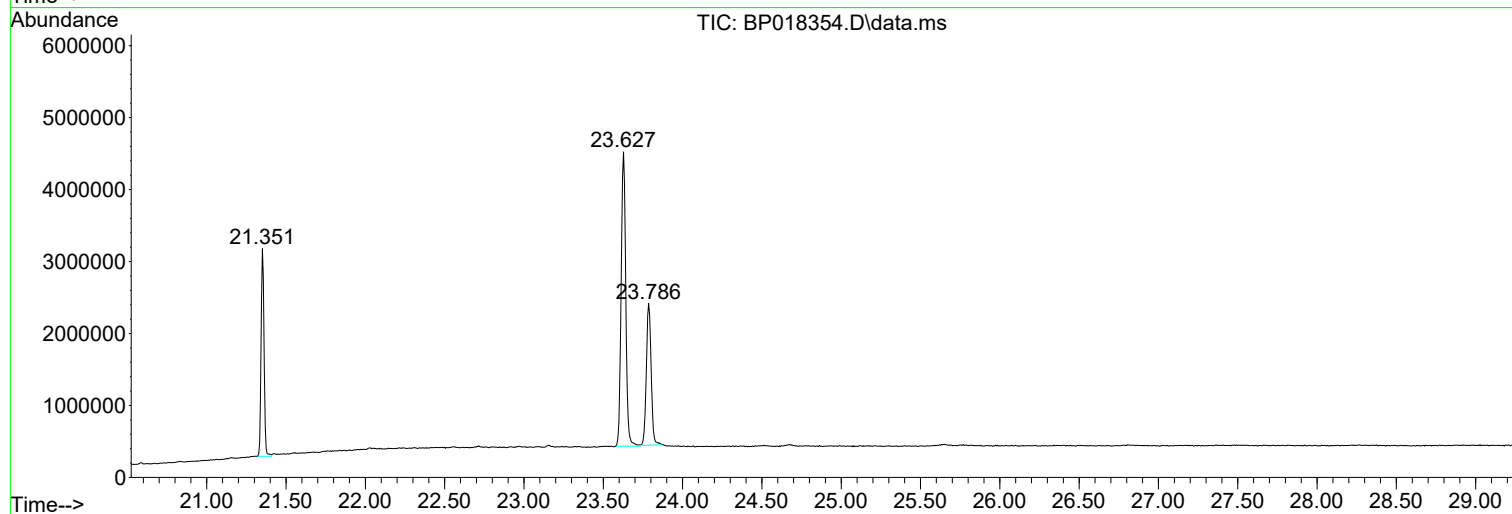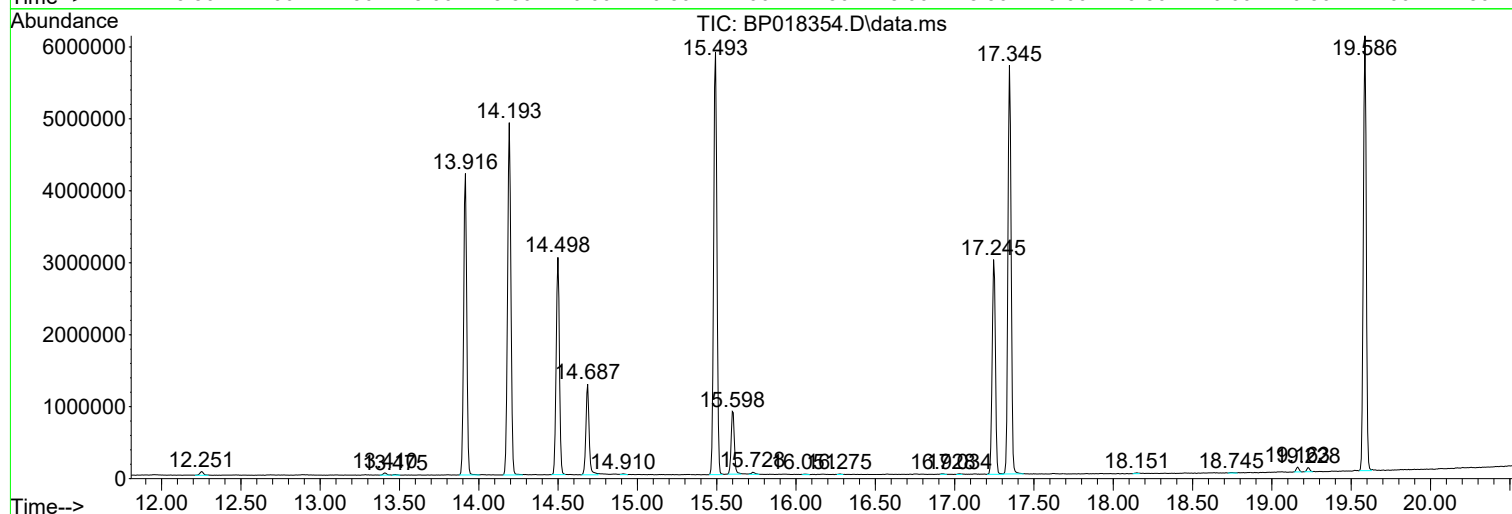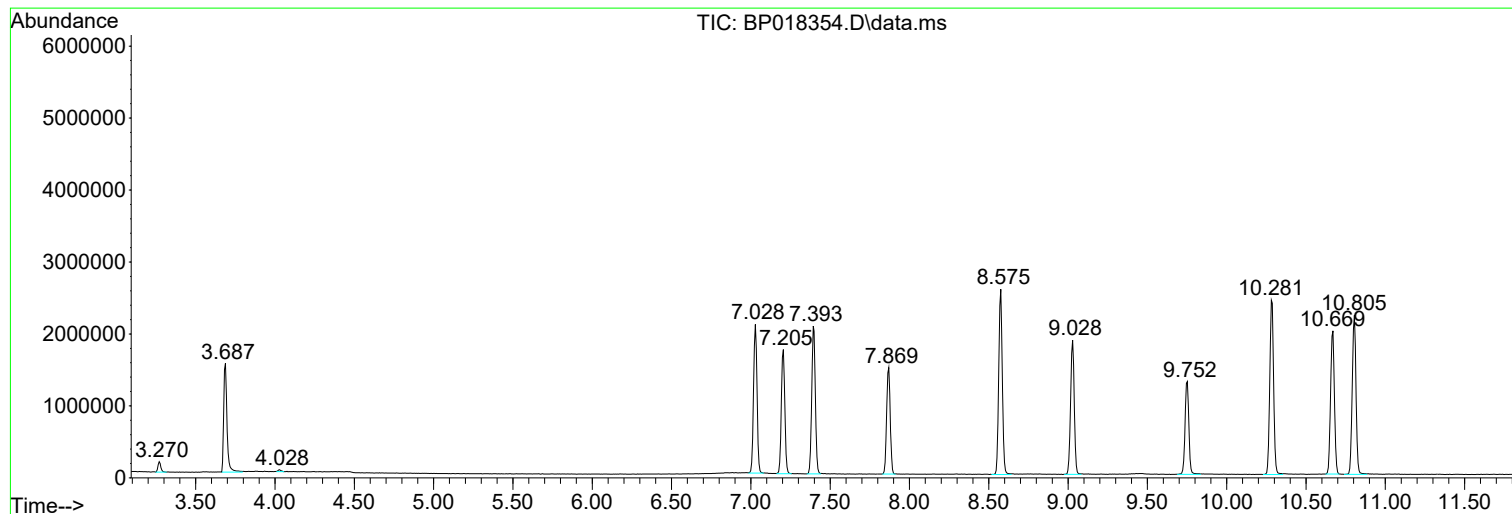

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018354.D
Acq On : 25 Nov 2023 06:53
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018354.D
Acq On : 25 Nov 2023 06:53
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc