

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018370.D
 Acq On : 25 Nov 2023 16:28
 Operator : MA/JU
 Sample : PB157275BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	38	rVB	138713	183550	2.17%	0.184%
2	3.687	98	102	116	rBV	1719168	2364821	28.02%	2.371%
3	4.028	157	160	167	rVB	35486	48661	0.58%	0.049%
4	6.581	588	594	596	rBV7	4690	10676	0.13%	0.011%
5	6.752	618	623	624	rBV5	6720	10680	0.13%	0.011%
6	7.028	663	670	681	rVB	1873045	2879096	34.11%	2.887%
7	7.199	693	699	711	rVB	1536268	2432471	28.82%	2.439%
8	7.393	724	732	741	rBV	1944005	3028438	35.88%	3.037%
9	7.458	741	743	748	rVB6	7066	9165	0.11%	0.009%
10	7.864	804	812	825	rVB	2052503	3257565	38.60%	3.267%
11	8.575	926	933	944	rBV	2278426	3625149	42.95%	3.635%
12	9.028	1002	1010	1017	rBV	1673784	2722296	32.26%	2.730%
13	9.746	1119	1132	1142	rBV	1257366	2079766	24.64%	2.086%
14	10.281	1216	1223	1236	rBV	2191302	3593565	42.58%	3.604%
15	10.663	1280	1288	1297	rVB	2629369	4448310	52.71%	4.461%
16	10.805	1304	1312	1322	rBV	2111448	3584072	42.47%	3.594%
17	11.963	1508	1509	1515	rVB6	8756	10325	0.12%	0.010%
18	12.252	1553	1558	1564	rVV2	45724	73417	0.87%	0.074%
19	12.422	1582	1587	1589	rBV6	5493	10077	0.12%	0.010%
20	13.299	1732	1736	1741	rBV8	5691	9492	0.11%	0.010%
21	13.410	1749	1755	1760	rBV	36878	60109	0.71%	0.060%
22	13.463	1760	1764	1773	rVB9	8543	17698	0.21%	0.018%
23	13.916	1834	1841	1851	rBV	3323552	4601912	54.53%	4.615%
24	14.193	1880	1888	1896	rBV	4036309	6051120	71.70%	6.068%
25	14.498	1933	1940	1951	rVB	3615569	5289094	62.67%	5.304%
26	14.687	1964	1972	1983	rBV	1079443	1589002	18.83%	1.593%
27	14.916	2006	2011	2016	rVB9	9490	17305	0.21%	0.017%
28	15.310	2073	2078	2081	rBV7	7667	12024	0.14%	0.012%
29	15.493	2102	2109	2116	rBV	4688584	6828208	80.91%	6.847%
30	15.598	2121	2127	2138	rBV	741890	1093982	12.96%	1.097%
31	15.728	2145	2149	2155	rBV2	22339	33160	0.39%	0.033%
32	16.751	2318	2323	2328	rBV8	5880	10393	0.12%	0.010%
33	16.928	2349	2353	2357	rBV7	8583	15876	0.19%	0.016%
34	17.034	2366	2371	2374	rBV4	7761	11991	0.14%	0.012%
35	17.122	2382	2386	2392	rBV9	8341	19063	0.23%	0.019%
36	17.245	2401	2407	2414	rBV	3632126	5109894	60.55%	5.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018370.D
 Acq On : 25 Nov 2023 16:28
 Operator : MA/JU
 Sample : PB157275BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK275

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.345	2417	2424	2438	rVB	4592014	6417571	76.04%	6.435%
38	18.151	2557	2561	2564	rBV6	12405	22456	0.27%	0.023%
39	18.745	2658	2662	2669	rBV10	8898	19103	0.23%	0.019%
40	19.163	2729	2733	2738	rBV2	58805	80032	0.95%	0.080%
41	19.228	2740	2744	2749	rBV	55995	78912	0.94%	0.079%
42	19.586	2799	2805	2812	rBV	5556600	7239901	85.79%	7.260%
43	21.357	3101	3106	3112	rBV	4565274	5726023	67.85%	5.742%
44	23.639	3486	3494	3504	rVB2	4228538	8439460	100.00%	8.463%
45	23.798	3513	3521	3529	rBV	3237682	6556543	77.69%	6.575%




Sum of corrected areas: 99722424

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018370.D
Acq On : 25 Nov 2023 16:28
Operator : MA/JU
Sample : PB157275BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

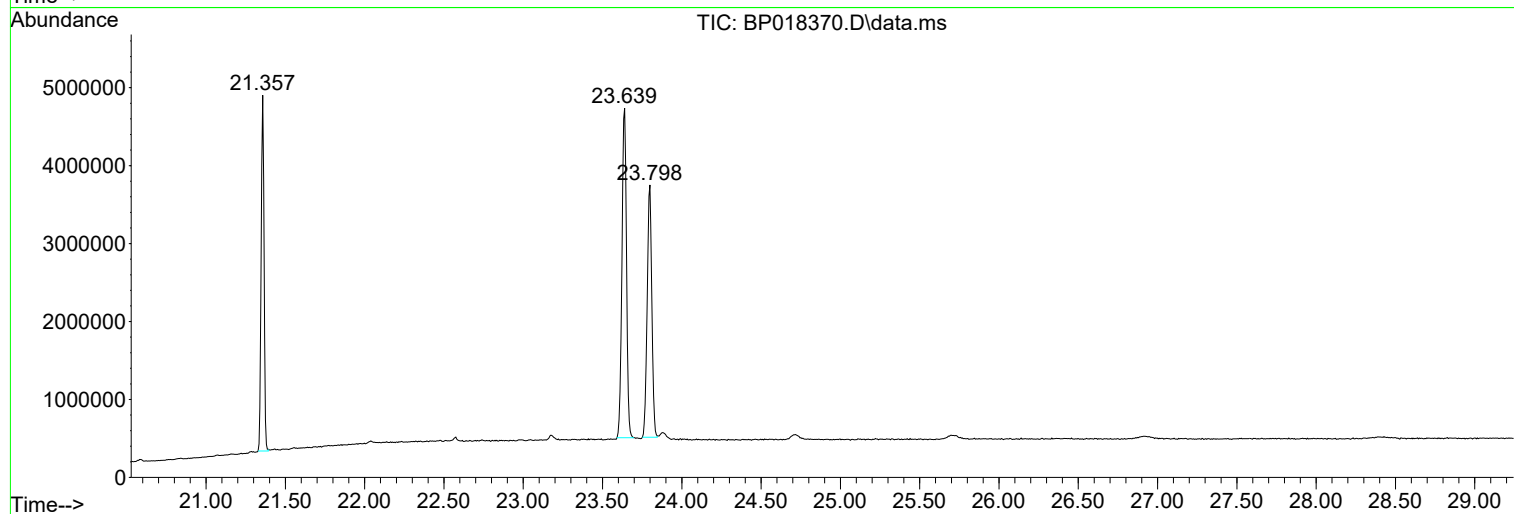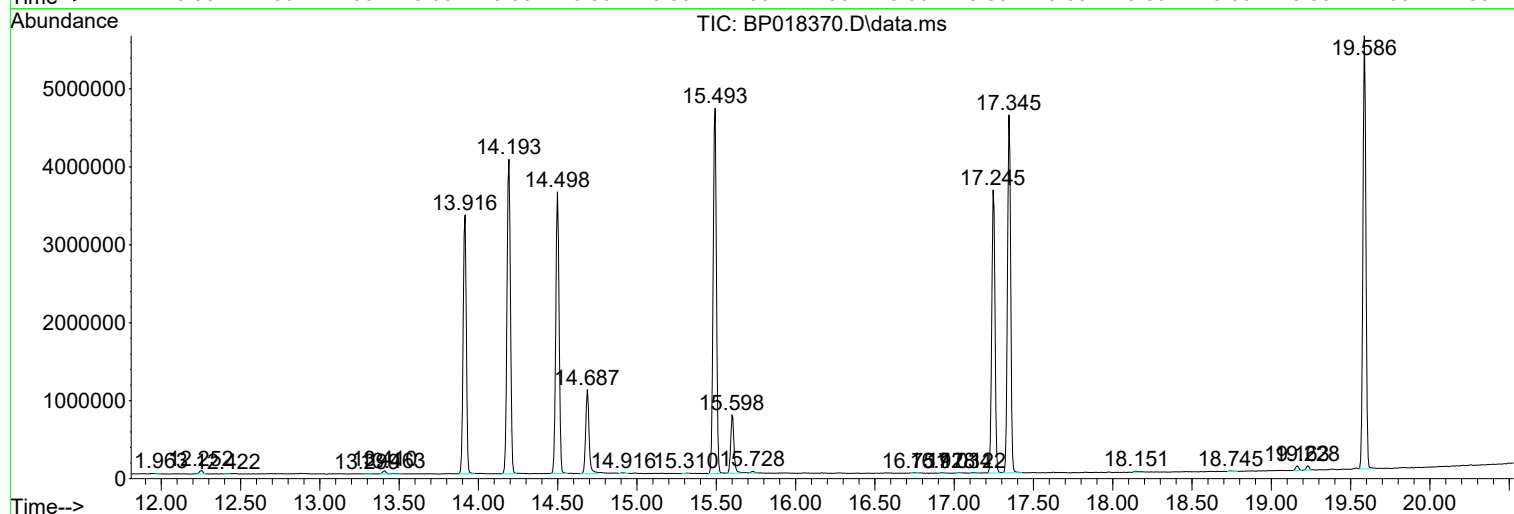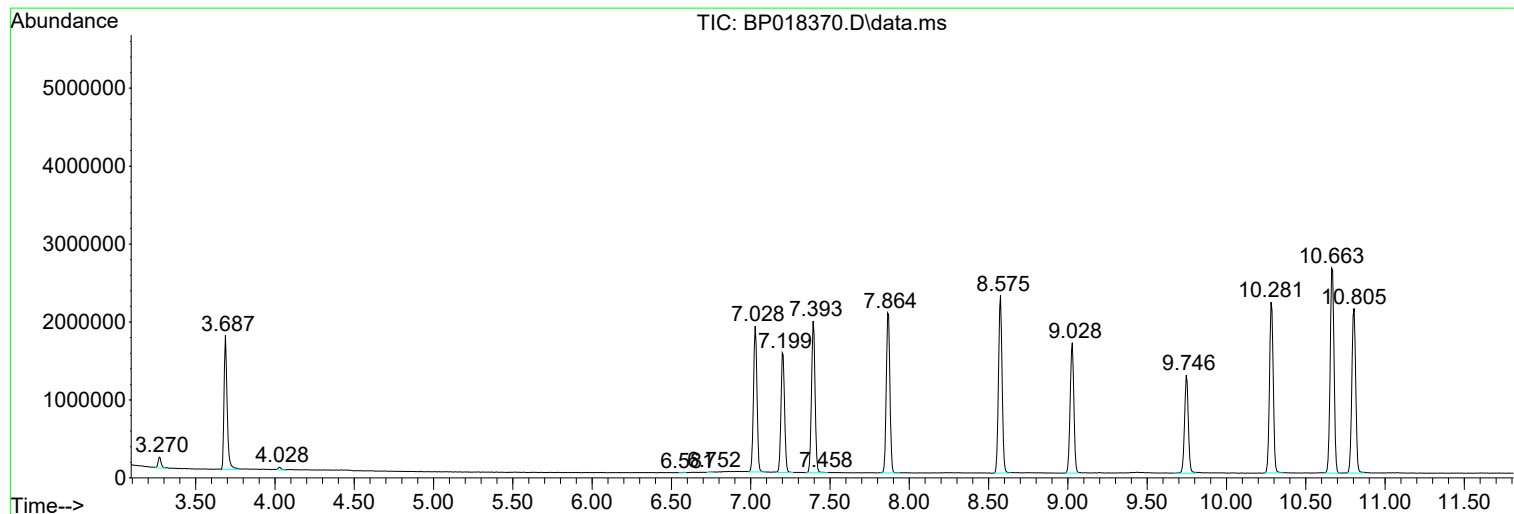

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018370.D
Acq On : 25 Nov 2023 16:28
Operator : MA/JU
Sample : PB157275BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018370.D
Acq On : 25 Nov 2023 16:28
Operator : MA/JU
Sample : PB157275BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------