

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018371.D
 Acq On : 25 Nov 2023 17:01
 Operator : MA/JU
 Sample : PB157191BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK191

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	40	rVB	133368	184057	2.21%	0.190%
2	3.687	97	102	120	rBV	1671518	2354616	28.23%	2.427%
3	4.028	156	160	169	rVB	28574	41231	0.49%	0.042%
4	7.028	663	670	685	rVB	1895626	2928299	35.11%	3.018%
5	7.199	693	699	709	rVB	1571933	2448210	29.36%	2.523%
6	7.393	725	732	740	rBV	1944805	3049339	36.57%	3.143%
7	7.869	805	813	820	rVB	1811248	2887184	34.62%	2.975%
8	8.575	925	933	941	rBV	2358154	3654488	43.82%	3.766%
9	9.028	999	1010	1022	rBV	1699351	2770018	33.22%	2.855%
10	9.746	1119	1132	1143	rBV	1252370	2080416	24.95%	2.144%
11	10.281	1216	1223	1239	rBV	2171706	3704871	44.43%	3.818%
12	10.663	1281	1288	1297	rVB	2351840	3989800	47.84%	4.112%
13	10.804	1304	1312	1325	rBV	2158760	3678328	44.11%	3.791%
14	11.951	1502	1507	1509	rBV6	7947	8873	0.11%	0.009%
15	12.251	1553	1558	1565	rVB2	44233	72401	0.87%	0.075%
16	12.881	1660	1665	1669	rBV7	8083	15883	0.19%	0.016%
17	13.292	1731	1735	1740	rVB8	6539	8405	0.10%	0.009%
18	13.404	1748	1754	1761	rBV2	43880	72283	0.87%	0.074%
19	13.475	1761	1766	1771	rVB9	9190	19410	0.23%	0.020%
20	13.916	1833	1841	1849	rBV	3486419	4754091	57.01%	4.899%
21	14.192	1879	1888	1895	rBV	4070157	6214569	74.52%	6.404%
22	14.498	1933	1940	1949	rBV	3285745	4816526	57.76%	4.964%
23	14.686	1964	1972	1992	rBV	1040788	1593613	19.11%	1.642%
24	14.910	2008	2010	2015	rVB6	9913	13097	0.16%	0.013%
25	15.492	2100	2109	2116	rBV	4789419	7019218	84.17%	7.234%
26	15.598	2121	2127	2137	rBV	756225	1093909	13.12%	1.127%
27	15.728	2144	2149	2157	rVB3	26072	44041	0.53%	0.045%
28	16.057	2203	2205	2209	rVB5	8519	10343	0.12%	0.011%
29	16.275	2238	2242	2246	rVB7	9000	14295	0.17%	0.015%
30	16.751	2319	2323	2328	rBV8	9667	16751	0.20%	0.017%
31	17.033	2368	2371	2374	rBV2	6762	9305	0.11%	0.010%
32	17.245	2400	2407	2414	rBV	3388458	4641826	55.66%	4.784%
33	17.345	2417	2424	2434	rVV	4657505	6525324	78.25%	6.725%
34	17.622	2465	2471	2473	rBV6	9440	14753	0.18%	0.015%
35	18.145	2557	2560	2565	rBV6	11079	23487	0.28%	0.024%
36	19.163	2728	2733	2738	rBV2	60103	86152	1.03%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018371.D
Acq On : 25 Nov 2023 17:01
Operator : MA/JU
Sample : PB157191BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK191

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.227	2740	2744	2749	rBV2	56649	84415	1.01%	0.087%
38	19.586	2799	2805	2814	rBV	5639474	7142868	85.65%	7.361%
39	21.351	3100	3105	3112	rBV	3748823	4982594	59.75%	5.135%
40	23.633	3485	3493	3504	rBV2	4225939	8339460	100.00%	8.594%
41	23.792	3513	3520	3530	rVB	2754663	5626289	67.47%	5.798%




Sum of corrected areas: 97035038

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018371.D
Acq On : 25 Nov 2023 17:01
Operator : MA/JU
Sample : PB157191BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK191

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

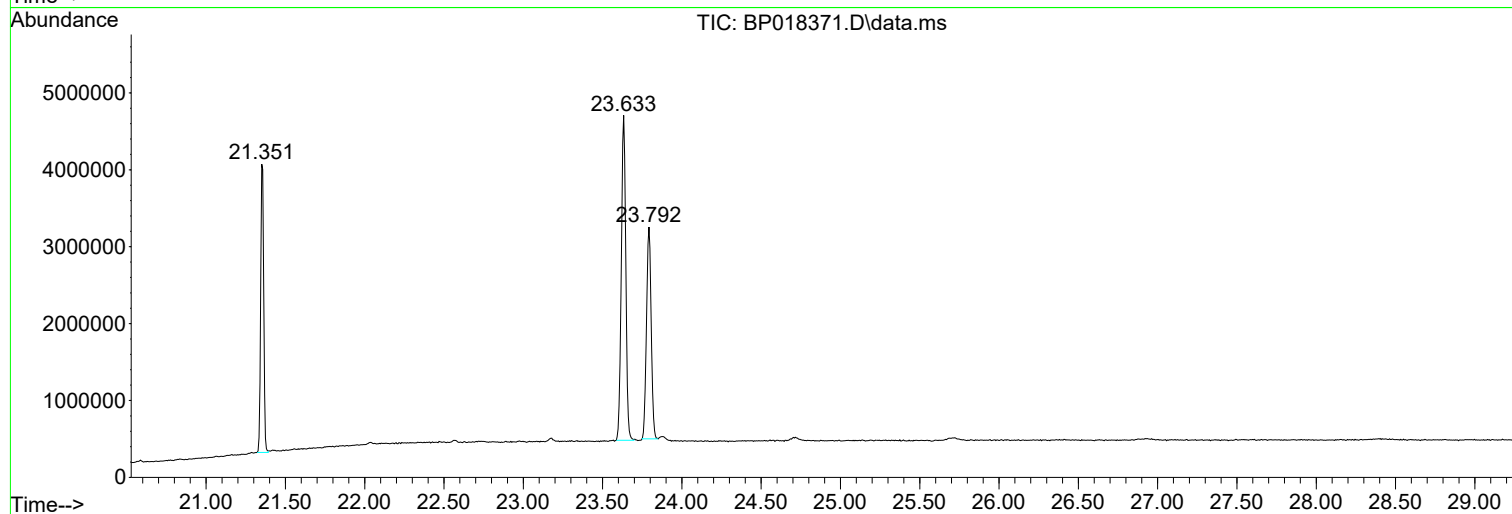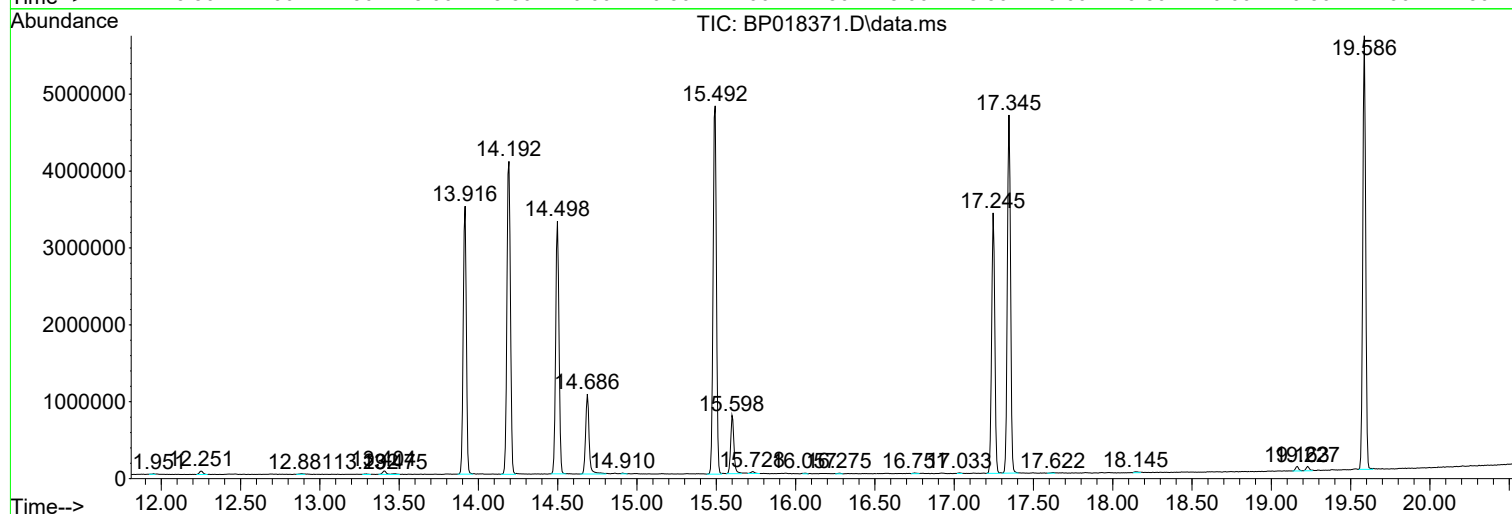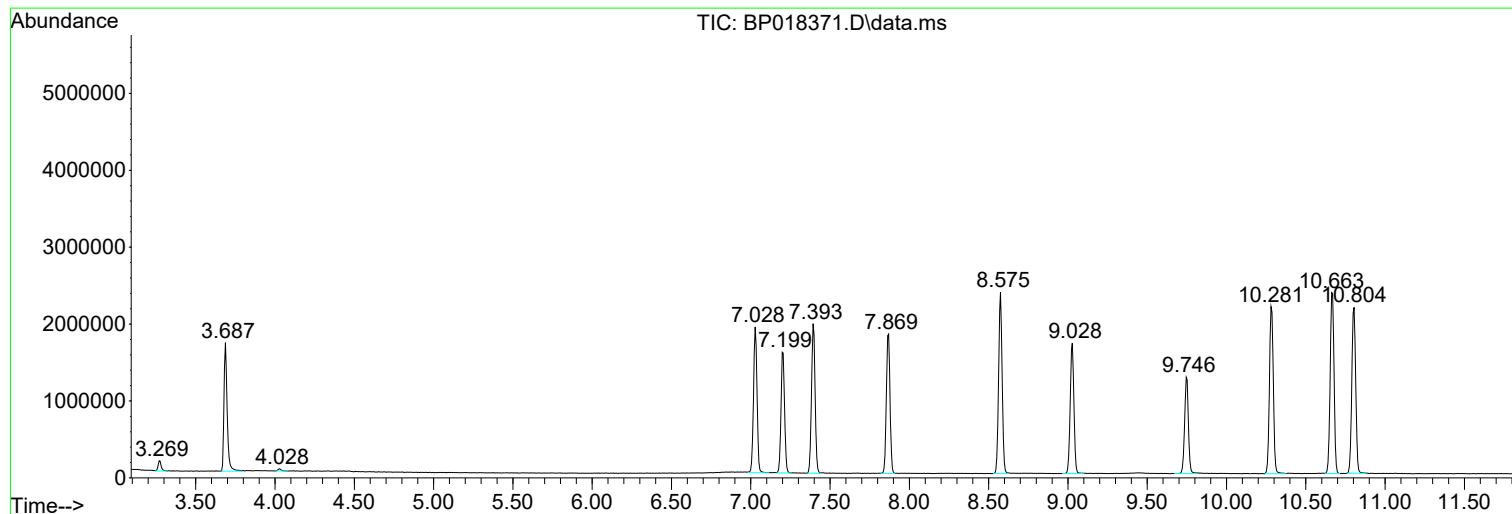

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018371.D
Acq On : 25 Nov 2023 17:01
Operator : MA/JU
Sample : PB157191BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK191

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018371.D
Acq On : 25 Nov 2023 17:01
Operator : MA/JU
Sample : PB157191BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK191

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------