

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018372.D
 Acq On : 25 Nov 2023 17:35
 Operator : MA/JU
 Sample : 05336-12
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	37	rBV	83087	106828	1.21%	0.118%
2	3.687	99	102	111	rBV	376698	536363	6.08%	0.595%
3	3.934	141	144	148	rVB2	19945	28008	0.32%	0.031%
4	4.023	156	159	164	rVB	25614	34119	0.39%	0.038%
5	5.140	344	349	354	rVB3	14829	21652	0.25%	0.024%
6	6.840	632	638	641	rBV6	7890	14981	0.17%	0.017%
7	7.028	663	670	682	rVB	317403	512320	5.81%	0.568%
8	7.199	691	699	708	rVB	1328618	2056081	23.31%	2.280%
9	7.393	724	732	739	rBV	1243819	1926943	21.85%	2.137%
10	7.863	805	812	819	rBV	1739278	2782852	31.55%	3.086%
11	7.928	819	823	832	rVB9	8104	21182	0.24%	0.023%
12	8.569	925	932	942	rBV	941490	1518770	17.22%	1.684%
13	9.028	1002	1010	1020	rBV	1455905	2382756	27.02%	2.642%
14	9.199	1035	1039	1042	rBV5	6854	8902	0.10%	0.010%
15	9.463	1079	1084	1090	rVB2	29163	52976	0.60%	0.059%
16	9.746	1123	1132	1143	rBV	1029904	1686988	19.13%	1.871%
17	10.281	1216	1223	1233	rBV	1770280	2905211	32.94%	3.221%
18	10.663	1280	1288	1296	rBV	2353140	3987634	45.21%	4.421%
19	10.799	1303	1311	1326	rBV	1554533	2644194	29.98%	2.932%
20	11.475	1419	1426	1430	rVB8	12566	27206	0.31%	0.030%
21	11.957	1503	1508	1515	rVB2	41883	67569	0.77%	0.075%
22	12.252	1551	1558	1565	rVB	40243	66005	0.75%	0.073%
23	12.693	1627	1633	1636	rVB8	5238	10377	0.12%	0.012%
24	12.875	1657	1664	1665	rBV7	8416	12492	0.14%	0.014%
25	12.893	1665	1667	1674	rVB8	10028	19418	0.22%	0.022%
26	13.122	1704	1706	1711	rVB5	7471	9894	0.11%	0.011%
27	13.340	1739	1743	1747	rVB3	18655	27109	0.31%	0.030%
28	13.404	1749	1754	1761	rVB4	36096	63610	0.72%	0.071%
29	13.469	1761	1765	1770	rVB7	7977	13537	0.15%	0.015%
30	13.810	1814	1823	1825	rBV10	8708	18034	0.20%	0.020%
31	13.916	1834	1841	1856	rBV	3534529	4902254	55.58%	5.436%
32	14.193	1877	1888	1899	rBV	3943937	5929459	67.23%	6.575%
33	14.498	1933	1940	1948	rVV	3520021	5132189	58.19%	5.691%
34	14.687	1966	1972	1979	rBV	179567	288266	3.27%	0.320%
35	14.769	1983	1986	1991	rVB7	8541	15809	0.18%	0.018%
36	14.822	1991	1995	1997	rBV5	8807	13587	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018372.D
 Acq On : 25 Nov 2023 17:35
 Operator : MA/JU
 Sample : 05336-12
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.893	2003	2007	2015	rBV2	23803	53090	0.60%	0.059%
38	15.040	2028	2032	2036	rVB5	11657	14806	0.17%	0.016%
39	15.110	2039	2044	2047	rBV7	7231	12492	0.14%	0.014%
40	15.157	2048	2052	2057	rVB7	13535	21200	0.24%	0.024%
41	15.240	2063	2066	2070	rVB2	9268	12013	0.14%	0.013%
42	15.316	2075	2079	2084	rVV5	8866	13848	0.16%	0.015%
43	15.493	2102	2109	2122	rBV	5133521	7568126	85.81%	8.392%
44	15.604	2122	2128	2139	rVV	930941	1362163	15.44%	1.510%
45	15.728	2146	2149	2157	rVB2	28325	45768	0.52%	0.051%
46	15.928	2174	2183	2186	rBV9	7319	18528	0.21%	0.021%
47	16.269	2239	2241	2248	rVB8	9351	11761	0.13%	0.013%
48	16.504	2277	2281	2286	rBV5	12197	18602	0.21%	0.021%
49	16.716	2313	2317	2320	rBV5	5568	9945	0.11%	0.011%
50	16.751	2320	2323	2327	rVB6	9389	14789	0.17%	0.016%
51	16.892	2343	2347	2351	rBV2	31341	47527	0.54%	0.053%
52	17.028	2365	2370	2374	rBV5	11753	23078	0.26%	0.026%
53	17.122	2382	2386	2390	rBV7	8341	15653	0.18%	0.017%
54	17.245	2400	2407	2417	rBV	3704420	5232737	59.33%	5.802%
55	17.345	2417	2424	2436	rVV2	5677259	8063360	91.42%	8.941%
56	17.622	2469	2471	2473	rBV2	10849	13147	0.15%	0.015%
57	17.651	2473	2476	2480	rVB	23620	31776	0.36%	0.035%
58	17.922	2519	2522	2525	rVB4	15424	15596	0.18%	0.017%
59	18.139	2555	2559	2567	rBV2	120491	179919	2.04%	0.199%
60	19.163	2729	2733	2738	rVB	72687	96081	1.09%	0.107%
61	19.228	2740	2744	2748	rBV	70527	97292	1.10%	0.108%
62	19.381	2767	2770	2777	rBV3	85234	103760	1.18%	0.115%
63	19.586	2799	2805	2812	rBV	6324810	8402672	95.27%	9.317%
64	21.351	3100	3105	3114	rBV	3793676	4781166	54.21%	5.301%
65	23.633	3485	3493	3507	rVB2	4343148	8820103	100.00%	9.780%
66	23.792	3513	3520	3529	rBV	2573707	5240858	59.42%	5.811%




Sum of corrected areas: 90187431

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018372.D
Acq On : 25 Nov 2023 17:35
Operator : MA/JU
Sample : 05336-12
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

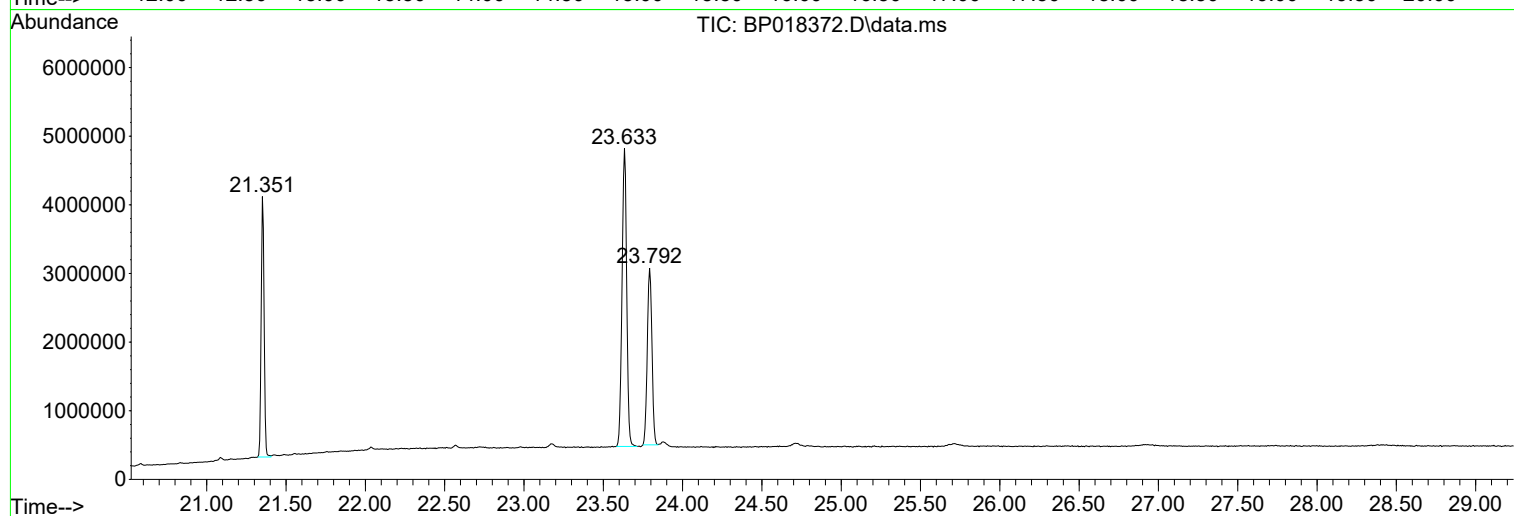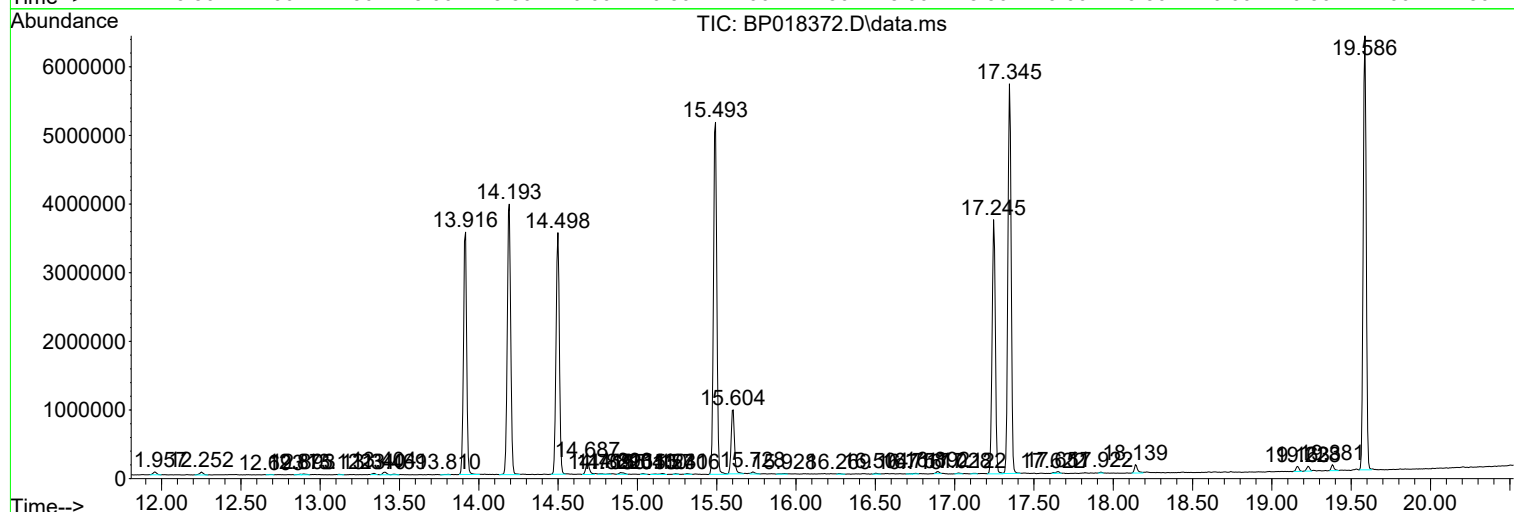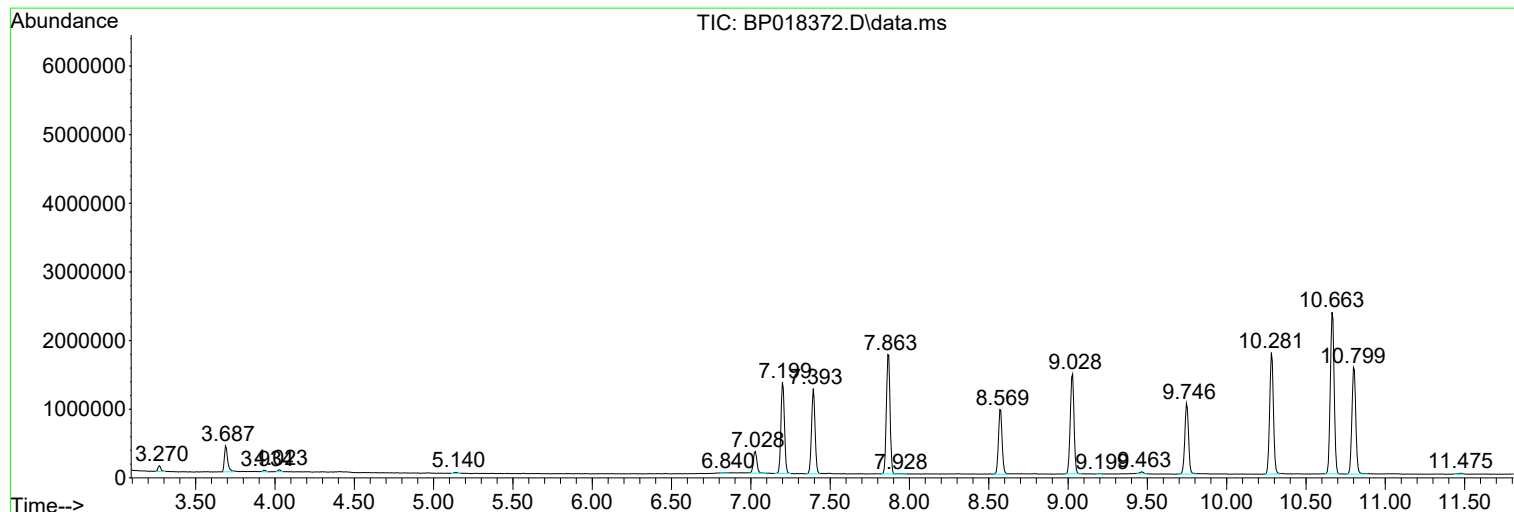

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018372.D
Acq On : 25 Nov 2023 17:35
Operator : MA/JU
Sample : 05336-12
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018372.D
Acq On : 25 Nov 2023 17:35
Operator : MA/JU
Sample : 05336-12
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------