

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018373.D
 Acq On : 25 Nov 2023 18:09
 Operator : MA/JU
 Sample : 05336-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	38	rVB	92452	120594	1.10%	0.109%
2	3.564	77	81	85	rBV3	13513	23241	0.21%	0.021%
3	3.687	98	102	113	rBV	512784	743452	6.81%	0.670%
4	3.934	140	144	148	rVB	22476	33647	0.31%	0.030%
5	4.022	156	159	165	rVB	24355	33459	0.31%	0.030%
6	5.140	343	349	353	rBV4	13827	25101	0.23%	0.023%
7	6.869	641	643	649	rVB6	8433	13997	0.13%	0.013%
8	7.028	663	670	679	rVB	388828	608849	5.57%	0.549%
9	7.199	692	699	707	rBV	1610131	2476908	22.68%	2.233%
10	7.393	725	732	742	rBV	1544404	2440518	22.35%	2.200%
11	7.499	747	750	757	rVB9	9711	14507	0.13%	0.013%
12	7.811	798	803	806	rBV	44403	70162	0.64%	0.063%
13	7.863	806	812	820	rVV	1960343	3110320	28.48%	2.804%
14	7.934	822	824	829	rVB6	11076	14426	0.13%	0.013%
15	8.569	925	932	941	rBV	1043480	1671663	15.31%	1.507%
16	9.022	1000	1009	1020	rBV	1793505	2996372	27.44%	2.701%
17	9.199	1035	1039	1045	rVB9	7476	11709	0.11%	0.011%
18	9.463	1077	1084	1095	rVB3	27619	74950	0.69%	0.068%
19	9.746	1120	1132	1146	rBV	1340440	2210247	20.24%	1.992%
20	9.875	1149	1154	1160	rVB2	13925	28206	0.26%	0.025%
21	9.975	1167	1171	1176	rBV	29158	49358	0.45%	0.044%
22	10.028	1176	1180	1186	rVB9	10997	21220	0.19%	0.019%
23	10.281	1214	1223	1235	rBV	2263859	3746358	34.30%	3.377%
24	10.663	1280	1288	1297	rVB	2757573	4596202	42.08%	4.143%
25	10.799	1304	1311	1320	rBV	1856989	3158702	28.92%	2.847%
26	11.063	1353	1356	1362	rVB8	8006	14499	0.13%	0.013%
27	11.457	1417	1423	1432	rBV5	55730	132328	1.21%	0.119%
28	11.957	1503	1508	1516	rBV3	33423	67663	0.62%	0.061%
29	12.251	1552	1558	1564	rVB2	50159	84890	0.78%	0.077%
30	12.775	1642	1647	1650	rBV6	14344	20276	0.19%	0.018%
31	12.887	1661	1666	1673	rBV6	8883	25913	0.24%	0.023%
32	13.281	1727	1733	1738	rVB10	5337	11350	0.10%	0.010%
33	13.404	1749	1754	1759	rBV	54793	90907	0.83%	0.082%
34	13.469	1761	1765	1772	rVB10	10503	22729	0.21%	0.020%
35	13.710	1804	1806	1811	rVB6	10699	11715	0.11%	0.011%
36	13.916	1834	1841	1852	rBV	4491971	6387966	58.49%	5.758%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018373.D
 Acq On : 25 Nov 2023 18:09
 Operator : MA/JU
 Sample : 05336-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.193	1877	1888	1898	rBV	5082194	7749483	70.96%	6.985%
38	14.498	1929	1940	1949	rBV	4158893	6264504	57.36%	5.647%
39	14.687	1966	1972	1979	rVV	237011	362040	3.31%	0.326%
40	14.916	2005	2011	2015	rVB9	20015	36259	0.33%	0.033%
41	15.157	2049	2052	2056	rVB6	11103	14940	0.14%	0.013%
42	15.316	2074	2079	2083	rBV5	10376	19947	0.18%	0.018%
43	15.357	2083	2086	2089	rVB4	16978	19620	0.18%	0.018%
44	15.492	2102	2109	2121	rBV	6850219	9826073	89.97%	8.857%
45	15.598	2121	2127	2139	rBV	1276957	1849722	16.94%	1.667%
46	15.728	2145	2149	2155	rVB	32802	49899	0.46%	0.045%
47	16.181	2221	2226	2230	rBV7	11371	25130	0.23%	0.023%
48	16.222	2230	2233	2238	rBV	36245	45083	0.41%	0.041%
49	16.745	2316	2322	2326	rBV9	12033	26560	0.24%	0.024%
50	16.792	2326	2330	2335	rVB3	29678	42559	0.39%	0.038%
51	16.922	2349	2352	2358	rVB8	12717	19337	0.18%	0.017%
52	17.022	2365	2369	2373	rBV2	57389	71744	0.66%	0.065%
53	17.075	2374	2378	2382	rVB5	13255	18446	0.17%	0.017%
54	17.128	2382	2387	2391	rBV4	16466	25755	0.24%	0.023%
55	17.245	2400	2407	2414	rBV	4936741	6871839	62.92%	6.194%
56	17.345	2417	2424	2435	rVV	7320141	10195329	93.35%	9.190%
57	17.486	2446	2448	2455	rVB4	10990	16434	0.15%	0.015%
58	17.628	2468	2472	2476	rBV3	11572	18768	0.17%	0.017%
59	17.692	2478	2483	2487	rBV4	18787	27359	0.25%	0.025%
60	17.763	2491	2495	2499	rBV	48154	54979	0.50%	0.050%
61	17.828	2503	2506	2510	rVB6	9080	13837	0.13%	0.012%
62	17.928	2519	2523	2528	rVB2	45801	67604	0.62%	0.061%
63	18.139	2555	2559	2563	rBV	100334	138532	1.27%	0.125%
64	18.439	2606	2610	2617	rBV3	40979	60676	0.56%	0.055%
65	18.598	2633	2637	2641	rBV4	24622	32121	0.29%	0.029%
66	19.051	2711	2714	2719	rVB3	29333	39046	0.36%	0.035%
67	19.163	2728	2733	2737	rBV	103330	138768	1.27%	0.125%
68	19.228	2740	2744	2748	rVB	84427	110668	1.01%	0.100%
69	19.380	2766	2770	2777	rBV3	90674	123444	1.13%	0.111%
70	19.533	2793	2796	2799	rVB5	21366	23501	0.22%	0.021%
71	19.586	2799	2805	2818	rBV	8121206	10921501	100.00%	9.844%
72	21.351	3100	3105	3112	rBV	4461645	5658991	51.82%	5.101%
73	23.633	3485	3493	3503	rBV	4495409	9084050	83.18%	8.188%
74	23.792	3513	3520	3529	rVB	2774250	5715174	52.33%	5.151%

Sum of corrected areas: 110944126




Instrument :
BNA_P
ClientSampleId :
DCKE2

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018373.D
Acq On : 25 Nov 2023 18:09
Operator : MA/JU
Sample : 05336-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

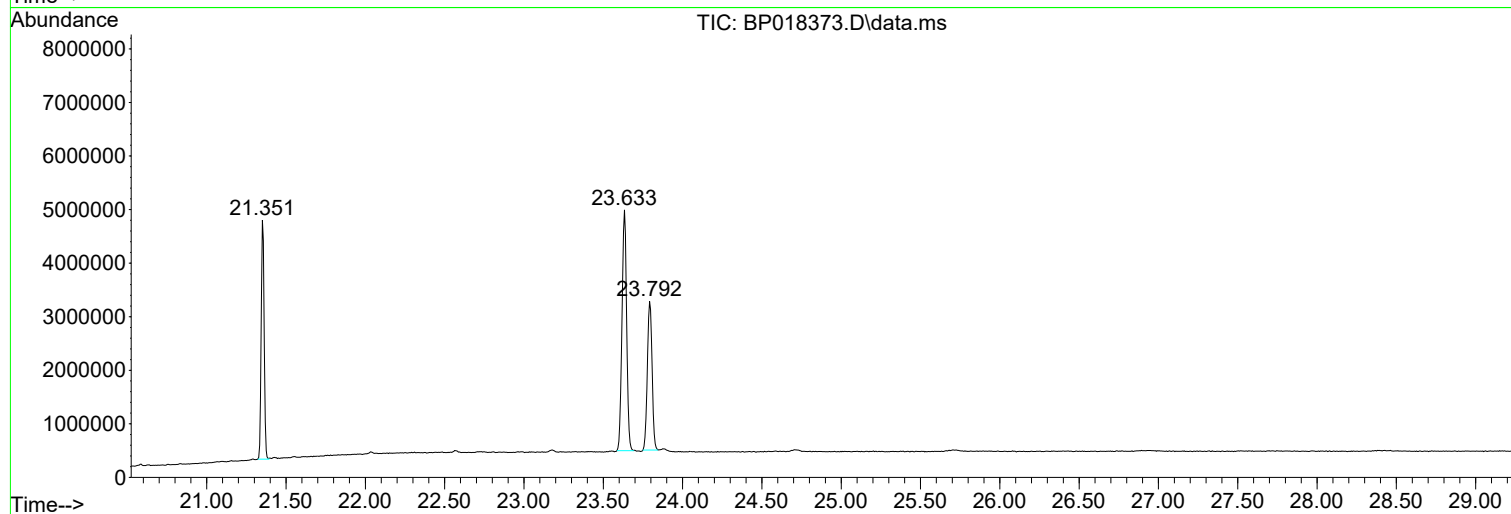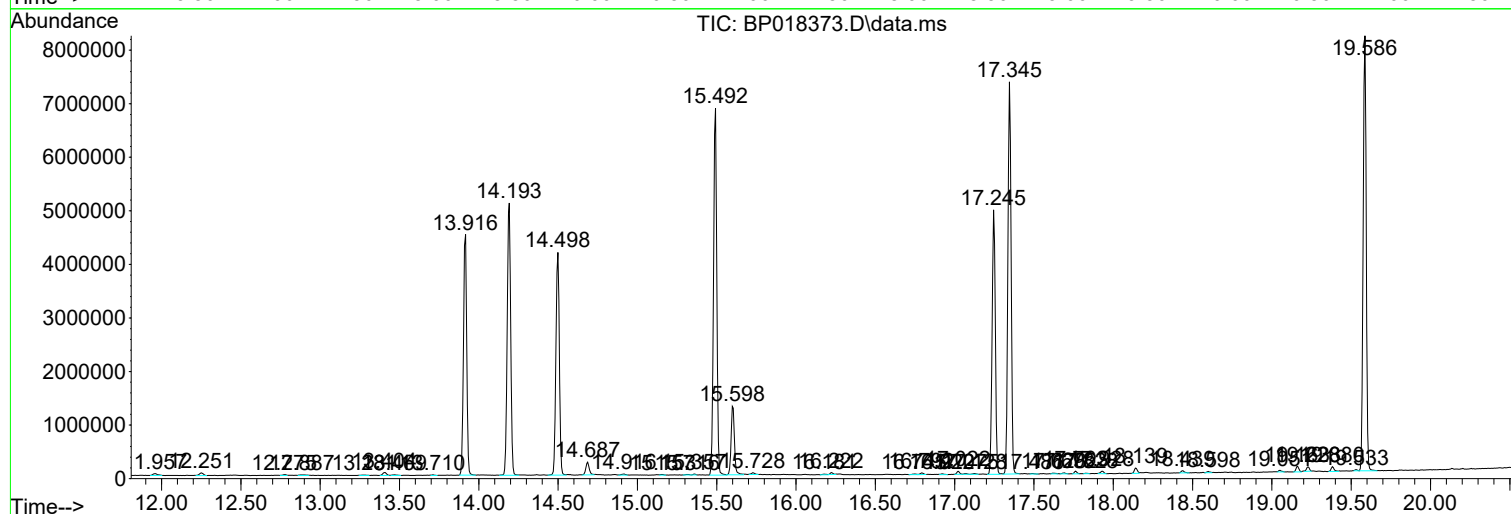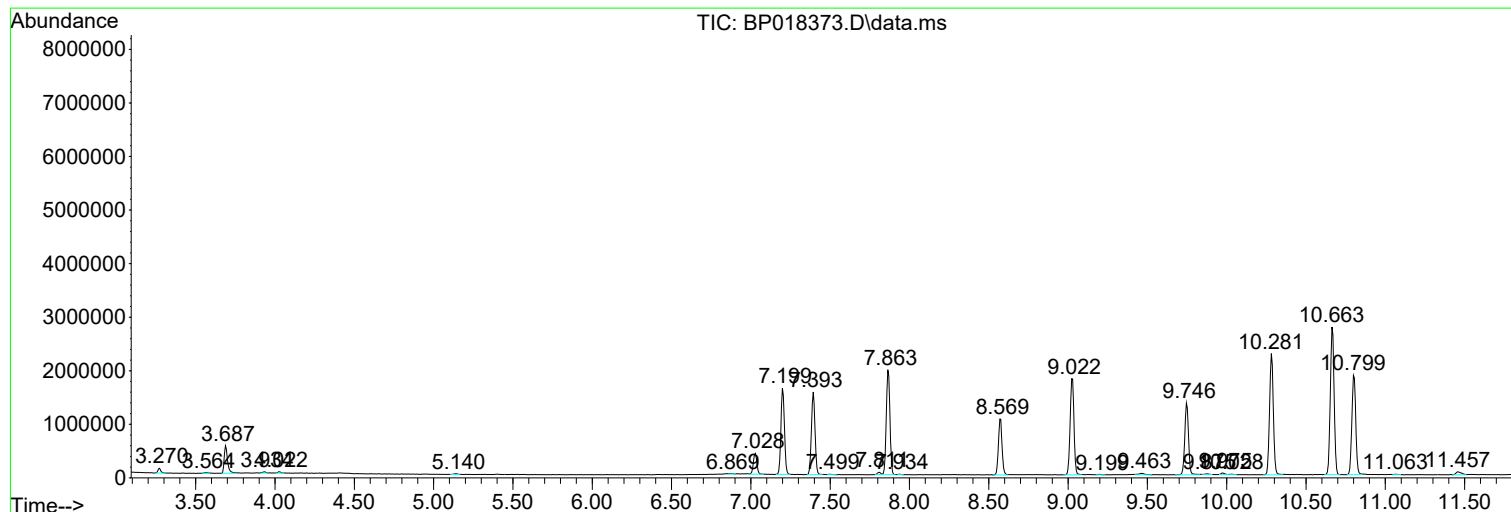

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018373.D
Acq On : 25 Nov 2023 18:09
Operator : MA/JU
Sample : 05336-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018373.D
Acq On : 25 Nov 2023 18:09
Operator : MA/JU
Sample : 05336-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc