

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018375.D
 Acq On : 25 Nov 2023 19:16
 Operator : MA/JU
 Sample : 05336-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	95384	126808	1.43%	0.147%
2	3.558	78	80	85	rVB2	23670	34706	0.39%	0.040%
3	3.687	98	102	113	rBV	488729	698807	7.91%	0.812%
4	3.940	141	145	150	rVB3	20992	34114	0.39%	0.040%
5	4.028	156	160	165	rVB	28322	42332	0.48%	0.049%
6	4.969	317	320	324	rVB5	7369	11185	0.13%	0.013%
7	6.840	636	638	644	rBV6	7648	9716	0.11%	0.011%
8	7.028	664	670	680	rVB	329183	527834	5.97%	0.614%
9	7.199	692	699	712	rVB	1413917	2190495	24.78%	2.546%
10	7.393	725	732	740	rBV	1264368	1942064	21.97%	2.257%
11	7.493	743	749	756	rVB	9584	22400	0.25%	0.026%
12	7.863	805	812	821	rBV	1838079	2882488	32.61%	3.350%
13	7.940	821	825	828	rVB4	6388	9909	0.11%	0.012%
14	8.569	924	932	943	rBV	964974	1549703	17.53%	1.801%
15	9.022	1002	1009	1020	rBV	1498605	2456938	27.80%	2.856%
16	9.463	1074	1084	1089	rBV2	34606	68585	0.78%	0.080%
17	9.746	1122	1132	1141	rBV	1028615	1669001	18.88%	1.940%
18	10.281	1214	1223	1234	rBV	1749923	2894332	32.75%	3.364%
19	10.663	1281	1288	1296	rVB	2403009	3940495	44.58%	4.580%
20	10.799	1304	1311	1326	rBV	1707863	2960494	33.49%	3.441%
21	11.022	1346	1349	1353	rBV6	6372	10893	0.12%	0.013%
22	11.069	1355	1357	1363	rVB7	7135	10781	0.12%	0.013%
23	11.451	1417	1422	1431	rVB7	7992	15813	0.18%	0.018%
24	11.957	1503	1508	1515	rVB	47549	74653	0.84%	0.087%
25	12.251	1551	1558	1566	rVB	36247	61905	0.70%	0.072%
26	12.422	1581	1587	1590	rBV8	4433	9113	0.10%	0.011%
27	12.904	1667	1669	1674	rVB6	6731	9412	0.11%	0.011%
28	13.116	1701	1705	1711	rVB6	11008	16300	0.18%	0.019%
29	13.340	1738	1743	1749	rBV10	7308	15031	0.17%	0.017%
30	13.404	1749	1754	1759	rBV3	15158	21917	0.25%	0.025%
31	13.910	1834	1840	1854	rBV	3281600	4639104	52.49%	5.392%
32	14.187	1877	1887	1898	rBV2	3647201	5667351	64.12%	6.587%
33	14.498	1932	1940	1950	rBV	3186831	4683978	52.99%	5.444%
34	14.575	1950	1953	1958	rVB6	8154	12893	0.15%	0.015%
35	14.687	1966	1972	1979	rBV	147895	246037	2.78%	0.286%
36	14.910	2004	2010	2016	rBV	11666	22930	0.26%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018375.D
 Acq On : 25 Nov 2023 19:16
 Operator : MA/JU
 Sample : 05336-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.151	2047	2051	2055	rVB6	19295	27922	0.32%	0.032%
38	15.316	2073	2079	2084	rBV6	13161	25067	0.28%	0.029%
39	15.486	2101	2108	2120	rBV	4728892	6736723	76.22%	7.830%
40	15.598	2120	2127	2138	rVV	699652	1017459	11.51%	1.183%
41	15.728	2145	2149	2155	rVB3	20370	34740	0.39%	0.040%
42	16.645	2302	2305	2308	rBV5	10661	14358	0.16%	0.017%
43	17.028	2365	2370	2373	rBV6	11524	18813	0.21%	0.022%
44	17.245	2399	2407	2414	rBV	3216631	4453370	50.38%	5.176%
45	17.345	2417	2424	2432	rBV2	4519392	6432389	72.77%	7.477%
46	17.728	2484	2489	2493	rBV	37949	57886	0.65%	0.067%
47	17.922	2519	2522	2528	rVB8	21015	33288	0.38%	0.039%
48	18.145	2555	2560	2566	rBV	160050	232753	2.63%	0.271%
49	18.598	2635	2637	2640	rBV4	14062	14090	0.16%	0.016%
50	19.163	2729	2733	2738	rBV	59090	81116	0.92%	0.094%
51	19.227	2740	2744	2749	rVV	57269	80426	0.91%	0.093%
52	19.380	2767	2770	2777	rBV2	93470	120958	1.37%	0.141%
53	19.586	2799	2805	2812	rBV	5683989	7369702	83.38%	8.566%
54	21.086	3057	3060	3066	rBV6	90847	132000	1.49%	0.153%
55	21.351	3100	3105	3115	rBV	3803771	5037860	57.00%	5.856%
56	23.633	3485	3493	3507	rVB2	4203776	8838889	100.00%	10.274%
57	23.792	3513	3520	3532	rVB	2742343	5683837	64.30%	6.606%




Sum of corrected areas: 86034163

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018375.D
Acq On : 25 Nov 2023 19:16
Operator : MA/JU
Sample : 05336-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

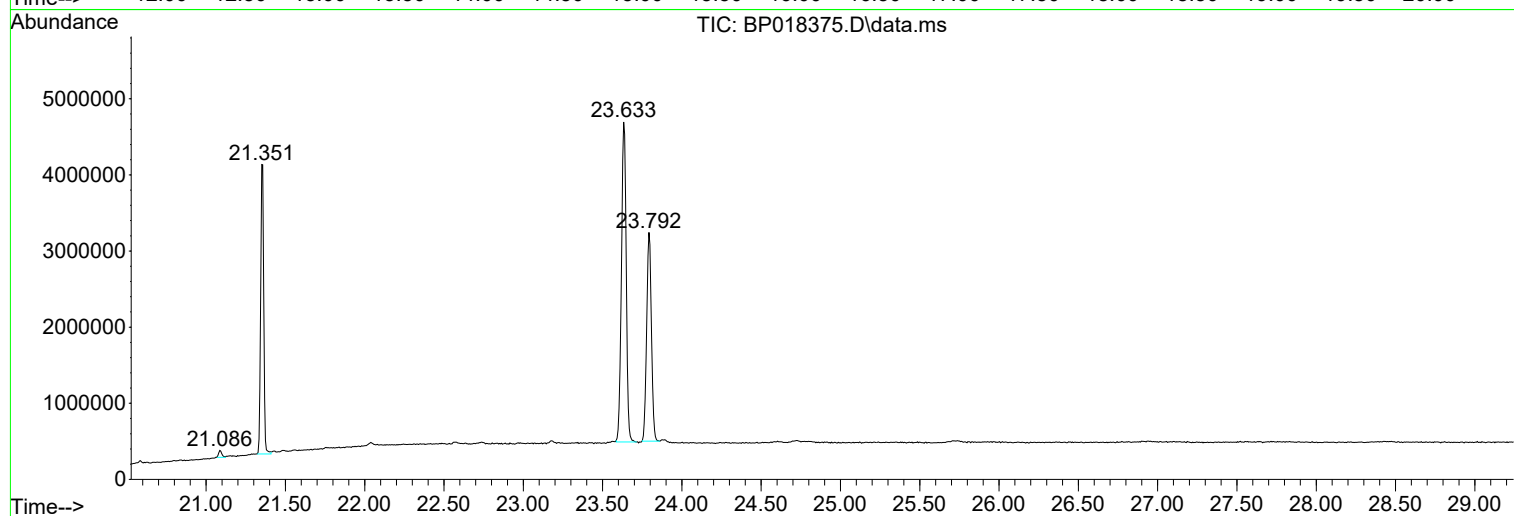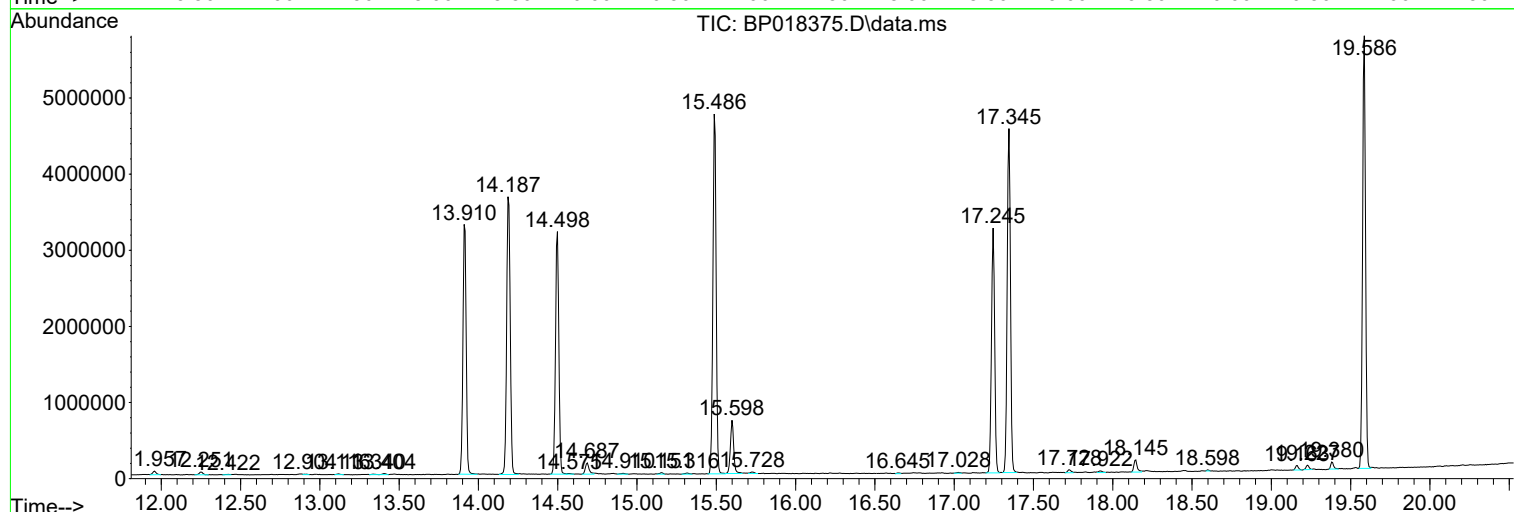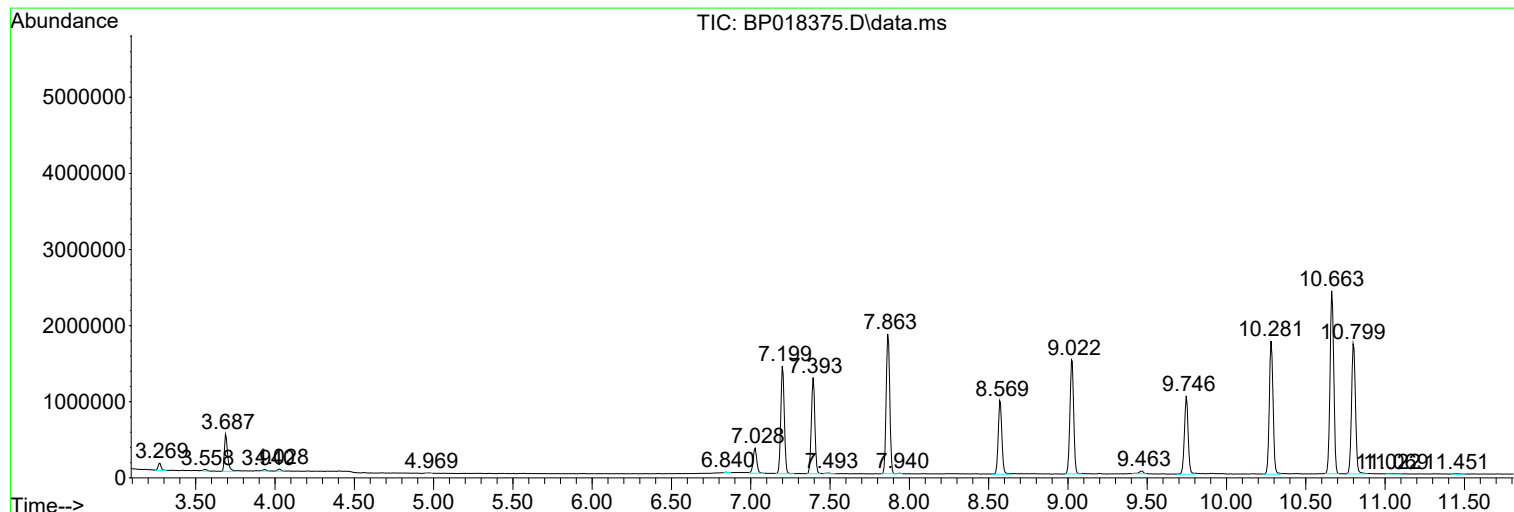

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018375.D
Acq On : 25 Nov 2023 19:16
Operator : MA/JU
Sample : 05336-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018375.D
Acq On : 25 Nov 2023 19:16
Operator : MA/JU
Sample : 05336-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc