

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018376.D
 Acq On : 25 Nov 2023 19:50
 Operator : MA/JU
 Sample : 05336-16
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	36	rVB	87448	108492	1.17%	0.102%
2	3.687	98	102	111	rBV	507582	727081	7.84%	0.680%
3	3.934	140	144	149	rVB2	23883	34506	0.37%	0.032%
4	4.028	156	160	165	rVB	37280	52920	0.57%	0.050%
5	4.564	248	251	256	rVB7	10549	16478	0.18%	0.015%
6	5.134	344	348	354	rBV8	9760	18098	0.20%	0.017%
7	7.028	663	670	681	rVB	399941	632180	6.82%	0.592%
8	7.199	690	699	709	rVB	1635995	2555003	27.55%	2.391%
9	7.393	725	732	743	rBV	1527399	2360347	25.45%	2.209%
10	7.493	743	749	755	rVB	11096	22875	0.25%	0.021%
11	7.863	804	812	820	rBV	1929025	3058652	32.98%	2.862%
12	8.575	921	933	944	rBV	1198954	1922656	20.73%	1.799%
13	8.710	952	956	961	rVB4	14781	24036	0.26%	0.022%
14	8.975	993	1001	1002	rBV8	10559	15588	0.17%	0.015%
15	9.028	1002	1010	1017	rVV	1769421	2943075	31.73%	2.754%
16	9.463	1080	1084	1094	rVB4	29555	57014	0.61%	0.053%
17	9.669	1112	1119	1123	rBV	36416	56580	0.61%	0.053%
18	9.746	1123	1132	1139	rVV	1252807	2068672	22.30%	1.936%
19	9.816	1140	1144	1152	rVB2	36174	60478	0.65%	0.057%
20	9.946	1160	1166	1171	rBV3	13683	22986	0.25%	0.022%
21	10.069	1180	1187	1194	rVB7	12958	27489	0.30%	0.026%
22	10.281	1216	1223	1234	rBV	2195288	3669990	39.57%	3.434%
23	10.410	1241	1245	1249	rVV4	11047	14848	0.16%	0.014%
24	10.581	1268	1274	1278	rBV3	22709	39397	0.42%	0.037%
25	10.663	1281	1288	1296	rVV	2609517	4416386	47.62%	4.133%
26	10.728	1296	1299	1304	rVB7	14120	19278	0.21%	0.018%
27	10.799	1304	1311	1332	rVB2	1904792	3885274	41.89%	3.636%
28	11.052	1350	1354	1360	rVB	40564	68929	0.74%	0.065%
29	11.275	1387	1392	1396	rVB5	13316	18790	0.20%	0.018%
30	11.781	1472	1478	1482	rBV8	9000	20082	0.22%	0.019%
31	12.222	1547	1553	1556	rVV	68605	131483	1.42%	0.123%
32	12.251	1556	1558	1561	rVV	45568	58555	0.63%	0.055%
33	12.281	1561	1563	1568	rVV4	20248	35589	0.38%	0.033%
34	12.328	1568	1571	1575	rVV5	16707	25239	0.27%	0.024%
35	12.440	1584	1590	1594	rVV6	13017	31751	0.34%	0.030%
36	12.516	1598	1603	1612	rVB2	31154	79761	0.86%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018376.D
 Acq On : 25 Nov 2023 19:50
 Operator : MA/JU
 Sample : 05336-16
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	12.646	1619	1625	1627	rBV7	8187	17265	0.19%	0.016%
38	12.687	1627	1632	1636	rVV	49705	74962	0.81%	0.070%
39	12.963	1674	1679	1688	rBV	50736	92775	1.00%	0.087%
40	13.198	1715	1719	1724	rBV	57983	83709	0.90%	0.078%

41	13.340	1738	1743	1749	rVB7	24446	40146	0.43%	0.038%
42	13.404	1749	1754	1761	rBV	35664	62152	0.67%	0.058%
43	13.481	1761	1767	1772	rBV2	39002	66446	0.72%	0.062%
44	13.546	1774	1778	1789	rVB2	42572	73253	0.79%	0.069%
45	13.669	1793	1799	1805	rBV2	11802	30252	0.33%	0.028%

46	13.916	1834	1841	1851	rBV	4177601	6045872	65.18%	5.658%
47	14.193	1874	1888	1898	rBV	4952198	7281294	78.50%	6.814%
48	14.410	1920	1925	1930	rBV	62896	93967	1.01%	0.088%
49	14.498	1930	1940	1946	rVV	3881412	5747301	61.96%	5.378%
50	14.557	1946	1950	1957	rVB	89625	139067	1.50%	0.130%

51	14.687	1966	1972	1983	rBV	198686	348804	3.76%	0.326%
52	14.810	1989	1993	1998	rBV	28581	44872	0.48%	0.042%
53	14.910	2004	2010	2016	rBV	319001	442442	4.77%	0.414%
54	15.034	2027	2031	2035	rBV2	50495	67606	0.73%	0.063%
55	15.081	2035	2039	2042	rVV5	15847	23075	0.25%	0.022%

56	15.110	2042	2044	2049	rVB6	12404	18648	0.20%	0.017%
57	15.163	2049	2053	2057	rVB6	11596	17848	0.19%	0.017%
58	15.310	2071	2078	2079	rBV6	13743	24746	0.27%	0.023%
59	15.416	2090	2096	2102	rBV	356255	532986	5.75%	0.499%
60	15.492	2102	2109	2121	rVV	6113517	9068742	97.77%	8.486%

61	15.598	2121	2127	2135	rVV	1026378	1474151	15.89%	1.379%
62	15.675	2135	2140	2146	rVV3	97853	213685	2.30%	0.200%
63	15.728	2147	2149	2153	rVV2	50336	68089	0.73%	0.064%
64	15.763	2153	2155	2159	rVV4	25945	37123	0.40%	0.035%
65	15.834	2160	2167	2174	rVV	48831	95765	1.03%	0.090%

66	15.898	2175	2178	2182	rVV5	14666	26497	0.29%	0.025%
67	15.939	2182	2185	2188	rVV3	21249	35289	0.38%	0.033%
68	15.981	2188	2192	2202	rVB	190681	290786	3.14%	0.272%
69	16.339	2250	2253	2255	rBV4	13221	16489	0.18%	0.015%
70	16.522	2281	2284	2287	rBV3	12730	16069	0.17%	0.015%

71	16.628	2297	2302	2304	rVV6	27692	45055	0.49%	0.042%
72	16.651	2304	2306	2313	rVB2	35881	52004	0.56%	0.049%
73	16.739	2318	2321	2327	rBV3	27199	47556	0.51%	0.045%
74	16.892	2339	2347	2356	rVB5	49807	101846	1.10%	0.095%
75	17.028	2366	2370	2374	rBV6	25591	41318	0.45%	0.039%

76	17.116	2381	2385	2389	rVB7	16819	24185	0.26%	0.023%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018376.D
 Acq On : 25 Nov 2023 19:50
 Operator : MA/JU
 Sample : 05336-16
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.157	2389	2392	2396	rBV2	19259	29740	0.32%	0.028%
78	17.245	2401	2407	2417	rVV	4011337	5719195	61.66%	5.352%
79	17.345	2417	2424	2434	rVB	6344563	8854768	95.47%	8.286%
80	17.622	2467	2471	2479	rBV2	72480	124453	1.34%	0.116%
81	17.698	2481	2484	2488	rVB4	20471	24630	0.27%	0.023%
82	17.739	2488	2491	2498	rVB6	18630	27480	0.30%	0.026%
83	17.804	2498	2502	2508	rBV	47179	78010	0.84%	0.073%
84	17.904	2516	2519	2523	rBV3	23953	32256	0.35%	0.030%
85	18.081	2544	2549	2554	rBV3	44187	71415	0.77%	0.067%
86	18.139	2555	2559	2564	rBV3	73258	109197	1.18%	0.102%
87	18.304	2585	2587	2591	rVB5	21689	26769	0.29%	0.025%
88	18.381	2596	2600	2605	rBV	52733	89405	0.96%	0.084%
89	18.481	2614	2617	2620	rBV	20424	21239	0.23%	0.020%
90	18.545	2625	2628	2633	rBV5	28787	41808	0.45%	0.039%
91	18.592	2633	2636	2640	rBV	38960	47294	0.51%	0.044%
92	19.139	2725	2729	2730	rBV	33337	42410	0.46%	0.040%
93	19.163	2730	2733	2739	rVB	83153	107079	1.15%	0.100%
94	19.228	2740	2744	2748	rBV	74869	99481	1.07%	0.093%
95	19.316	2756	2759	2767	rVB5	34034	53936	0.58%	0.050%
96	19.380	2767	2770	2777	rBV4	44669	56499	0.61%	0.053%
97	19.586	2799	2805	2812	rBV	6727862	9032448	97.38%	8.452%
98	21.351	3100	3105	3114	rBV	3837861	5002698	53.94%	4.681%
99	23.633	3485	3493	3505	rVB2	4600396	9275194	100.00%	8.679%
100	23.792	3513	3520	3529	rVB	2666567	5572165	60.08%	5.214%




Sum of corrected areas: 106864264

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018376.D
Acq On : 25 Nov 2023 19:50
Operator : MA/JU
Sample : 05336-16
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

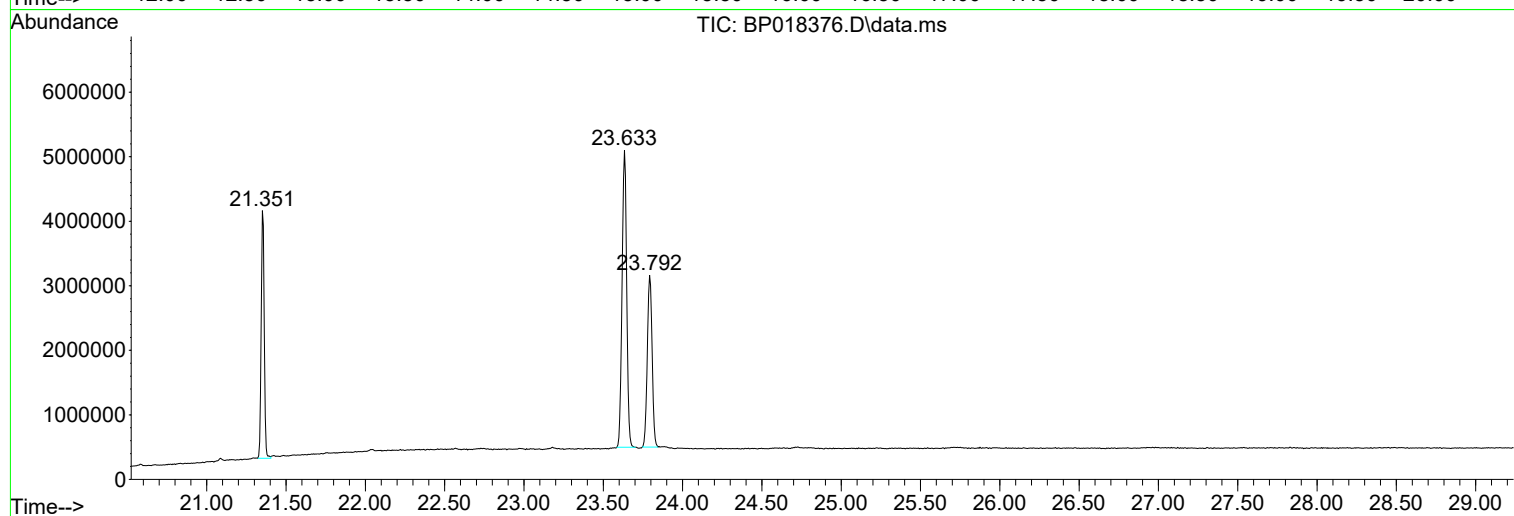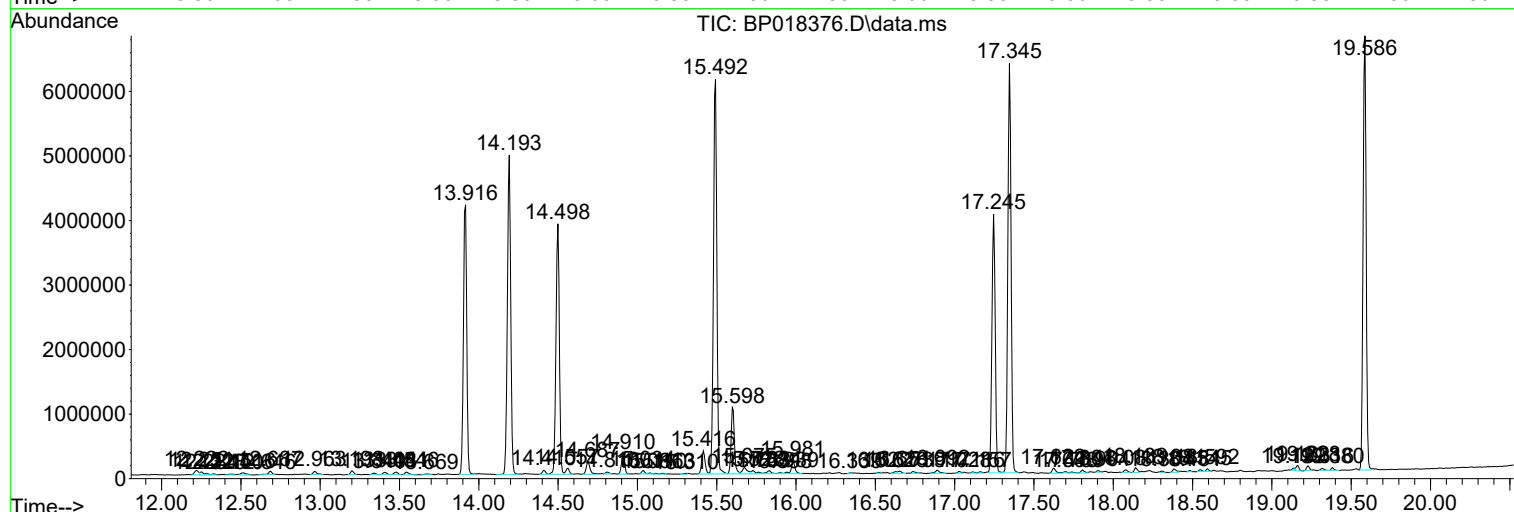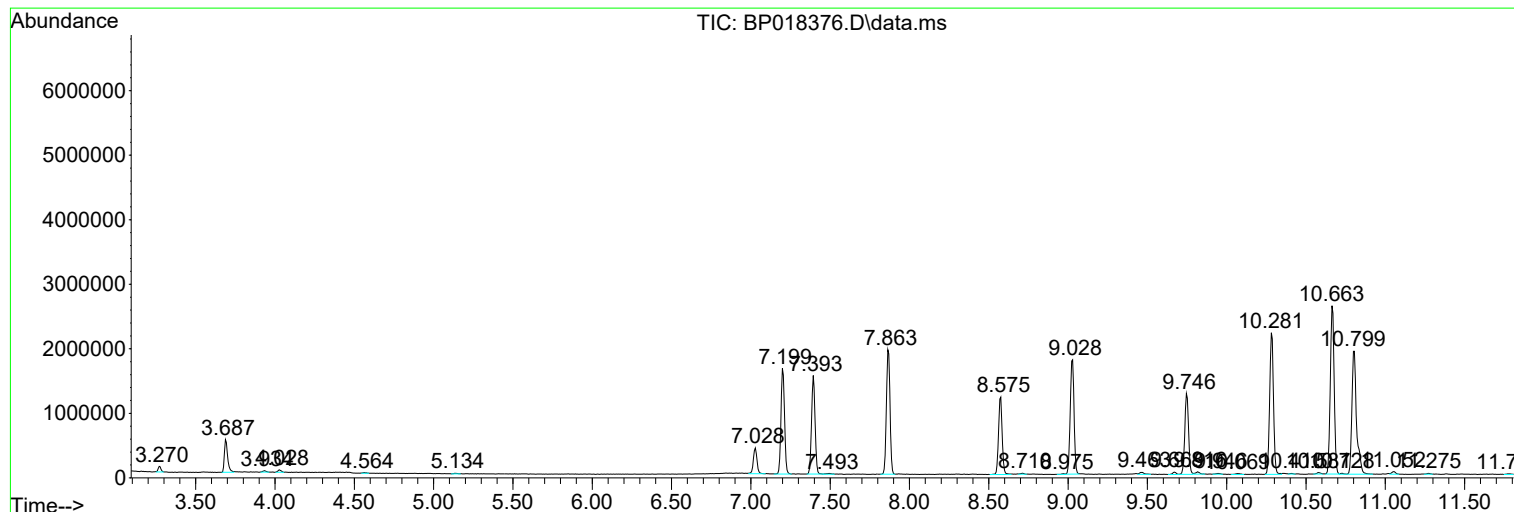

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018376.D
Acq On : 25 Nov 2023 19:50
Operator : MA/JU
Sample : 05336-16
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018376.D
Acq On : 25 Nov 2023 19:50
Operator : MA/JU
Sample : 05336-16
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------