

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
 Data File : BP018388.D
 Acq On : 26 Nov 2023 03:11
 Operator : MA/JU
 Sample : PB157165BL
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	130381	164589	2.06%	0.178%
2	3.687	98	102	123	rBV	1619069	2303722	28.77%	2.496%
3	4.028	156	160	168	rVB	38565	54270	0.68%	0.059%
4	7.028	663	670	683	rVB	1800634	2750160	34.34%	2.979%
5	7.199	692	699	708	rVB	1521575	2330758	29.10%	2.525%
6	7.393	725	732	745	rVB	1875860	2887162	36.05%	3.128%
7	7.863	805	812	822	rVB	1800890	2777300	34.68%	3.009%
8	8.575	925	933	947	rBV	2141421	3467498	43.30%	3.756%
9	9.022	1002	1009	1016	rBV	1603665	2586395	32.30%	2.802%
10	9.428	1067	1078	1079	rBV10	7616	18404	0.23%	0.020%
11	9.746	1120	1132	1143	rBV	1226752	1944569	24.28%	2.107%
12	10.281	1212	1223	1239	rBV	2119634	3497789	43.68%	3.789%
13	10.663	1280	1288	1300	rVB	2326538	3831089	47.84%	4.150%
14	10.798	1300	1311	1324	rBV	2021981	3455295	43.15%	3.743%
15	11.945	1500	1506	1508	rBV7	5642	9512	0.12%	0.010%
16	12.251	1552	1558	1566	rBV	41607	72182	0.90%	0.078%
17	12.469	1589	1595	1598	rVB8	4810	9450	0.12%	0.010%
18	12.881	1661	1665	1668	rBV6	5716	9009	0.11%	0.010%
19	13.404	1748	1754	1759	rBV	31188	47452	0.59%	0.051%
20	13.475	1761	1766	1770	rVB7	7533	12227	0.15%	0.013%
21	13.804	1820	1822	1829	rVB8	4565	8485	0.11%	0.009%
22	13.910	1833	1840	1851	rBV	3136257	4420155	55.20%	4.788%
23	14.187	1880	1887	1900	rBV	3902076	5760434	71.93%	6.240%
24	14.492	1932	1939	1950	rBV	2968404	4593486	57.36%	4.976%
25	14.686	1966	1972	1983	rBV	968672	1445520	18.05%	1.566%
26	15.310	2074	2078	2084	rBV8	6495	8362	0.10%	0.009%
27	15.486	2101	2108	2115	rBV	4621781	6557748	81.89%	7.104%
28	15.598	2121	2127	2138	rBV	680029	950402	11.87%	1.030%
29	15.728	2144	2149	2154	rVB	21831	32809	0.41%	0.036%
30	16.051	2202	2204	2211	rVB8	4917	9201	0.11%	0.010%
31	16.922	2346	2352	2356	rBV8	6973	13416	0.17%	0.015%
32	17.028	2367	2370	2375	rBV3	6940	10423	0.13%	0.011%
33	17.245	2400	2407	2417	rBV	3195947	4440530	55.45%	4.810%
34	17.345	2417	2424	2438	rVV	4306793	6077409	75.89%	6.584%
35	17.622	2468	2471	2474	rBV5	9345	14593	0.18%	0.016%
36	17.969	2528	2530	2536	rBV7	4605	8552	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018388.D
Acq On : 26 Nov 2023 03:11
Operator : MA/JU
Sample : PB157165BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M

Title : SVOA CALIBRATION

37	18.145	2556	2560	2565	rBV7	11249	18892	0.24%	0.020%
38	19.163	2729	2733	2738	rVB2	55729	71029	0.89%	0.077%
39	19.227	2740	2744	2749	rBV	49886	68767	0.86%	0.074%
40	19.586	2799	2805	2812	rBV	5403024	6886475	85.99%	7.460%
41	21.357	3100	3106	3115	rBV	3792991	5012851	62.60%	5.430%
42	23.639	3487	3494	3508	rVB2	3866889	8008198	100.00%	8.675%
43	23.798	3514	3521	3534	rVB	2635940	5664687	70.74%	6.137%




Sum of corrected areas: 92311256

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018388.D
Acq On : 26 Nov 2023 03:11
Operator : MA/JU
Sample : PB157165BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

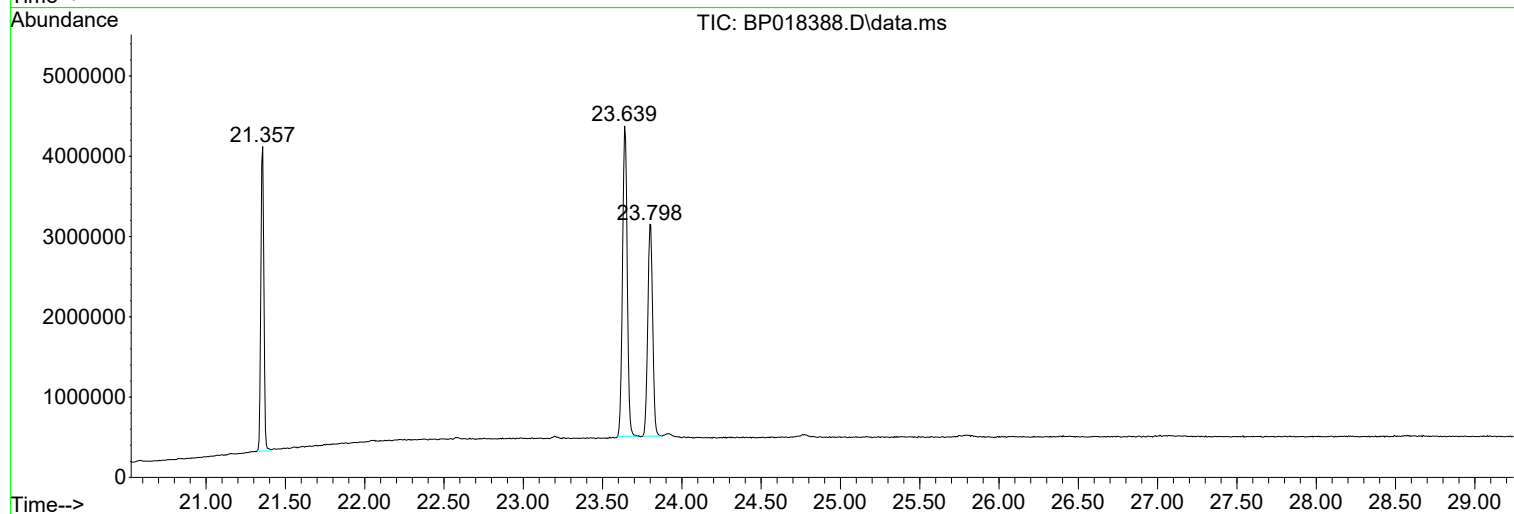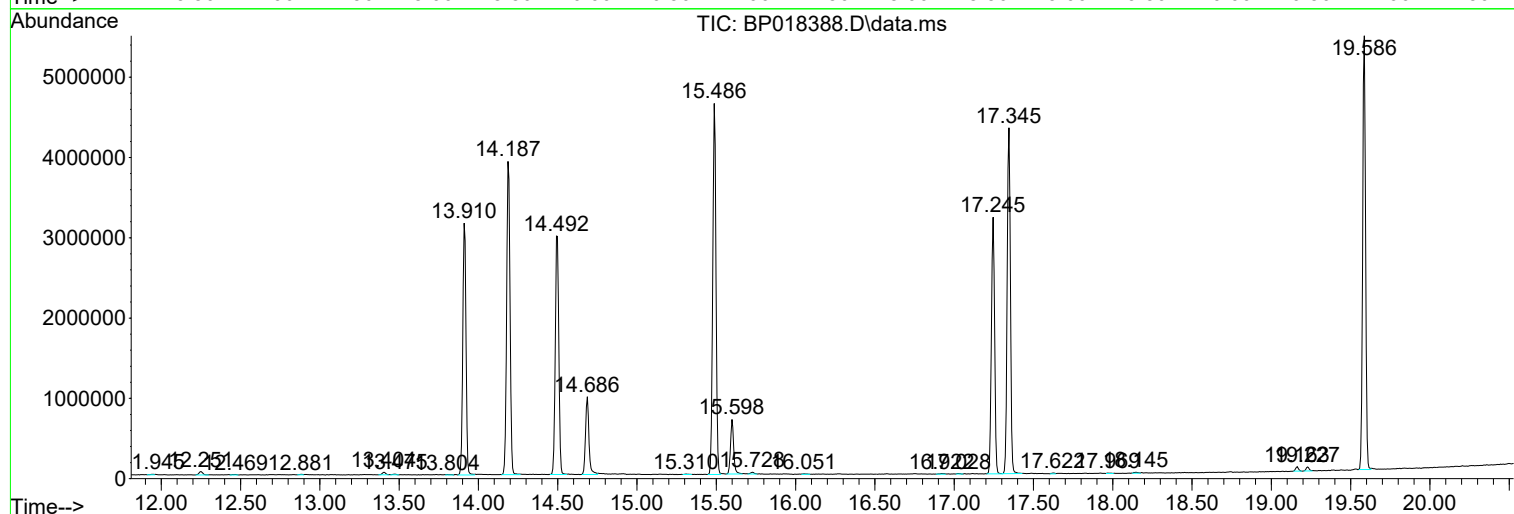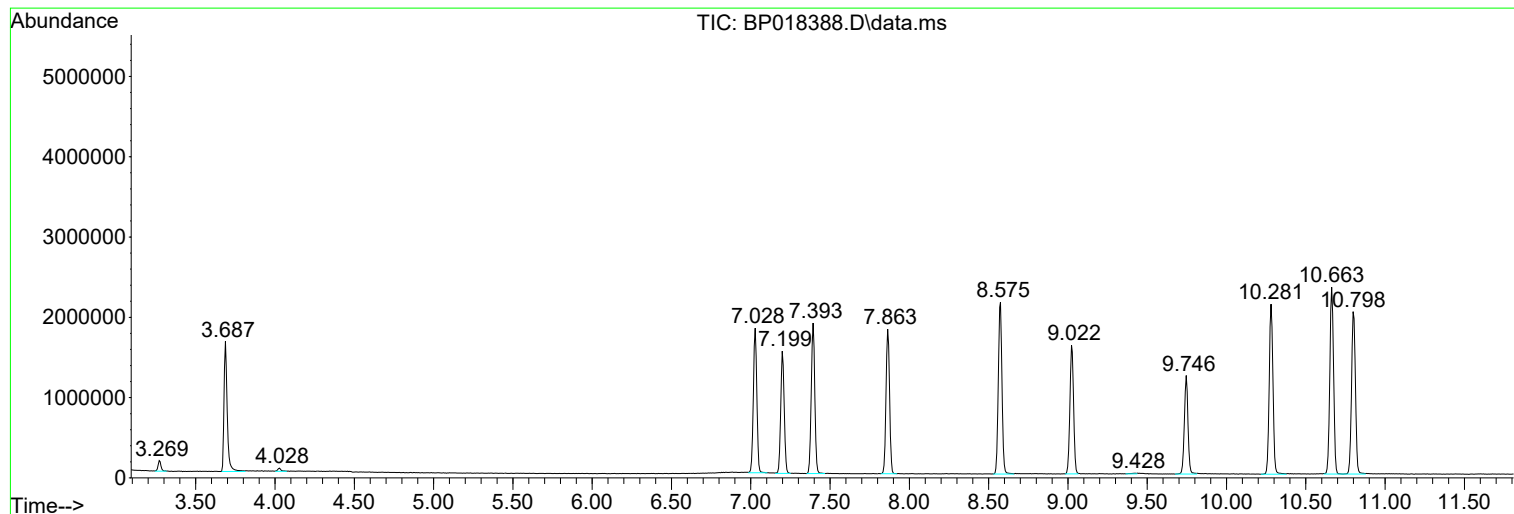

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018388.D
Acq On : 26 Nov 2023 03:11
Operator : MA/JU
Sample : PB157165BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112423\
Data File : BP018388.D
Acq On : 26 Nov 2023 03:11
Operator : MA/JU
Sample : PB157165BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------