

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
Data File : BP004094.D
Acq On : 25 Nov 2020 13:06
Operator : CG/JU
Sample : PB133245BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133245BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.922	3	6	27	rVB	13068462	15771601	100.00%	31.376%
2	5.799	488	495	513	rBV	2716960	4211983	26.71%	8.379%
3	7.451	768	776	798	rBV	2513260	4120603	26.13%	8.198%
4	8.269	905	915	927	rBV	519739	845669	5.36%	1.682%
5	9.434	1105	1113	1128	rBV	1612308	2689942	17.06%	5.351%
6	11.098	1388	1396	1407	rBV	629532	1078585	6.84%	2.146%
7	13.516	1799	1807	1829	rBV	3590252	5398637	34.23%	10.740%
8	14.898	2035	2042	2058	rBV2	873406	1327409	8.42%	2.641%
9	16.386	2288	2295	2314	rBV	2311253	3587342	22.75%	7.137%
10	17.633	2500	2507	2517	rBV	1078670	1477762	9.37%	2.940%
11	20.133	2926	2932	2940	rBV	5709546	6959809	44.13%	13.846%
12	21.668	3188	3193	3201	rBV	1092179	1420945	9.01%	2.827%
13	24.151	3608	3615	3622	rVB	679453	1376109	8.73%	2.738%


Sum of corrected areas: 50266396

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
Data File : BP004094.D
Acq On : 25 Nov 2020 13:06
Operator : CG/JU
Sample : PB133245BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133245BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

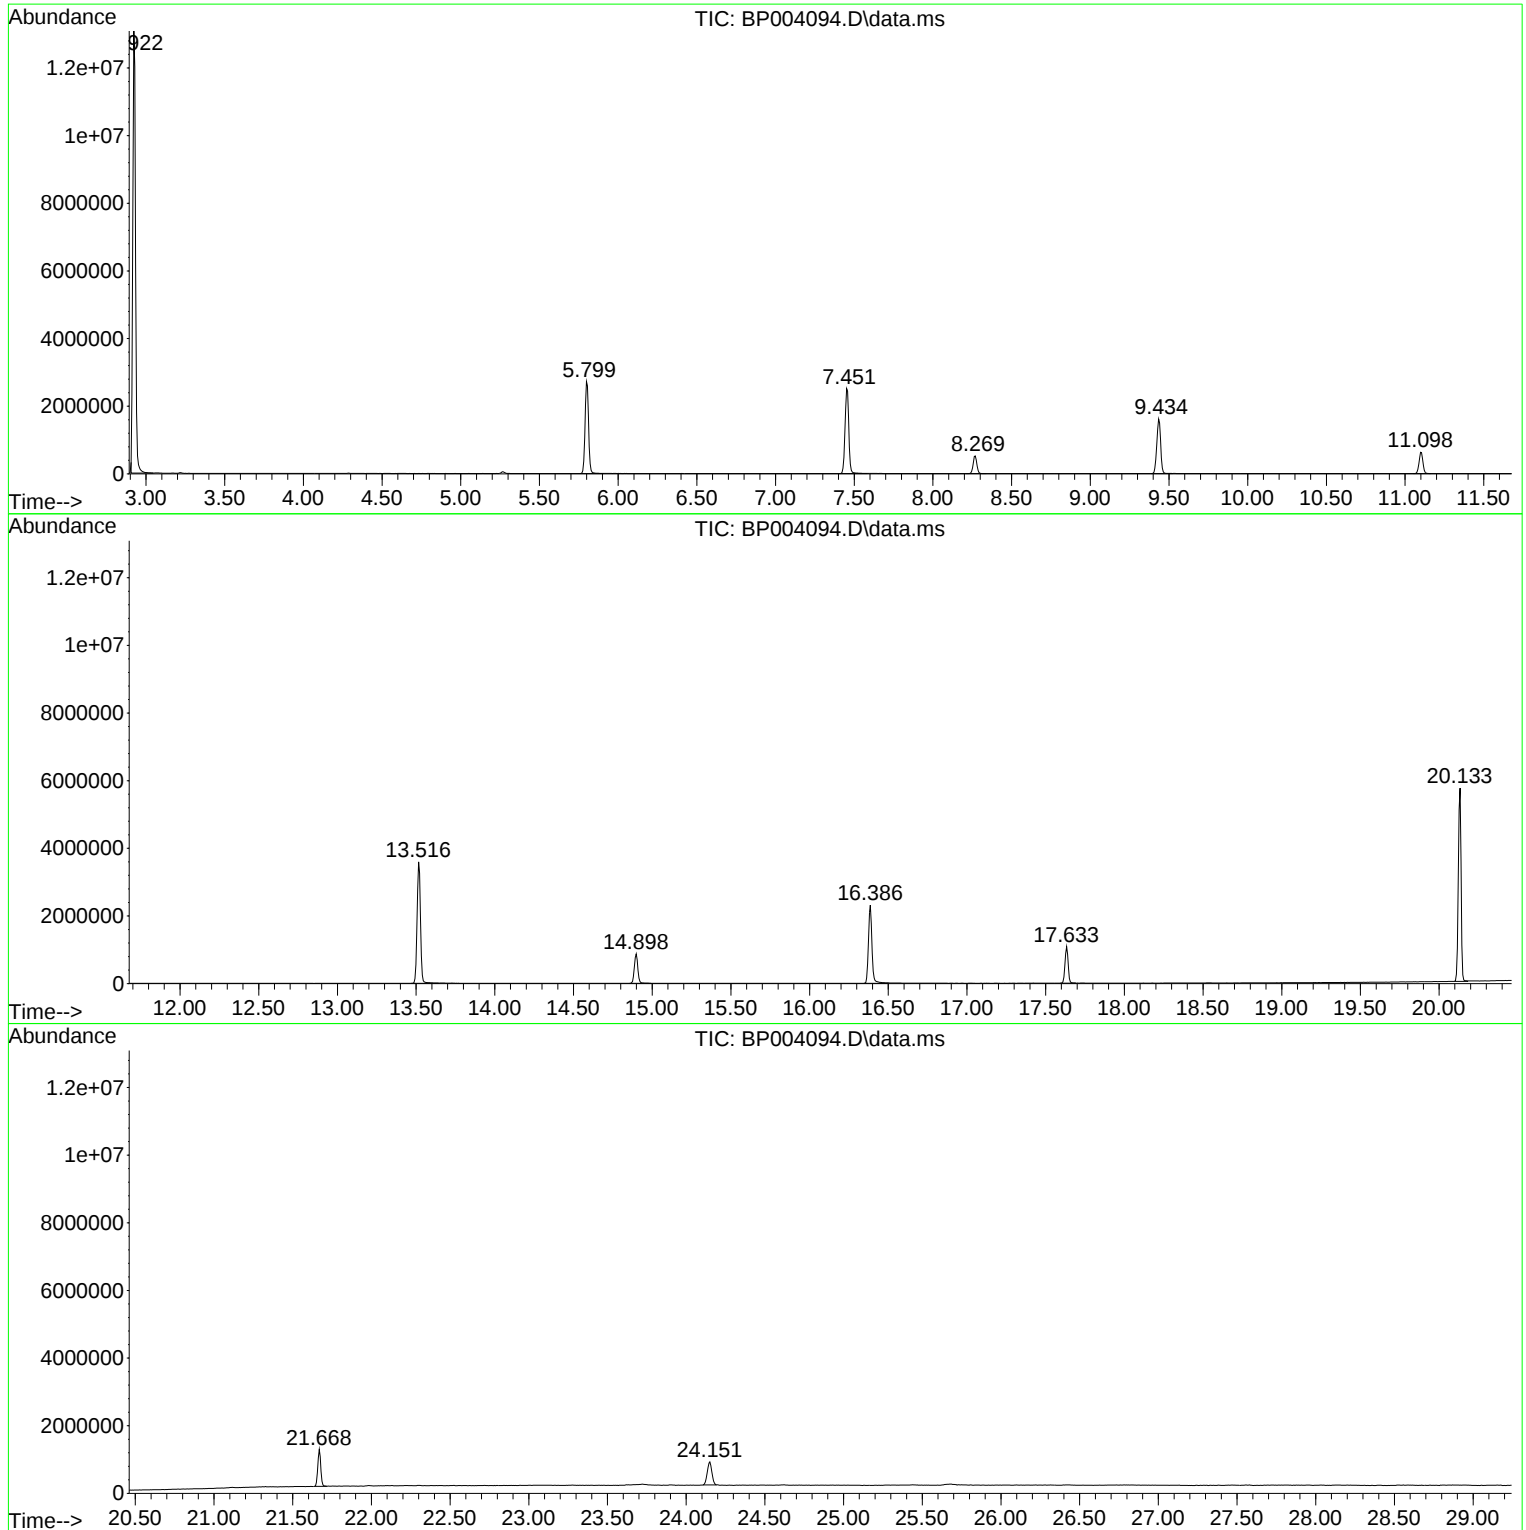

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
Data File : BP004094.D
Acq On : 25 Nov 2020 13:06
Operator : CG/JU
Sample : PB133245BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133245BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.922	373.00 ng	15771600	1,4-Dichlorobenzene-d4	8.269

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	72
2			1-Propanol, 2-methyl-	74	C4H10O	000078-83-1	9
3			N-Ethylformamide	73	C3H7NO	000627-45-2	9
4			1,3-Diaminoguanidine	89	CH7N5	004364-78-7	9
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

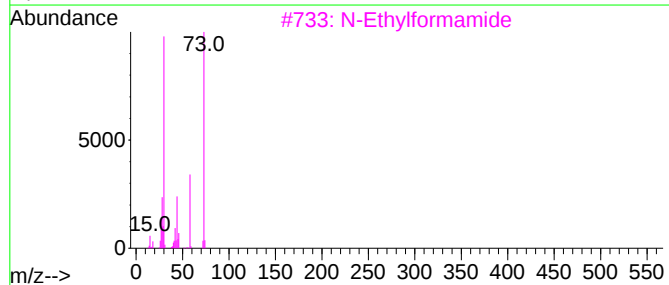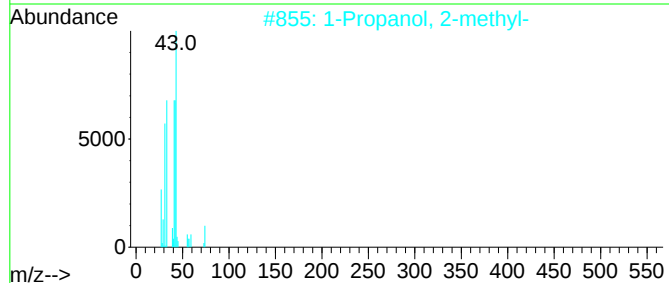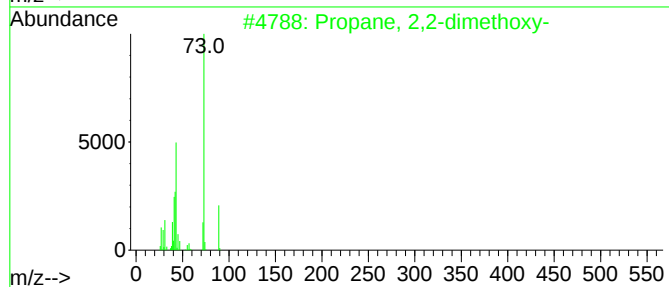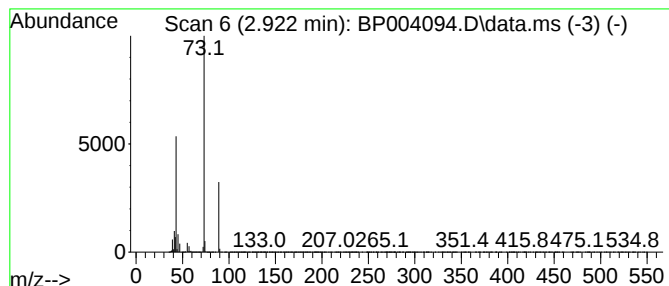

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
Data File : BP004094.D
Acq On : 25 Nov 2020 13:06
Operator : CG/JU
Sample : PB133245BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133245BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-di...	2.922	373.0	ng	15771600	1	8.269	845669	20.0