

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
 Data File : BP004096.D
 Acq On : 25 Nov 2020 14:20
 Operator : CG/JU
 Sample : PB133255BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB133255BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.969	179	184	191	rBV	77663	102478	1.40%	0.262%
2	4.628	290	296	311	rBV	1095817	1470245	20.08%	3.758%
3	5.263	398	404	416	rBV	1646005	2390356	32.65%	6.110%
4	5.805	489	496	512	rBV	2850863	4356524	59.51%	11.137%
5	6.399	591	597	609	rBV	122047	177369	2.42%	0.453%
6	7.457	768	777	795	rBV	2511315	4199625	57.36%	10.735%
7	8.269	908	915	928	rVB	493486	783500	10.70%	2.003%
8	9.434	1104	1113	1126	rBV	1666979	2767630	37.80%	7.075%
9	11.098	1387	1396	1406	rBV	608119	1017207	13.89%	2.600%
10	13.516	1799	1807	1827	rBV	3880830	5688089	77.70%	14.540%
11	14.892	2034	2041	2055	rBV	801081	1234535	16.86%	3.156%
12	16.380	2287	2294	2322	rBV	2448920	3735749	51.03%	9.550%
13	17.627	2499	2506	2518	rBV	952810	1368653	18.69%	3.499%
14	20.127	2925	2931	2944	rBV	6125681	7320975	100.00%	18.715%
15	21.663	3187	3192	3202	rBV	1010076	1333741	18.22%	3.409%
16	24.139	3607	3613	3623	rVB2	537620	1172404	16.01%	2.997%




Sum of corrected areas: 39119080

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
Data File : BP004096.D
Acq On : 25 Nov 2020 14:20
Operator : CG/JU
Sample : PB133255BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133255BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

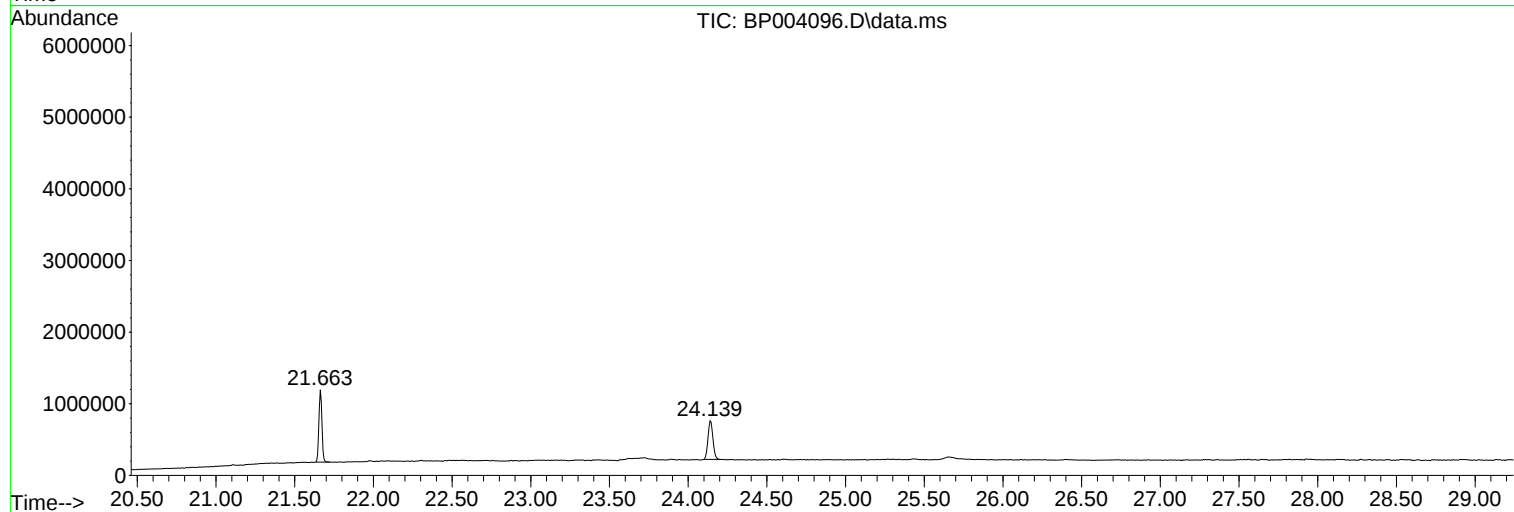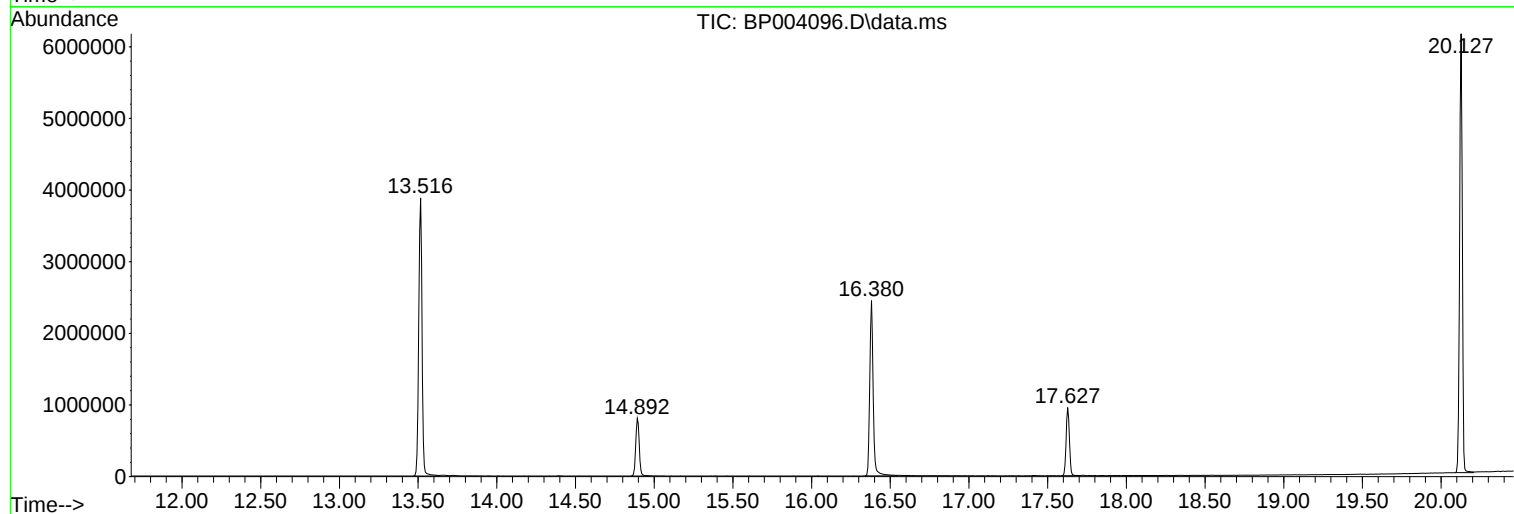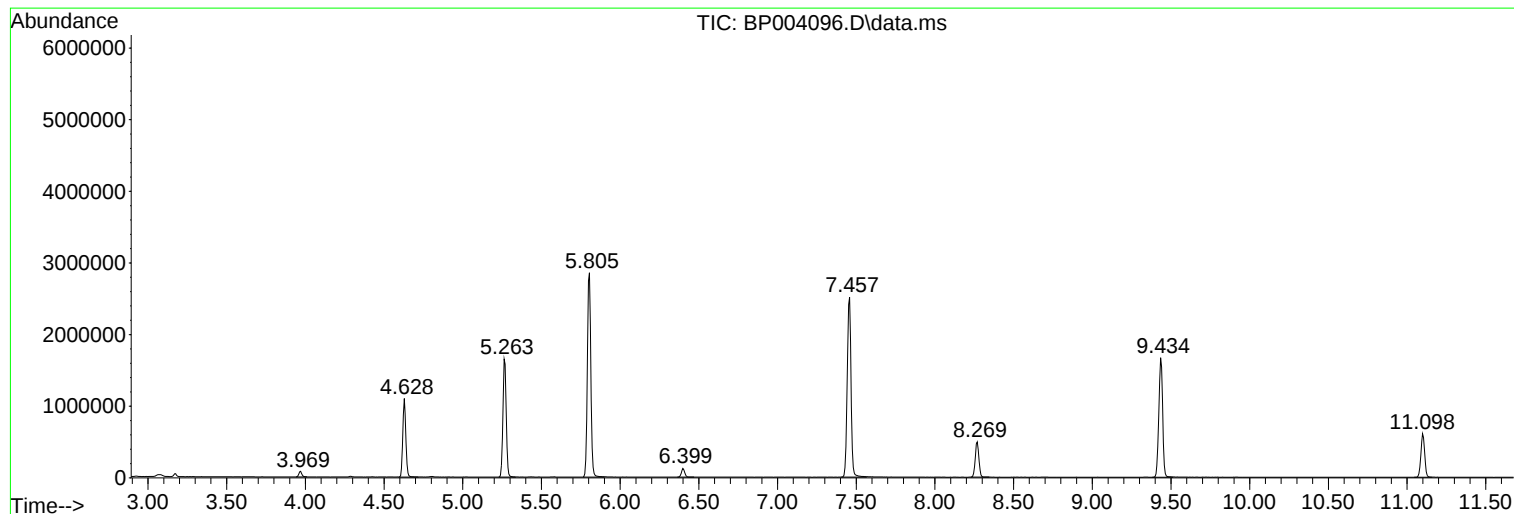

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
Data File : BP004096.D
Acq On : 25 Nov 2020 14:20
Operator : CG/JU
Sample : PB133255BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133255BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
Data File : BP004096.D
Acq On : 25 Nov 2020 14:20
Operator : CG/JU
Sample : PB133255BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133255BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------