

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112520\  
 Data File : BP004099.D  
 Acq On : 25 Nov 2020 16:14  
 Operator : CG/JU  
 Sample : L4880-02  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 KENS-B4-112320-0-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270E-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004099.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.158       | 42            | 46          | 69           | rVB      | 168336         | 297307        | 6.96%           | 1.032%        |
| 2         | 5.263       | 399           | 404         | 413          | rVB      | 56354          | 86527         | 2.03%           | 0.300%        |
| 3         | 5.799       | 488           | 495         | 509          | rBV      | 1479409        | 2293508       | 53.69%          | 7.958%        |
| 4         | 7.451       | 769           | 776         | 793          | rBV      | 1458929        | 2401253       | 56.22%          | 8.332%        |
| 5         | 7.840       | 837           | 842         | 852          | rVB      | 29719          | 51441         | 1.20%           | 0.178%        |
| 6         | 8.263       | 908           | 914         | 923          | rBV      | 399497         | 637858        | 14.93%          | 2.213%        |
| 7         | 9.428       | 1104          | 1112        | 1121         | rBV      | 901374         | 1544426       | 36.16%          | 5.359%        |
| 8         | 11.098      | 1388          | 1396        | 1403         | rBV      | 510541         | 869639        | 20.36%          | 3.018%        |
| 9         | 13.510      | 1799          | 1806        | 1825         | rBV      | 2089465        | 3123791       | 73.13%          | 10.839%       |
| 10        | 13.775      | 1846          | 1851        | 1859         | rVB      | 52803          | 78790         | 1.84%           | 0.273%        |
| 11        | 14.316      | 1937          | 1943        | 1951         | rBV      | 295158         | 426738        | 9.99%           | 1.481%        |
| 12        | 14.698      | 2002          | 2008        | 2018         | rBV3     | 23292          | 71177         | 1.67%           | 0.247%        |
| 13        | 14.892      | 2035          | 2041        | 2050         | rVB      | 762633         | 1140671       | 26.71%          | 3.958%        |
| 14        | 15.992      | 2223          | 2228        | 2240         | rBV4     | 53506          | 125464        | 2.94%           | 0.435%        |
| 15        | 16.375      | 2287          | 2293        | 2305         | rBV      | 1645156        | 2407758       | 56.37%          | 8.355%        |
| 16        | 17.622      | 2499          | 2505        | 2512         | rBV      | 957922         | 1373443       | 32.15%          | 4.766%        |
| 17        | 17.763      | 2520          | 2529        | 2530         | rBV5     | 47515          | 108550        | 2.54%           | 0.377%        |
| 18        | 18.463      | 2644          | 2648        | 2653         | rBV      | 61181          | 86521         | 2.03%           | 0.300%        |
| 19        | 18.521      | 2655          | 2658        | 2663         | rVB      | 32193          | 43220         | 1.01%           | 0.150%        |
| 20        | 18.733      | 2690          | 2694        | 2698         | rBV2     | 39934          | 59403         | 1.39%           | 0.206%        |
| 21        | 19.269      | 2782          | 2785        | 2791         | rBV4     | 34503          | 64293         | 1.51%           | 0.223%        |
| 22        | 19.910      | 2884          | 2894        | 2907         | rVB      | 318896         | 965382        | 22.60%          | 3.350%        |
| 23        | 20.121      | 2925          | 2930        | 2935         | rVB      | 3595337        | 4271367       | 100.00%         | 14.821%       |
| 24        | 21.045      | 3080          | 3087        | 3095         | rBV      | 402976         | 858328        | 20.09%          | 2.978%        |
| 25        | 21.304      | 3128          | 3131        | 3140         | rVB      | 340386         | 514981        | 12.06%          | 1.787%        |
| 26        | 21.492      | 3158          | 3163        | 3170         | rVB5     | 137683         | 312074        | 7.31%           | 1.083%        |
| 27        | 21.657      | 3186          | 3191        | 3196         | rBV      | 1125875        | 1609577       | 37.68%          | 5.585%        |
| 28        | 21.974      | 3240          | 3245        | 3262         | rVB3     | 239512         | 677953        | 15.87%          | 2.352%        |
| 29        | 23.015      | 3418          | 3422        | 3433         | rVB3     | 147672         | 329997        | 7.73%           | 1.145%        |
| 30        | 23.262      | 3461          | 3464        | 3470         | rVB      | 113064         | 161452        | 3.78%           | 0.560%        |
| 31        | 24.133      | 3605          | 3612        | 3621         | rVB2     | 858680         | 1826243       | 42.76%          | 6.337%        |




Sum of corrected areas: 28819132

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112520\  
Data File : BP004099.D  
Acq On : 25 Nov 2020 16:14  
Operator : CG/JU  
Sample : L4880-02  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
KENS-B4-112320-0-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270E-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

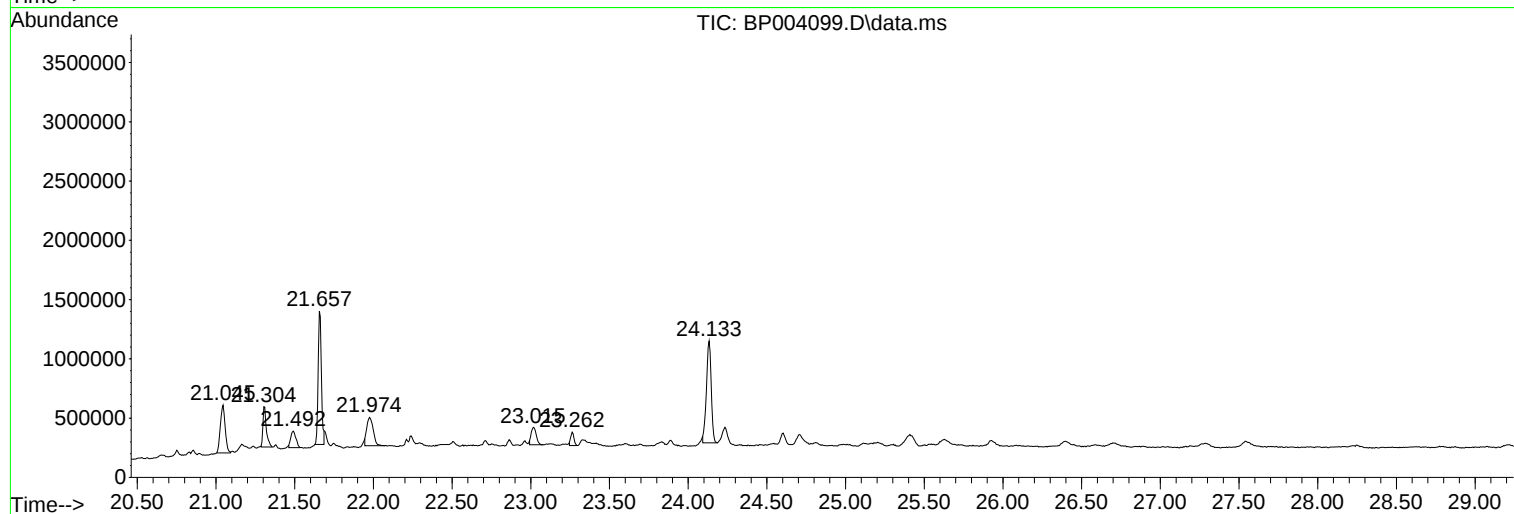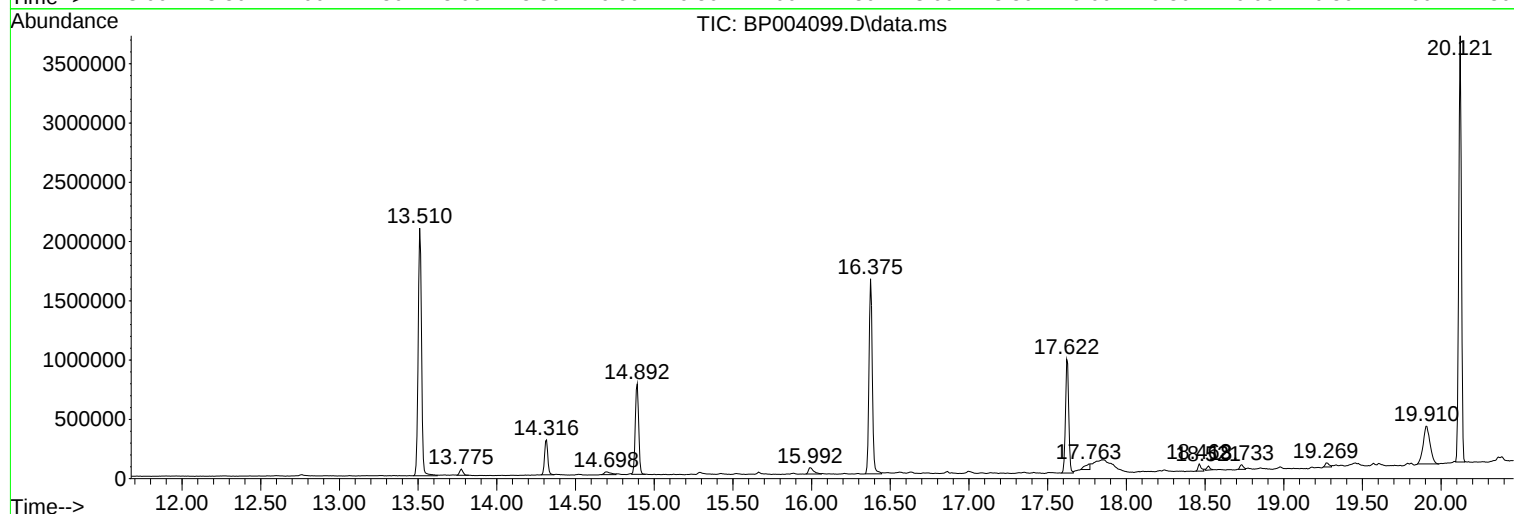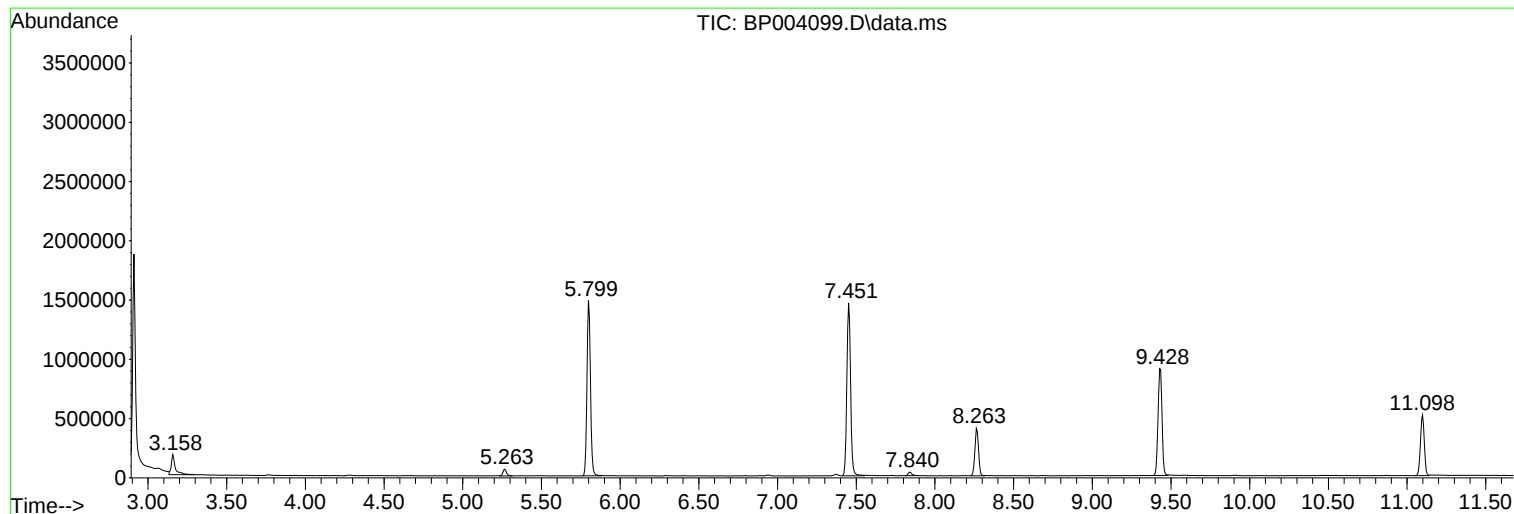

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112520\  
Data File : BP004099.D  
Acq On : 25 Nov 2020 16:14  
Operator : CG/JU  
Sample : L4880-02  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
KENS-B4-112320-0-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270E-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112520\  
Data File : BP004099.D  
Acq On : 25 Nov 2020 16:14  
Operator : CG/JU  
Sample : L4880-02  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
KENS-B4-112320-0-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270E-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----