


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112520\
 Data File : BP004090.D
 Acq On : 25 Nov 2020 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 23 16:42:41 2020

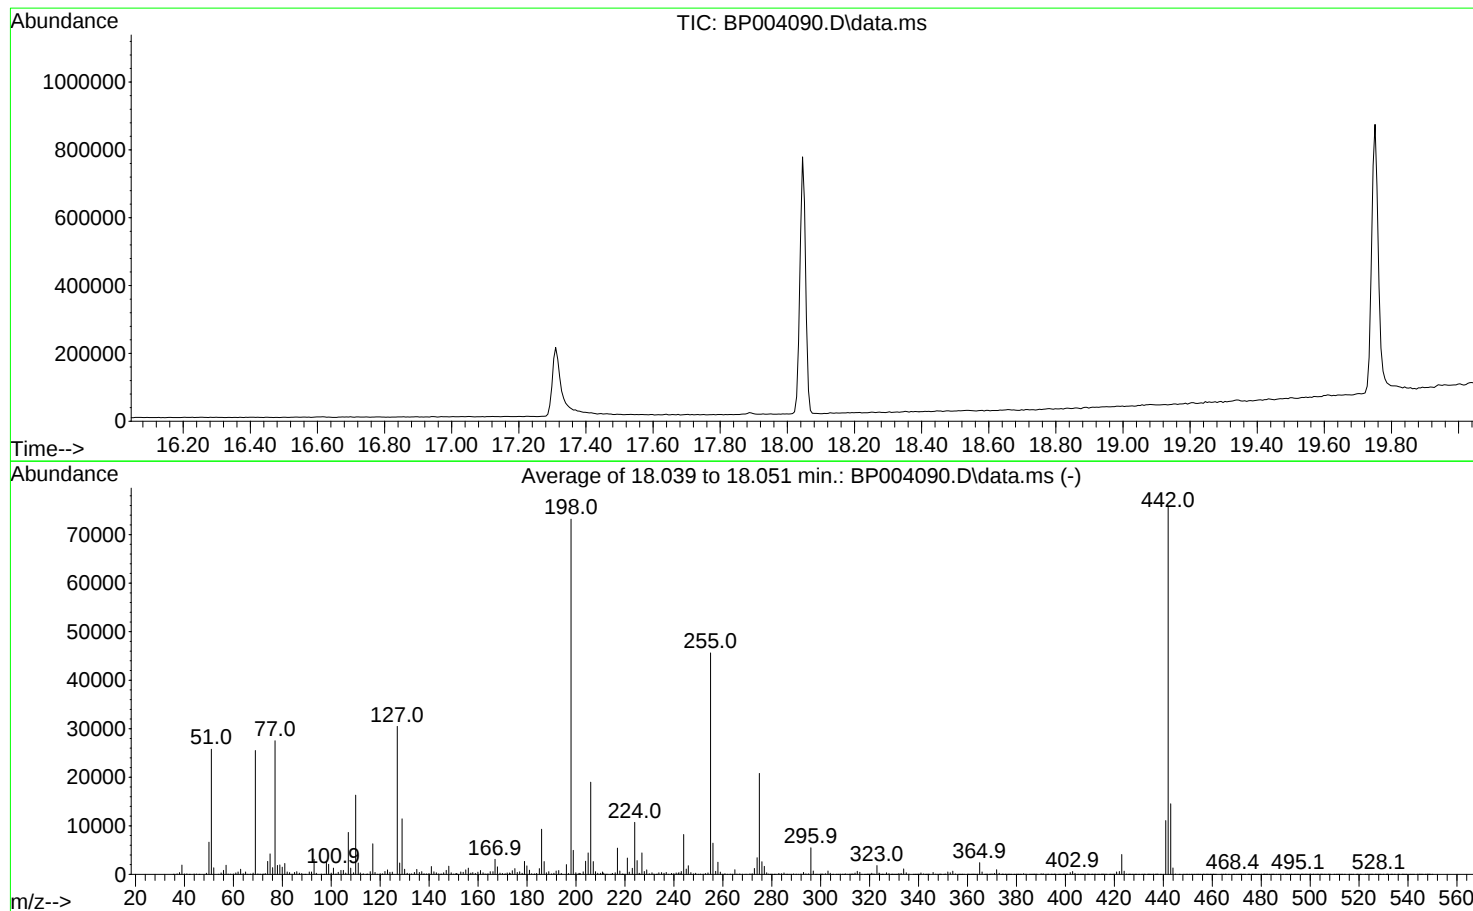

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	25795	PASS
68	69	0.00	2	1.1	279	PASS
69	198	0.00	100	34.9	25529	PASS
70	69	0.00	2	0.4	110	PASS
127	198	10	80	41.7	30488	PASS
197	198	0.00	2	0.2	175	PASS
198	198	100	100	100.0	73181	PASS
199	198	5	9	6.8	4963	PASS
275	198	10	60	28.4	20816	PASS
365	198	1	100	3.3	2427	PASS
441	198	0.01	100	15.1	11067	PASS
442	442	100	100	100.0	75797	PASS
443	442	15	24	19.2	14532	PASS