
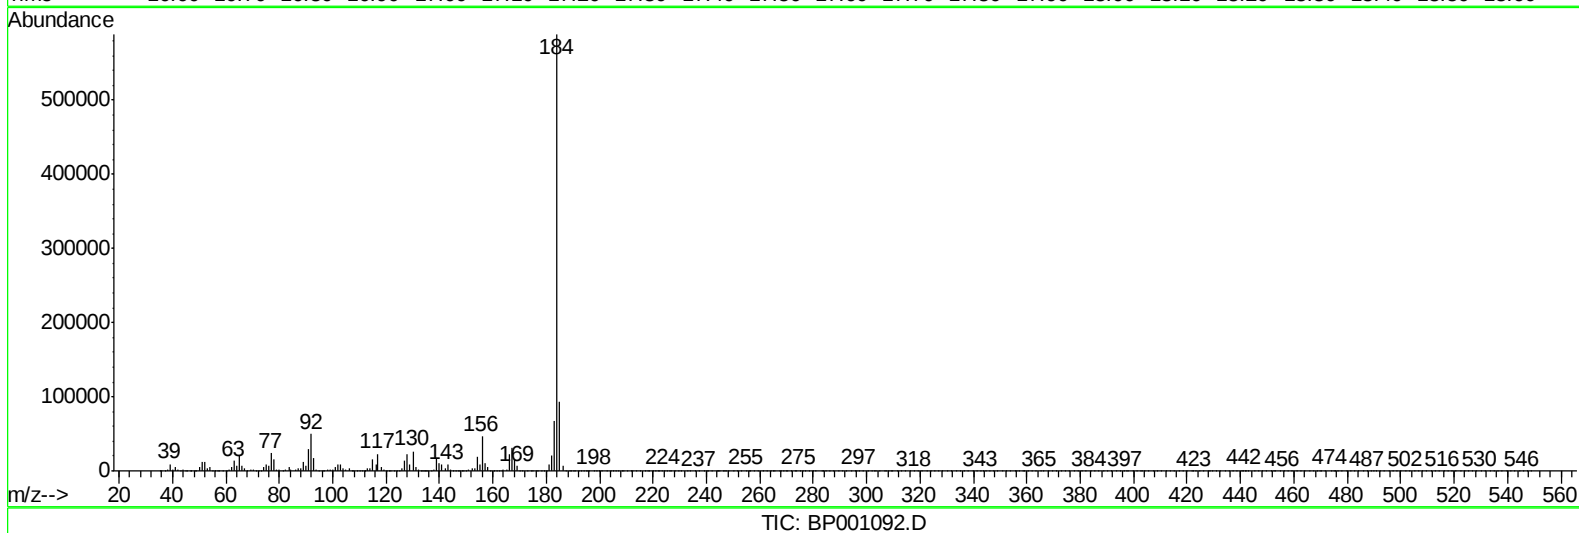


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP112719\
Data File : BP001092.D
Acq On : 27 Nov 2019 21:07
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 05:38:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 17:38:46 2019
Response via : Initial Calibration

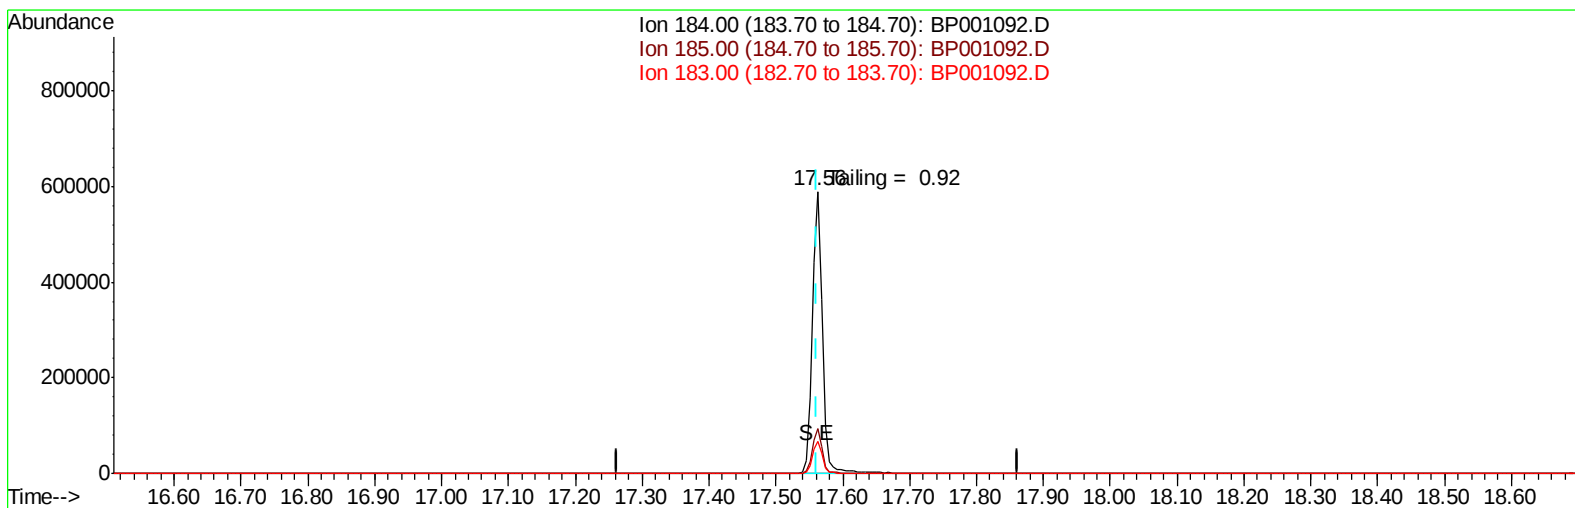

TIC: BP001092.D

(77) Benzidine



17.563min (+0.000) 1731096.07ng

response 625738

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	15.91
183.00	11.60	11.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP112719\
Data File : BP001092.D
Acq On : 27 Nov 2019 21:07
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 05:38:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 17:38:46 2019
Response via : Initial Calibration

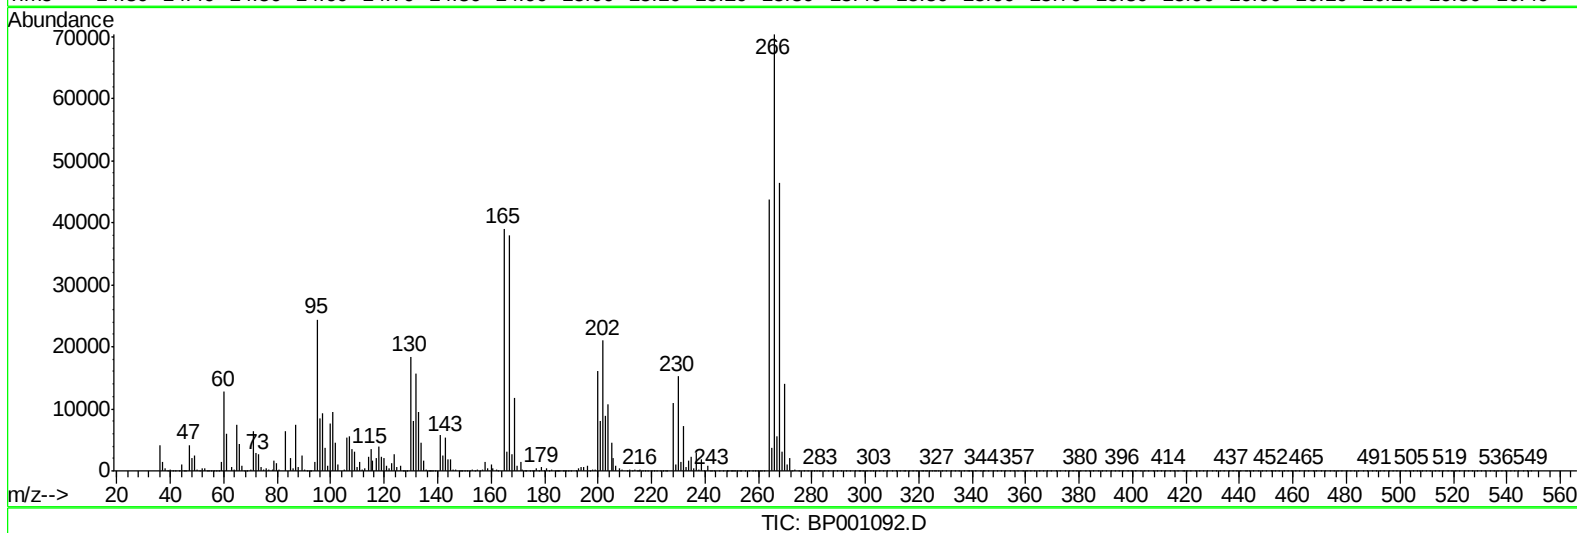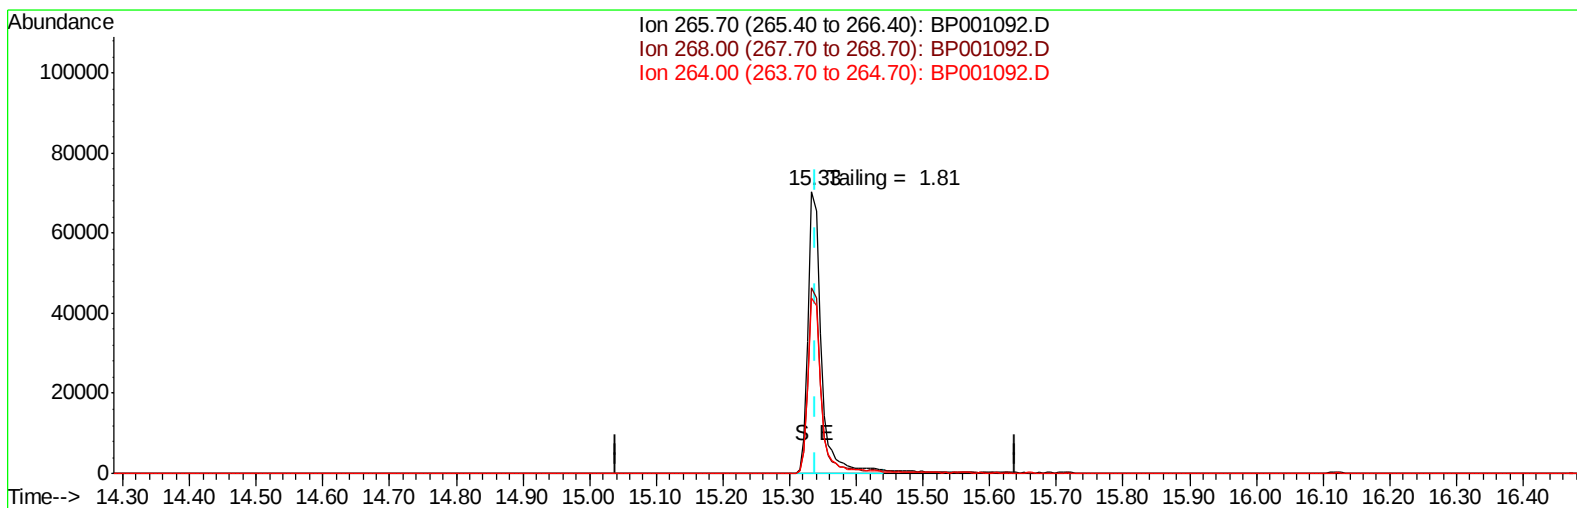

(70) Pentachlorophenol (C)

15.333min (-0.006) 1897802.11ng

response 94447

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	65.91
264.00	65.30	62.29
0.00	0.00	0.00