
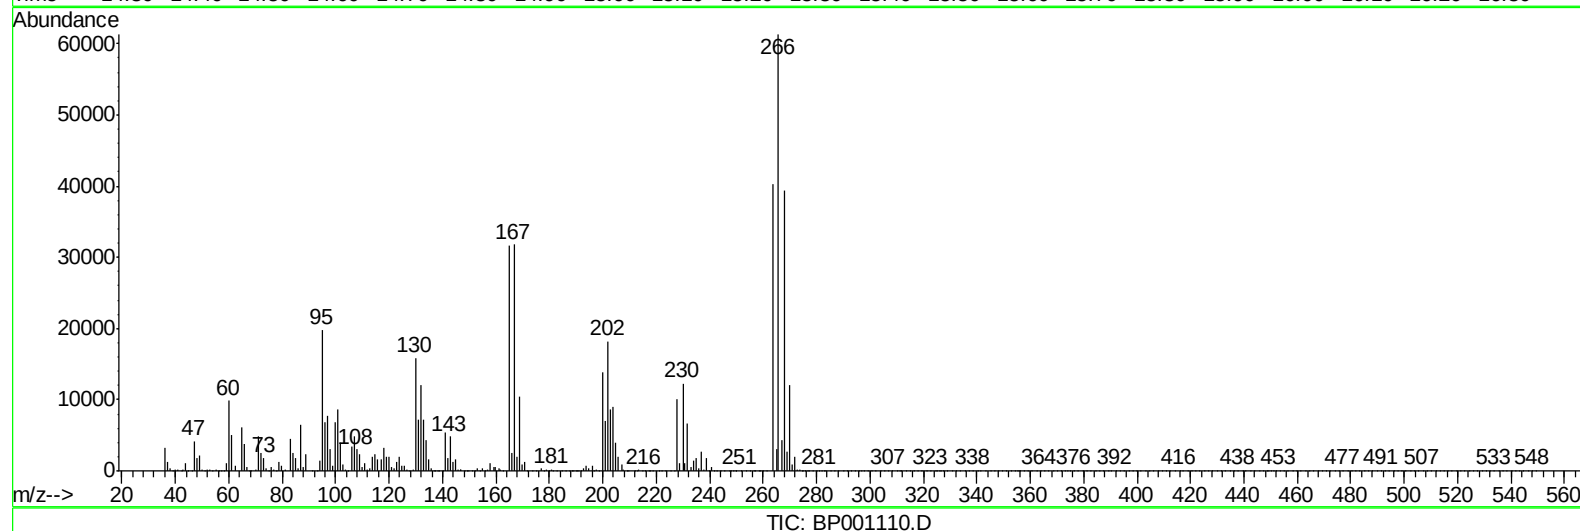


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP112719\
Data File : BP001110.D
Acq On : 28 Nov 2019 06:07
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 29 05:39:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 17:38:46 2019
Response via : Initial Calibration

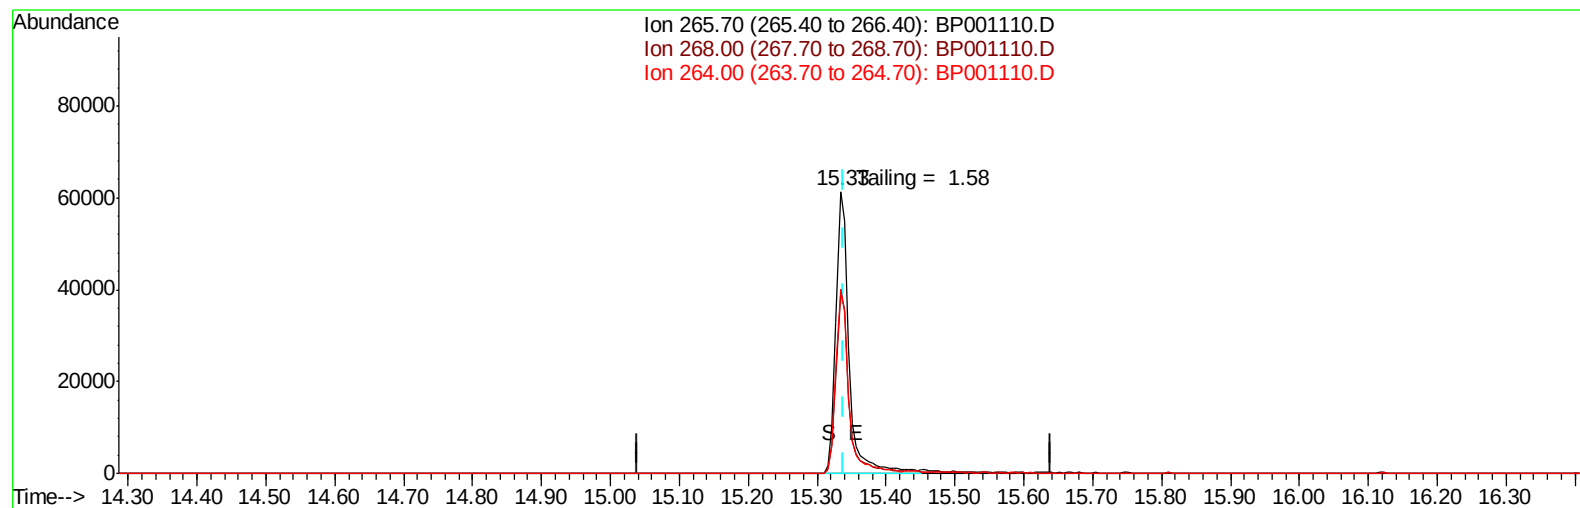

TIC: BP001110.D

(70) Pentachlorophenol (C)



15.334min (-0.006) 3176553.46ng

response 79043

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.21
264.00	65.30	65.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP112719\
 Data File : BP001110.D
 Acq On : 28 Nov 2019 06:07
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Quant Time: Nov 29 05:39:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 27 17:38:46 2019
 Response via : Initial Calibration

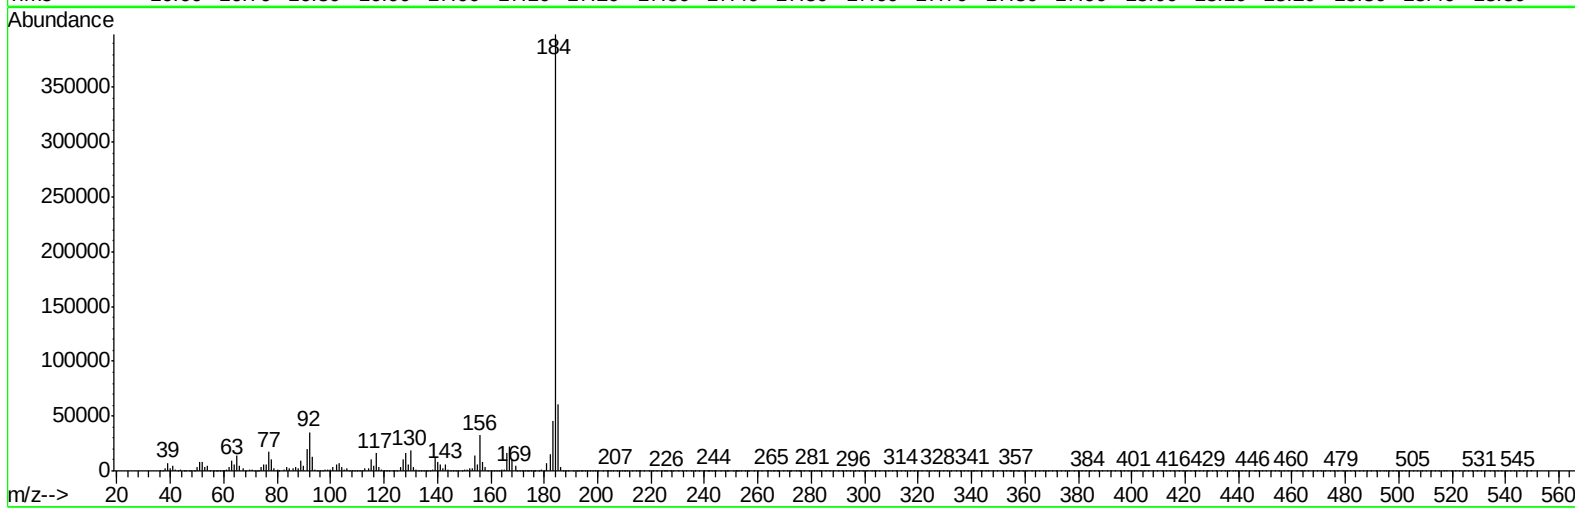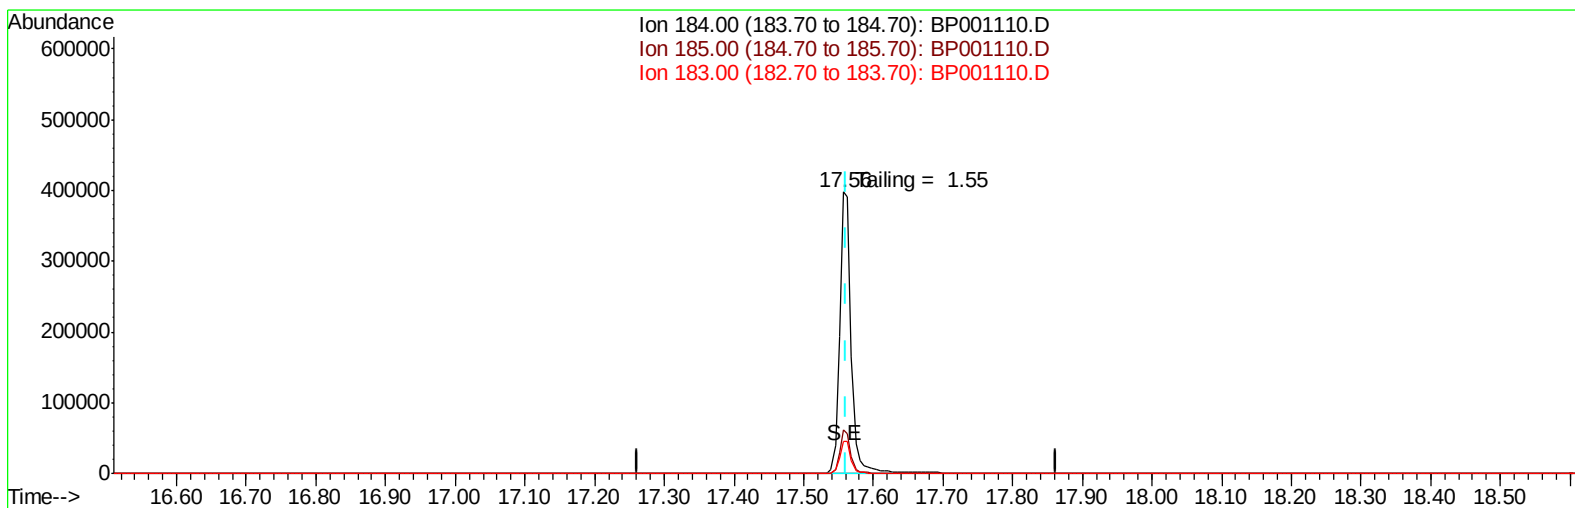

TIC: BP001110.D

(77) Benzidine

17.557min (-0.006) 1760927.65ng

response 454658

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	15.33
183.00	11.60	11.55
0.00	0.00	0.00