
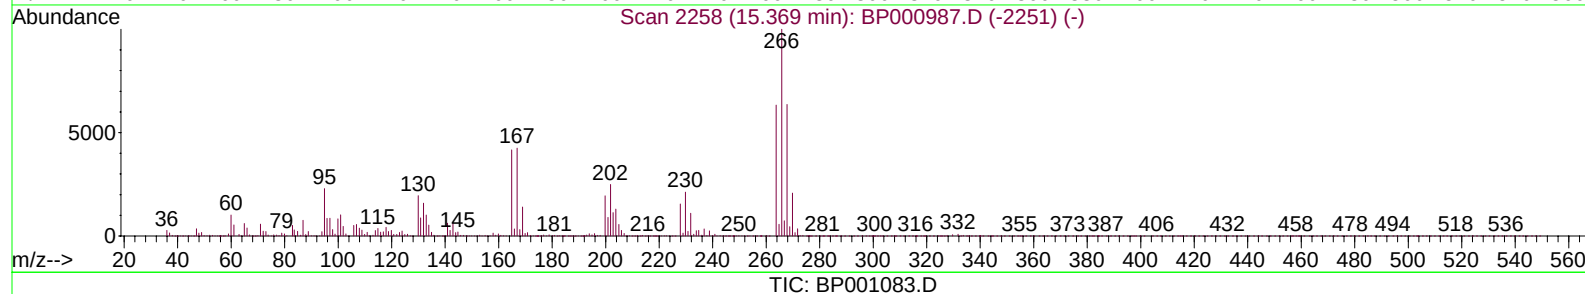
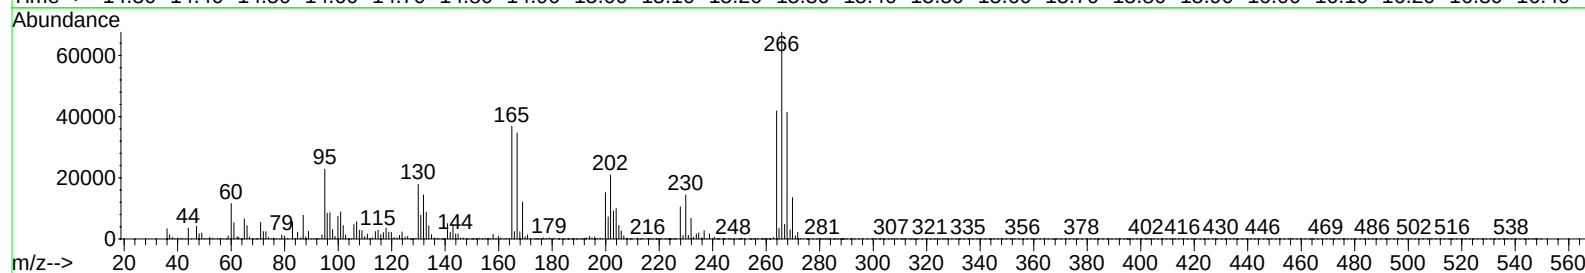


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP112719\
Data File : BP001083.D
Acq On : 27 Nov 2019 11:46
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 12:20:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

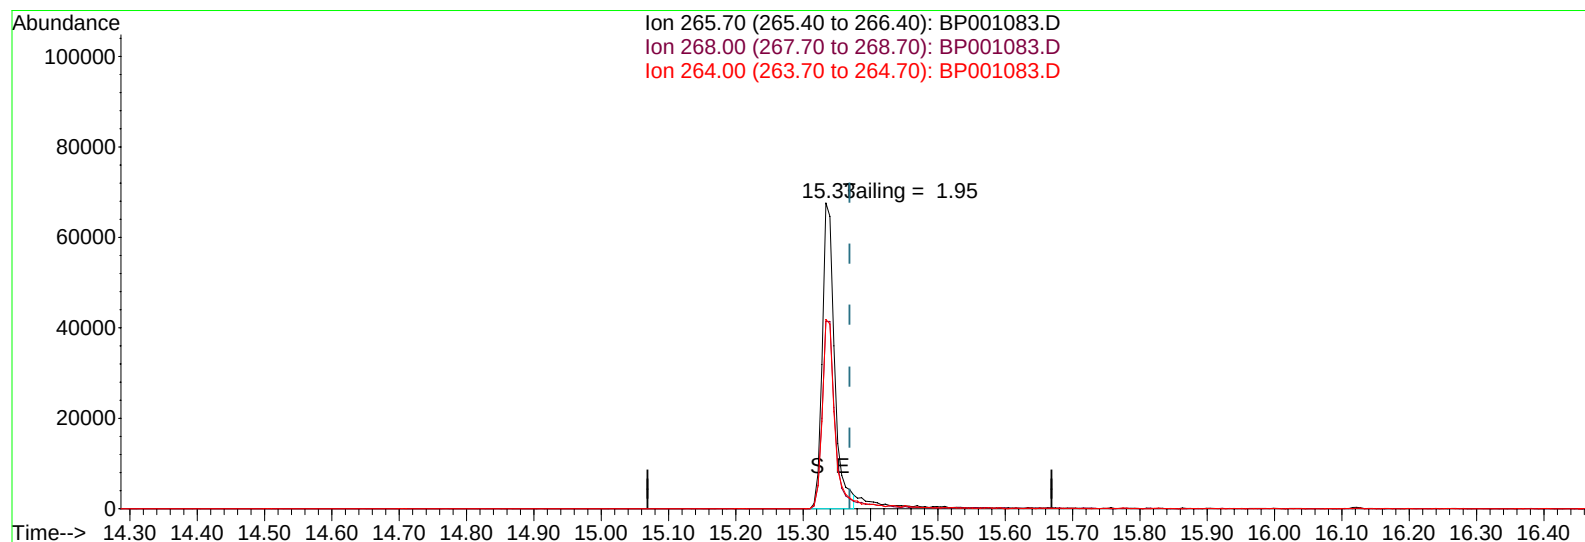

(70) Pentachlorophenol (C)




15.334min (-0.035) 1890562.56ng

response 91845

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	61.25
264.00	63.30	61.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP112719\
 Data File : BP001083.D
 Acq On : 27 Nov 2019 11:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 12:20:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 06 17:07:13 2019
 Response via : Initial Calibration

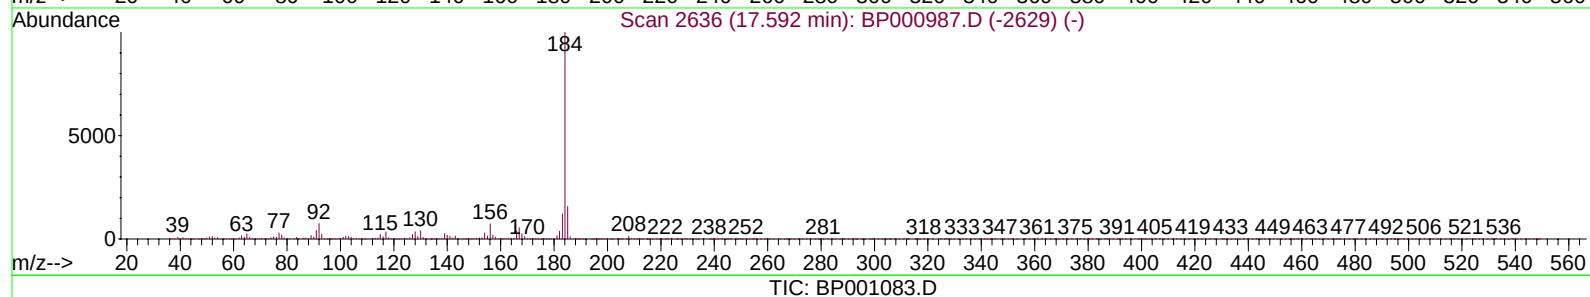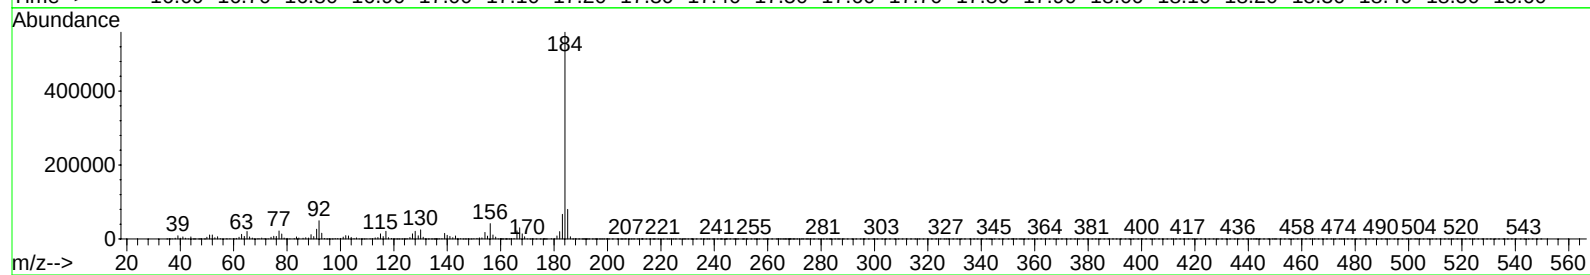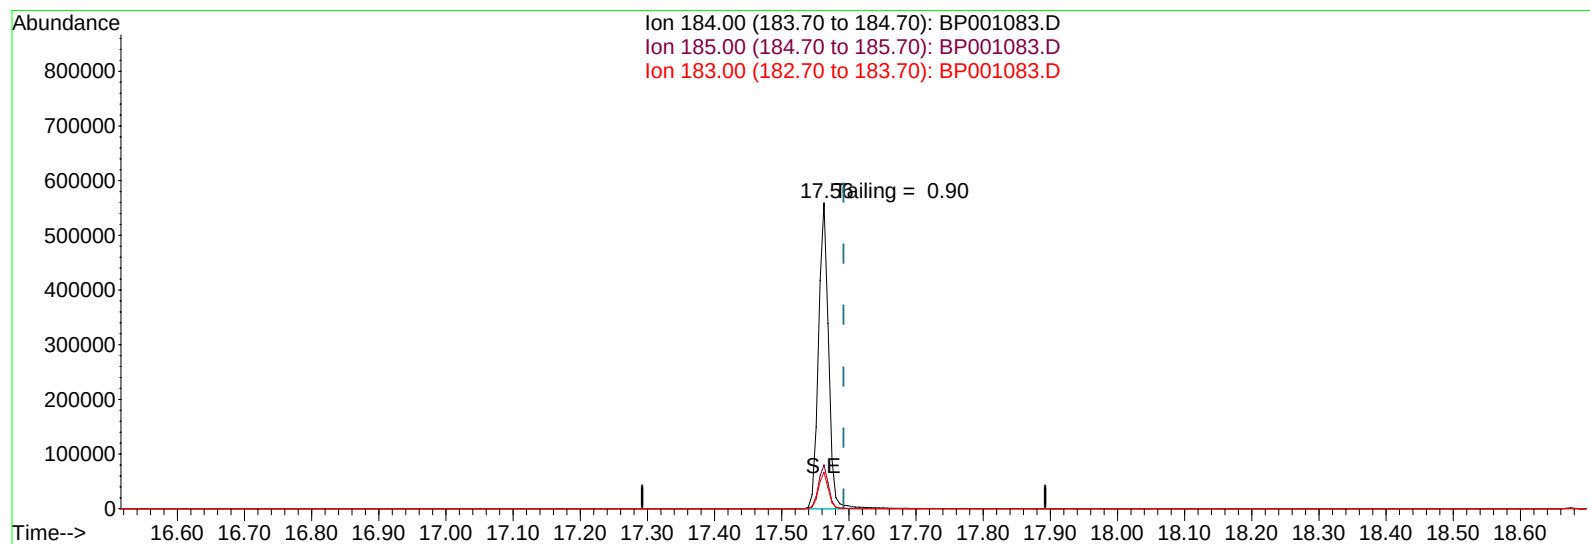

(77) Benzidine

17.563min (-0.029) 1441175.99ng

response 583799

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.33
183.00	12.20	11.90
0.00	0.00	0.00