


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP112719\
 Data File : BP001092.D
 Acq On : 27 Nov 2019 21:07
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 27 17:38:46 2019

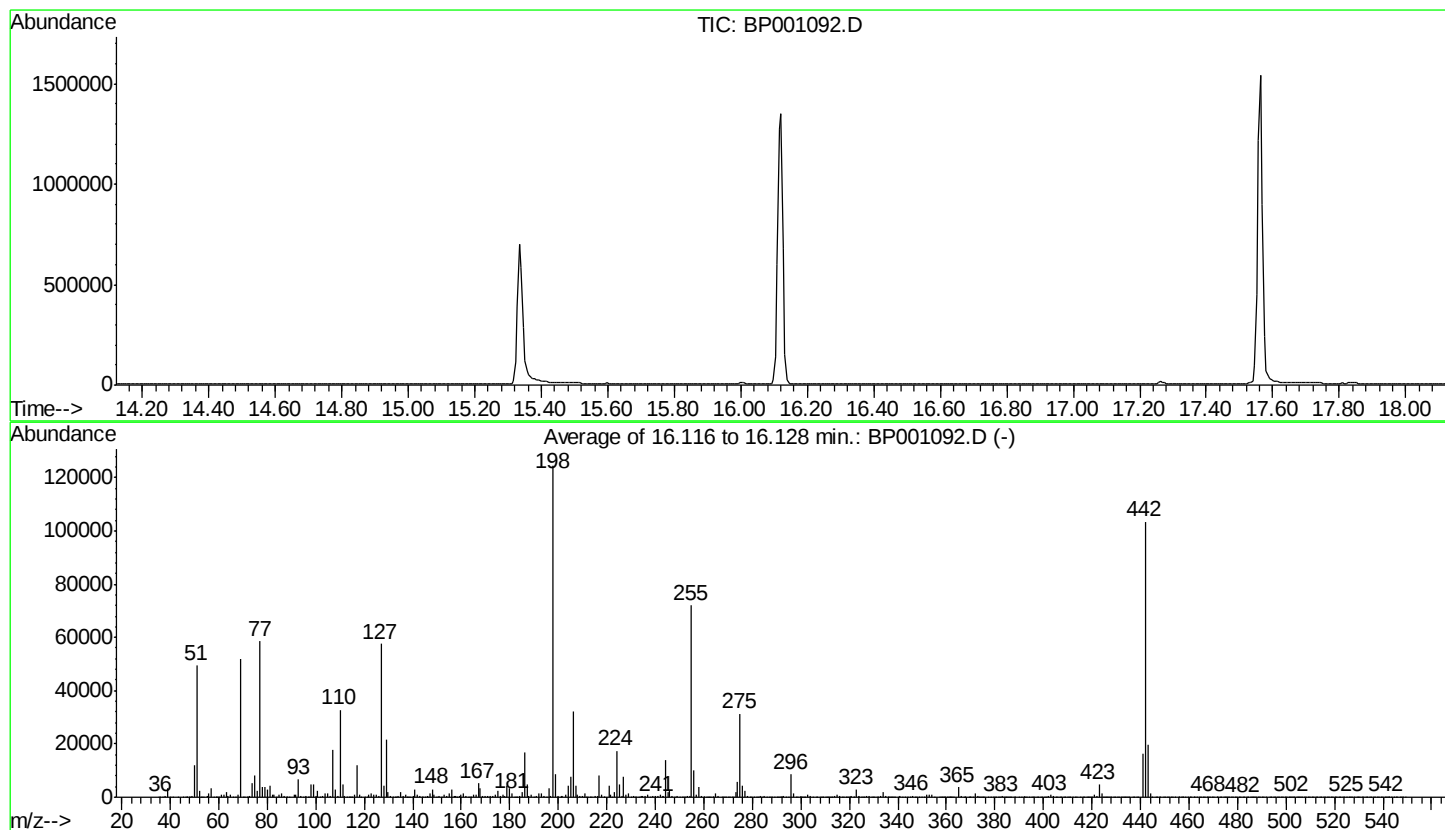

AutoFind: Scans 2385, 2386, 2387; Background Corrected with Scan 2378

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	49402	PASS
68	69	0.00	2	1.9	988	PASS
69	198	0.00	100	41.6	51813	PASS
70	69	0.00	2	0.4	202	PASS
127	198	10	80	46.2	57501	PASS
197	198	0.00	2	0.5	683	PASS
198	198	100	100	100.0	124485	PASS
199	198	5	9	6.8	8496	PASS
275	198	10	60	25.2	31333	PASS
365	198	1	100	3.1	3808	PASS
441	198	0.01	100	13.3	16567	PASS
442	198	50	100	83.1	103400	PASS
443	442	15	24	19.1	19709	PASS