


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP112719\
 Data File : BP001110.D
 Acq On : 28 Nov 2019 06:07
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 27 17:38:46 2019

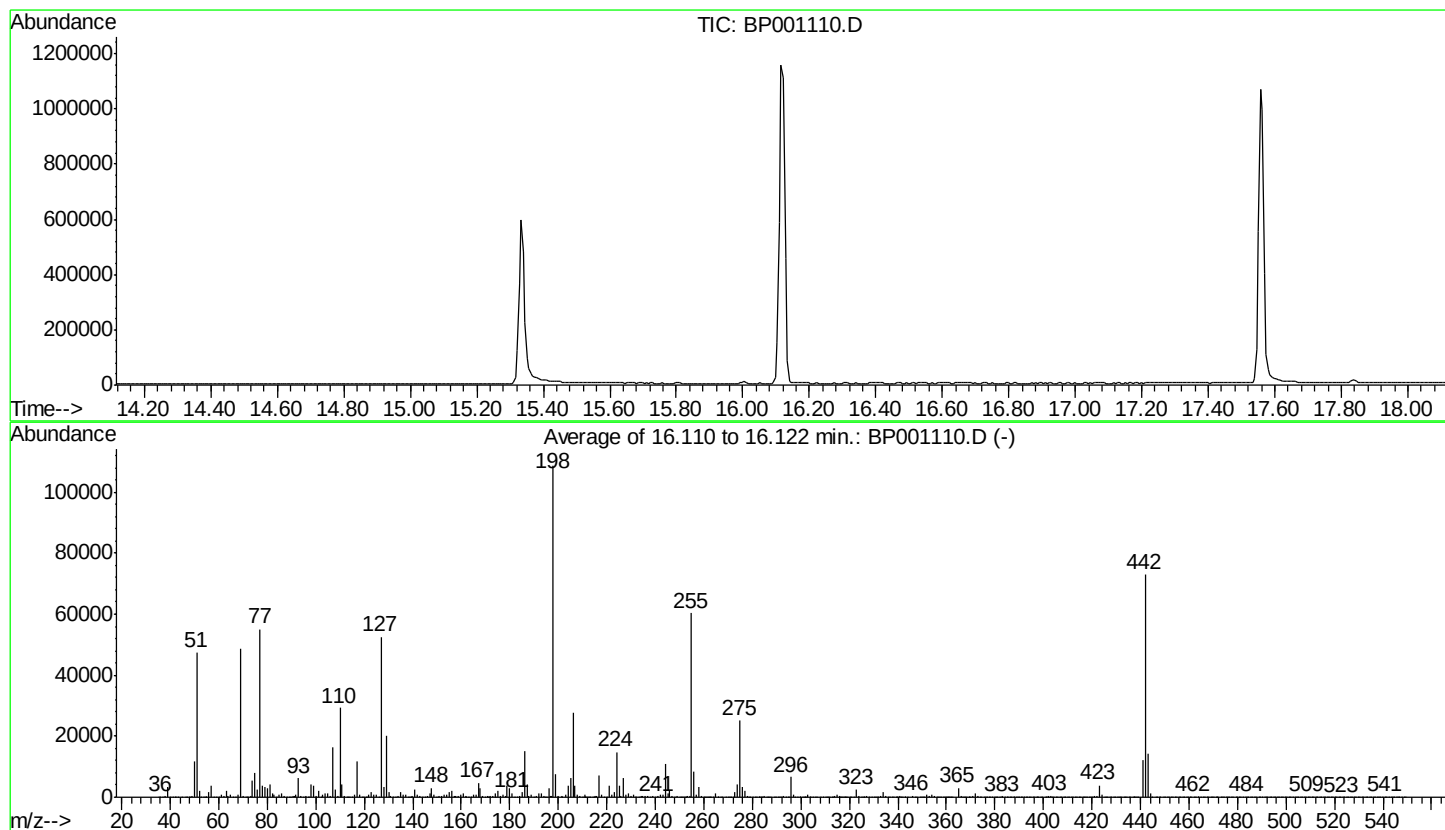

AutoFind: Scans 2384, 2385, 2386; Background Corrected with Scan 2375

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	47403	PASS
68	69	0.00	2	1.8	888	PASS
69	198	0.00	100	44.9	48838	PASS
70	69	0.00	2	0.6	270	PASS
127	198	10	80	48.3	52450	PASS
197	198	0.00	2	0.4	484	PASS
198	198	100	100	100.0	108688	PASS
199	198	5	9	6.8	7407	PASS
275	198	10	60	23.2	25166	PASS
365	198	1	100	2.8	3049	PASS
441	198	0.01	100	11.1	12040	PASS
442	198	50	100	67.1	72970	PASS
443	442	15	24	19.5	14245	PASS