

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM112723\  
 Data File : BM043053.D  
 Acq On : 27 Nov 2023 17:35  
 Operator : MA/JU  
 Sample : PB157274BL  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :

Quant Time: Nov 28 00:22:51 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM112423.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Nov 27 02:36:19 2023  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min)    |
|-----------------------------|--------|------|----------|-------|--------|-------------|
| -----                       |        |      |          |       |        |             |
| Internal Standards          |        |      |          |       |        |             |
| 1) 1,4-Dichlorobenzene-d4   | 7.805  | 152  | 882      | 0.400 | ng/ul  | #-0.08      |
| 4) Naphthalene-d8           | 10.605 | 136  | 2970     | 0.400 | ng/ul  | #-0.04      |
| 9) Acenaphthene-d10         | 14.454 | 164  | 1644     | 0.400 | ng/ul  | -0.01       |
| 13) Phenanthrene-d10        | 17.304 | 188  | 329950   | 0.400 | ng/ul  | # 0.07      |
| 17) Chrysene-d12            | 21.424 | 240  | 2087     | 0.400 | ng/ul  | 0.00        |
| 23) Perylene-d12            | 0.000  | 264  | 0        | 0.000 | ng/ul  | -23.78      |
| System Monitoring Compounds |        |      |          |       |        |             |
| 3) 1,4-Dioxane-d8           | 3.155  | 96   | 5849     | 4.322 | ng/ul  | -0.01       |
| 6) 2-Methylnaphthalene-d10  | 12.244 | 152  | 1061     | 0.267 | ng/ul  | 0.00        |
| 18) Fluoranthene-d10        | 19.242 | 212  | 2875     | 0.378 | ng/ul  | -0.02       |
| Target Compounds            |        |      |          |       |        |             |
| 20) Pyrene                  | 19.600 | 202  | 709      | 0.056 | ng/ul# | Qvalue<br>1 |
| -----                       |        |      |          |       |        |             |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM112723\  
Data File : BM043053.D  
Acq On : 27 Nov 2023 17:35  
Operator : MA/JU  
Sample : PB157274BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :


Quant Time: Nov 28 00:22:51 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM112423.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 27 02:36:19 2023  
Response via : Initial Calibration

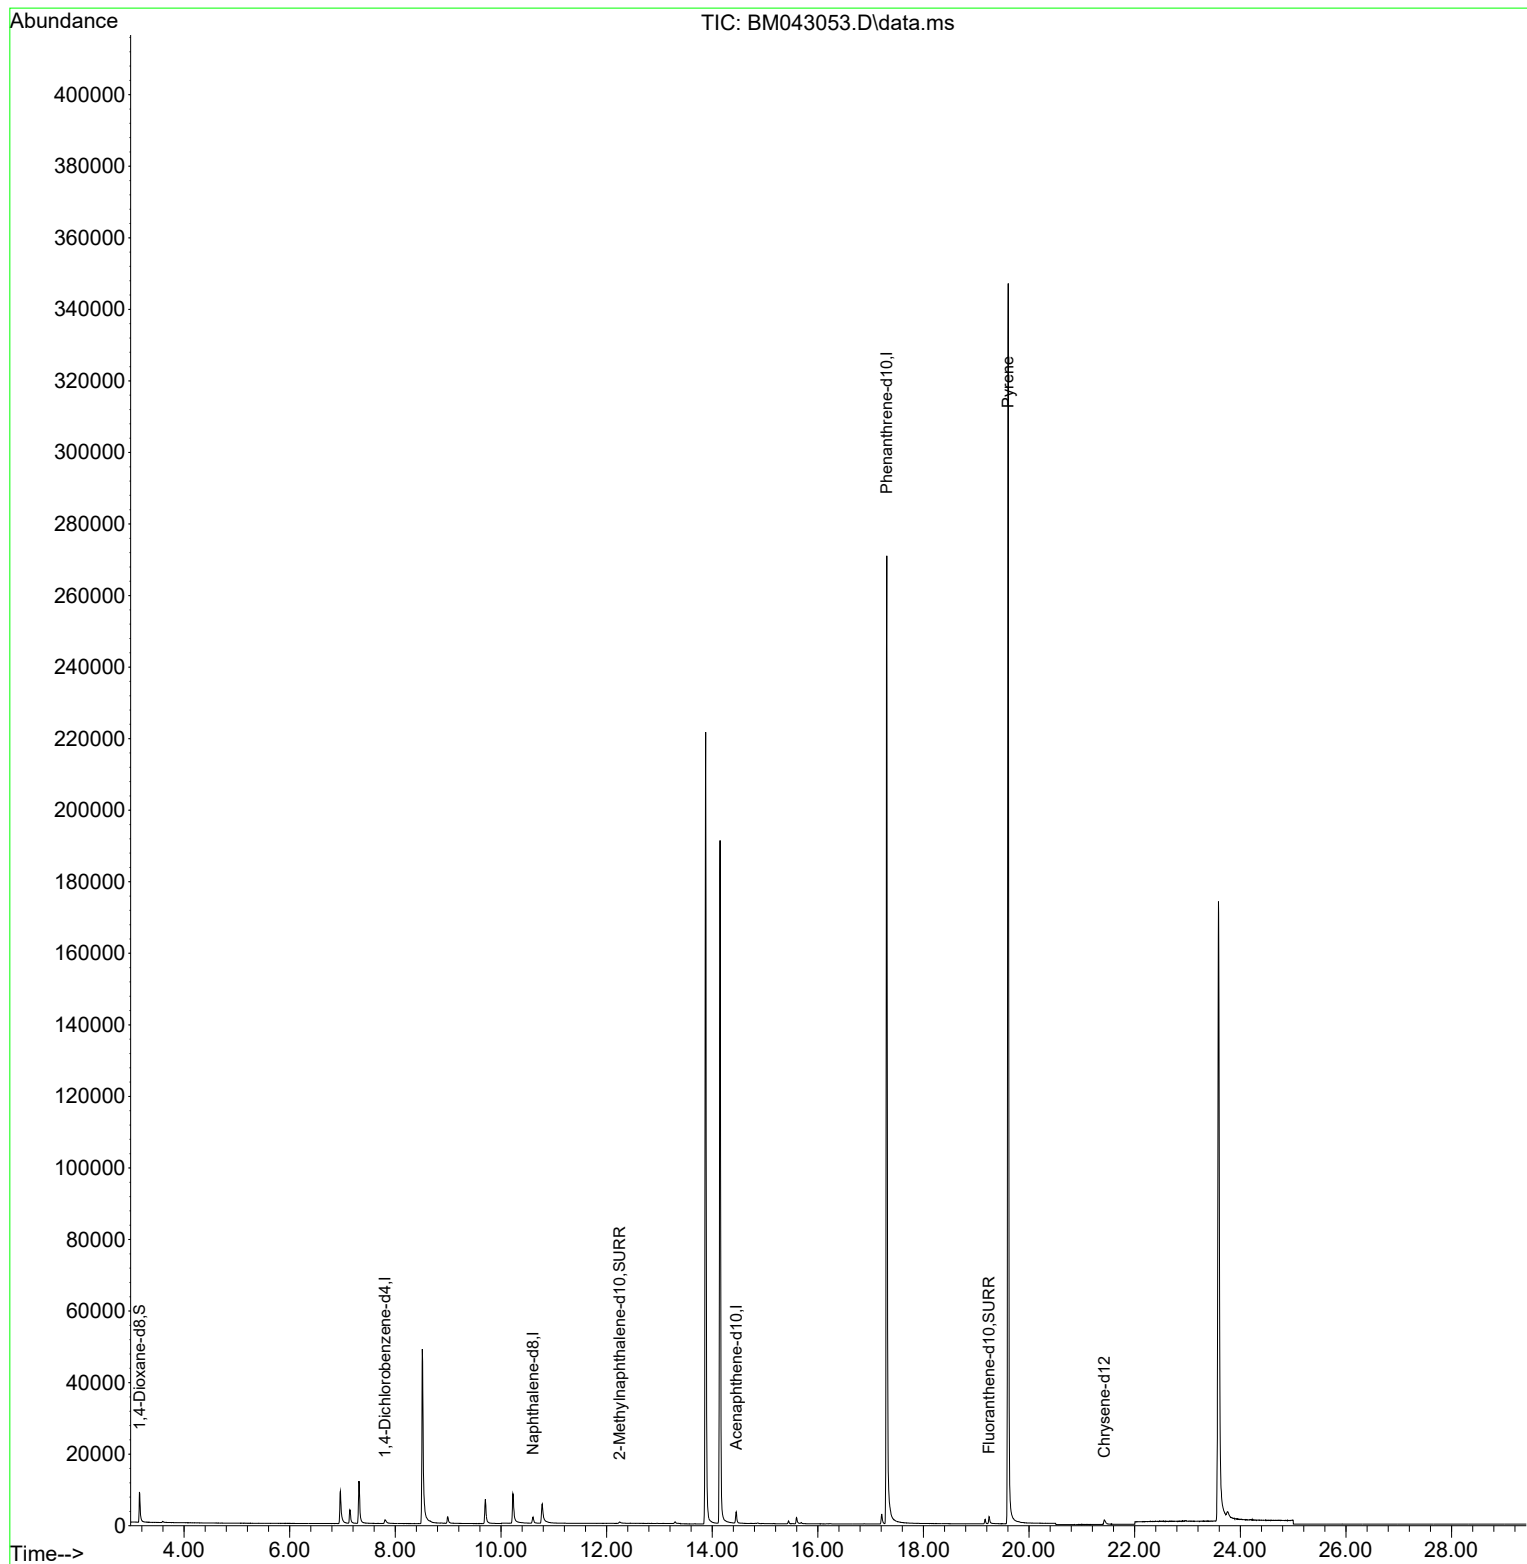

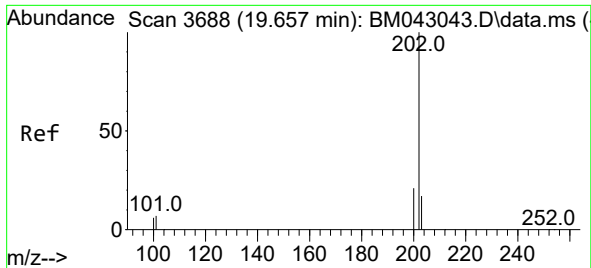

#20  
 Pyrene  
 Concen: 0.056 ng/ul  
 RT: 19.600 min Scan# 30  
 Delta R.T. -0.060 min  
 Lab File: BM043053.D  
 Acq: 27 Nov 2023 17:35

Instrument :  
 BNA\_P  
 ClientSampleId :

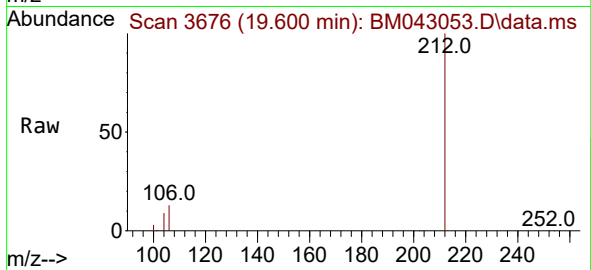

Tgt Ion:202 Resp: 709  
 Ion Ratio Lower Upper  
 202 100  
 101 187.1 8.7 13.1#  
 100 1556.4 7.8 11.8#

