




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018404.D
 Acq On : 27 Nov 2023 17:13
 Operator : MA/JU
 Sample : 05341-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF2

Manual IntegrationsAPPROVED

Quant Time: Nov 27 21:57:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 27 21:50:01 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 12/01/2023

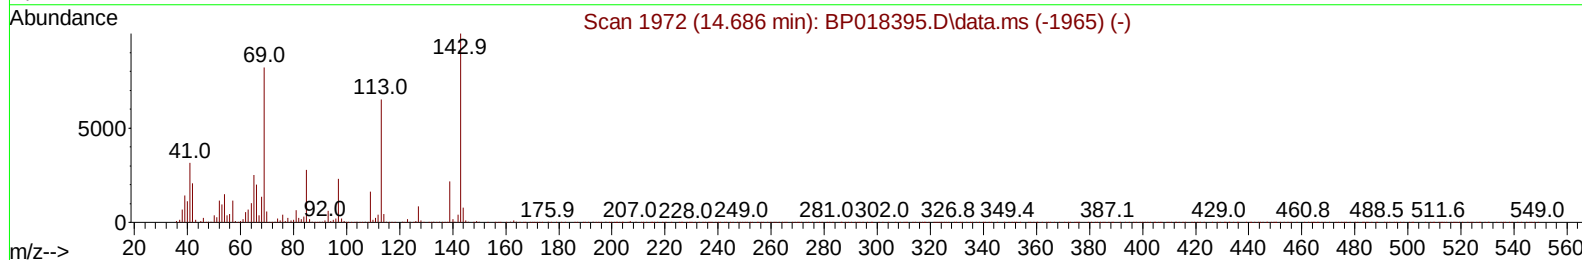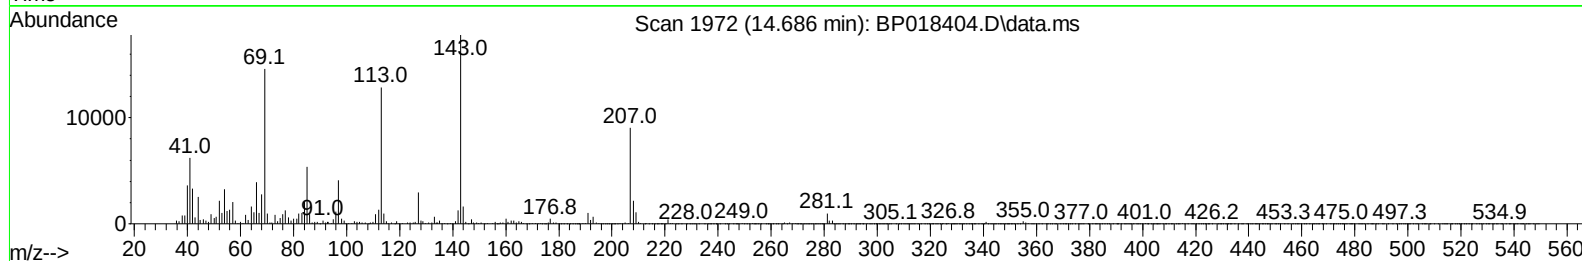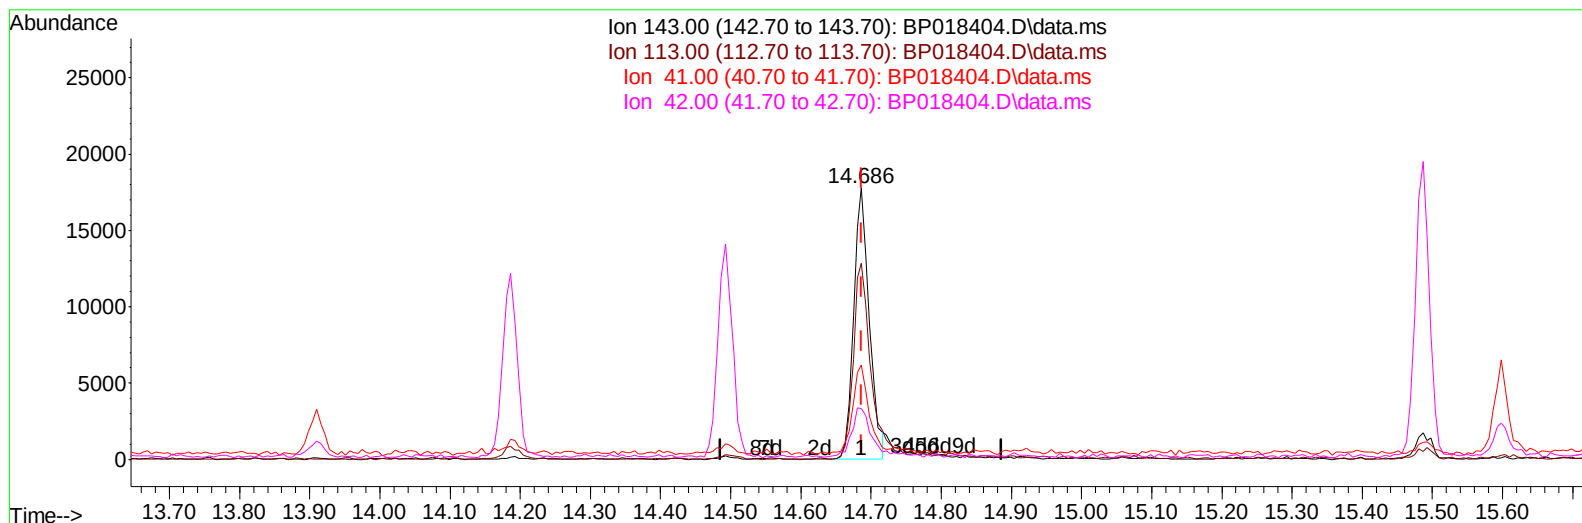

TIC: BP018404.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (+ 0.000) 2.41 ng/ul

response 27584

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.70	72.30
41.00	36.10	34.78
42.00	25.00	18.72#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018404.D
 Acq On : 27 Nov 2023 17:13
 Operator : MA/JU
 Sample : 05341-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF2

Manual IntegrationsAPPROVED

Quant Time: Nov 27 21:57:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 27 21:50:01 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 12/01/2023

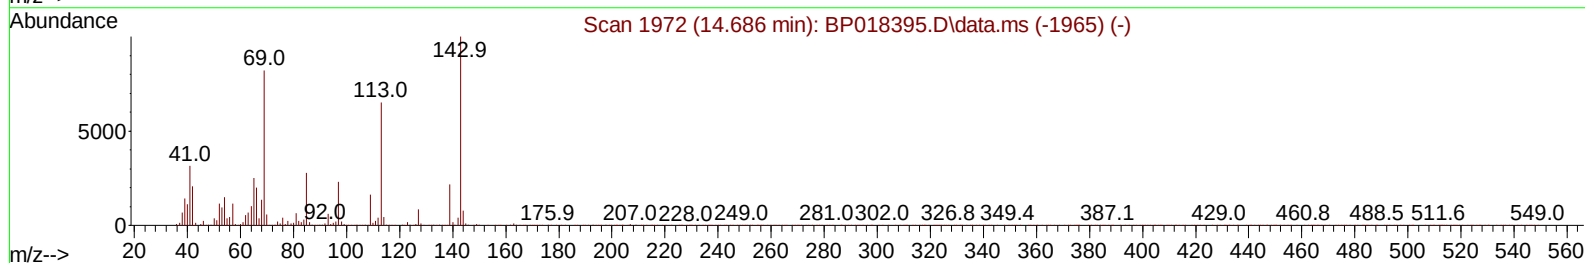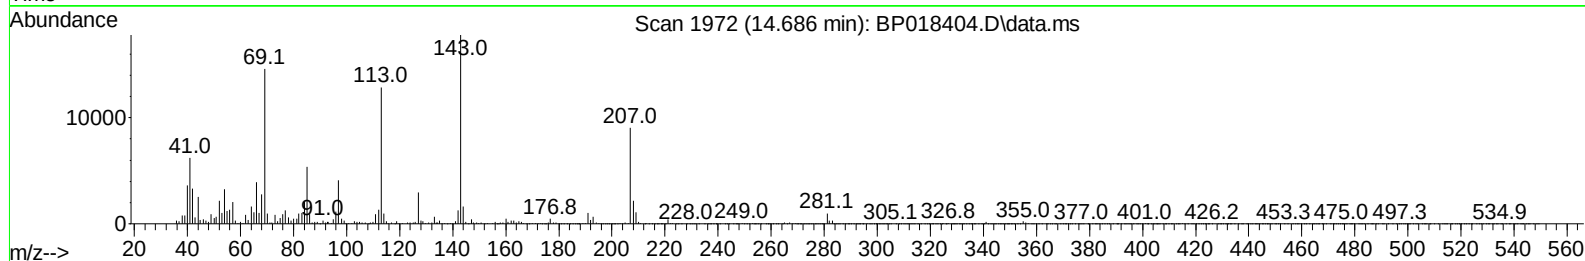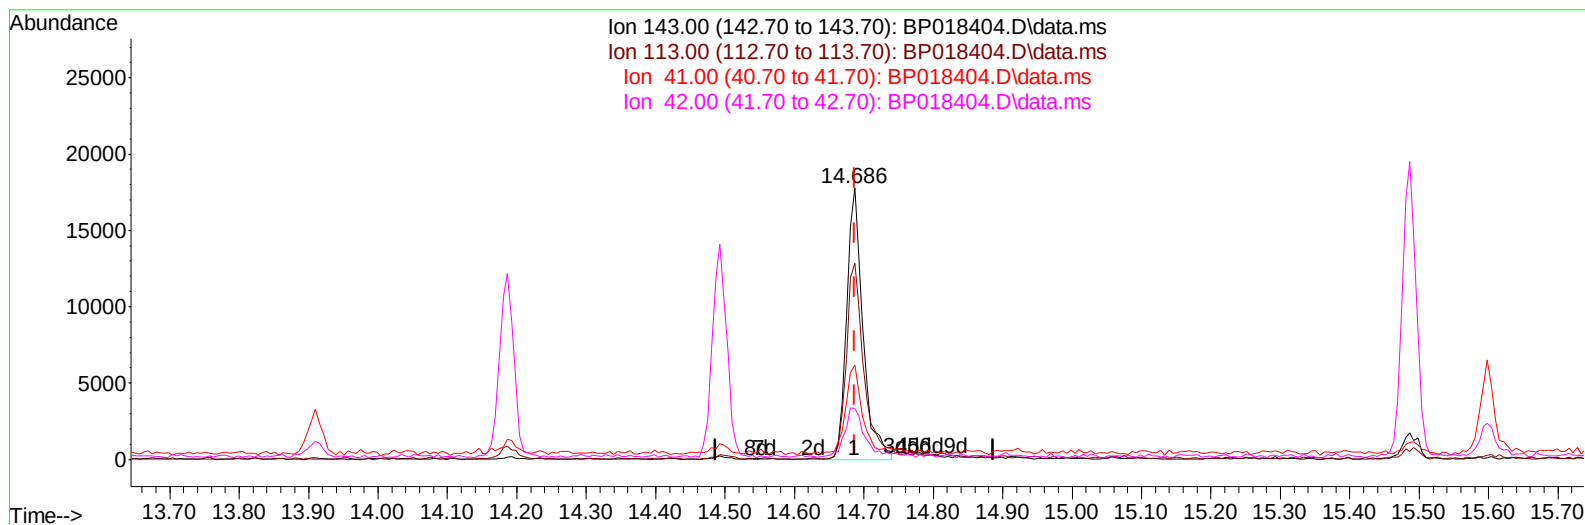

TIC: BP018404.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (+ 0.000) 2.53 ng/ul m

response 28980

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.70	72.30
41.00	36.10	34.78
42.00	25.00	18.72#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018404.D
 Acq On : 27 Nov 2023 17:13
 Operator : MA/JU
 Sample : 05341-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 12/01/2023

Quant Time: Nov 27 22:22:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 27 21:50:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	435755	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	1639349	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	932029	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	2061654	20.000	ng/ul	0.00
79) Chrysene-d12	21.374	240	2094840	20.000	ng/ul	0.00
88) Perylene-d12	23.880	264	2386451	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	45202	3.885	ng/uL	0.00
4) Pyridine-d5	3.693	84	151639	4.743	ng/ul	0.00
7) Phenol-d5	7.022	99	163400	4.103	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.193	67	454904	19.103	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	519794	15.546	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	298993	9.303	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	298861	22.445	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	262578	21.353	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	542260	18.277	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	657620	16.435	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	1776993	21.427	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	2018855	21.364	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	28980m	2.531	ng/ul	0.00
60) Fluorene-d10	15.486	176	1601281	23.084	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	123301	14.049	ng/ul	0.00
73) Anthracene-d10	17.345	188	2771146	25.148	ng/ul	0.00
81) Pyrene-d10	19.592	212	3378558	20.264	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.715	264	3450612	24.940	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018404.D
Acq On : 27 Nov 2023 17:13
Operator : MA/JU
Sample : 05341-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 12/01/2023

Quant Time: Nov 27 22:22:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 27 21:50:01 2023
Response via : Initial Calibration

