

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018440.D
 Acq On : 28 Nov 2023 14:43
 Operator : MA/JU
 Sample : 05416-07
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK3

Quant Time: Nov 29 01:13:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 28 08:59:50 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	414071	20.000	ng/u1	0.00
20) Naphthalene-d8	10.652	136	1557075	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.493	164	812367	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	1545047	20.000	ng/u1	0.00
79) Chrysene-d12	21.410	240	1576935	20.000	ng/u1	0.01
88) Perylene-d12	24.027	264	1834069	20.000	ng/u1	0.06
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	21055	1.905	ng/uL	0.00
4) Pyridine-d5	3.687	84	61941	2.039	ng/u1	0.00
7) Phenol-d5	7.017	99	320415	8.467	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	201690	8.913	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	283036	8.908	ng/u1	0.00
15) 4-Methylphenol-d8	8.564	113	173791	5.691	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	119678	9.463	ng/u1	0.00
24) 2-Nitrophenol-d4	9.740	143	107871	9.235	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	238149	8.451	ng/u1	0.00
31) 4-Chloroaniline-d4	10.793	131	197625	5.200	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	688341	9.523	ng/u1	0.00
49) Acenaphthylene-d8	14.181	160	780911	9.481	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	63518	6.365	ng/u1	0.00
60) Fluorene-d10	15.487	176	577861	9.558	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	40333	6.132	ng/u1	0.00
73) Anthracene-d10	17.340	188	819979	9.929	ng/u1	0.00
81) Pyrene-d10	19.598	212	1086790	8.659	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	1096541	10.312	ng/u1	0.05
Target Compounds						
16) Acetophenone	8.681	105	116184	2.486	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018440.D
Acq On : 28 Nov 2023 14:43
Operator : MA/JU
Sample : 05416-07
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK3


Quant Time: Nov 29 01:13:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 28 08:59:50 2023
Response via : Initial Calibration

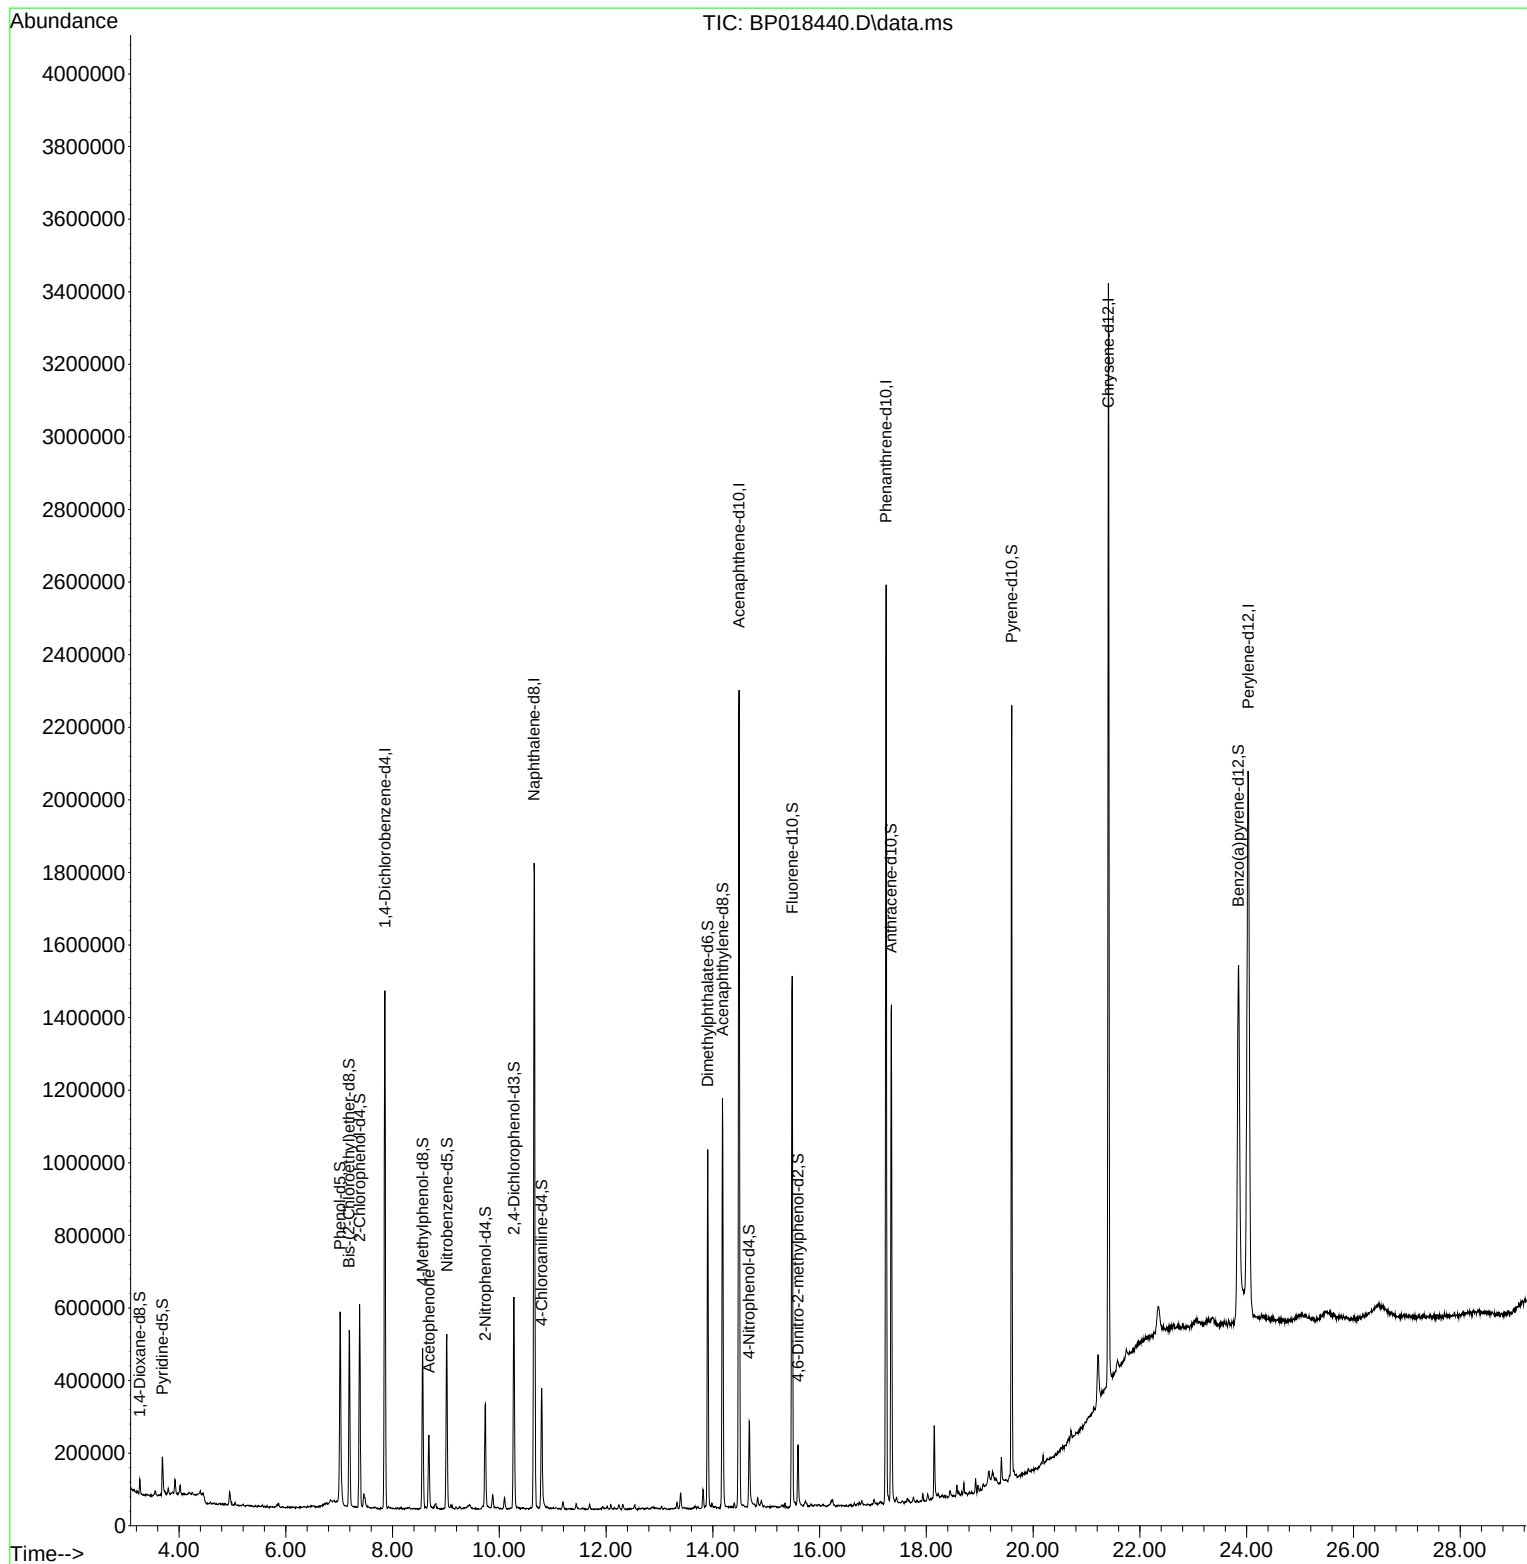

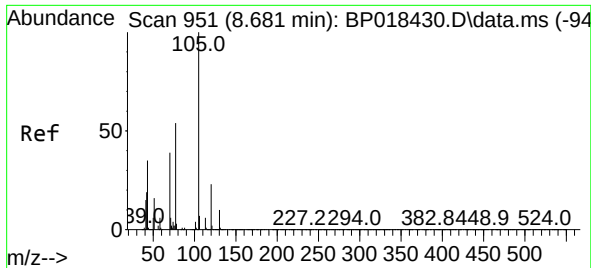

#16
 Acetophenone
 Concen: 2.486 ng/ul
 RT: 8.681 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP018440.D
 Acq: 28 Nov 2023 14:43

Instrument :
 BNA_P
 ClientSampleId :
 C0AK3

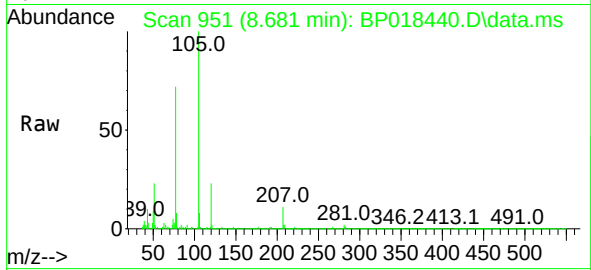

Tgt Ion:	105	Resp:	116184
Ion	Ratio	Lower	Upper
105	100		
77	71.5	59.5	89.3
51	22.7	20.5	30.7

