

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018441.D
 Acq On : 28 Nov 2023 15:17
 Operator : MA/JU
 Sample : 05416-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG6

Quant Time: Nov 29 01:14:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 28 08:59:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	406059	20.000	ng/u1	0.00
20) Naphthalene-d8	10.652	136	1602875	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.493	164	892861	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	1520946	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	1325943	20.000	ng/u1	0.02
88) Perylene-d12	24.039	264	1577593	20.000	ng/u1	0.08
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	21752	2.006	ng/uL	0.00
4) Pyridine-d5	3.687	84	72490	2.433	ng/u1	0.00
7) Phenol-d5	7.016	99	344676	9.288	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	212702	9.585	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	294258	9.444	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	192734	6.436	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	131581	10.107	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	117404	9.764	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	260414	8.977	ng/u1	0.00
31) 4-Chloroaniline-d4	10.793	131	204793	5.234	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	787141	9.908	ng/u1	0.00
49) Acenaphthylene-d8	14.181	160	879570	9.716	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	49898	4.550	ng/u1	0.00
60) Fluorene-d10	15.481	176	641340	9.651	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	36375	5.618	ng/u1	0.00
73) Anthracene-d10	17.345	188	797617	9.812	ng/u1	0.00
81) Pyrene-d10	19.598	212	903746	8.564	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	903836	9.882	ng/u1	0.06
Target Compounds						
					Qvalue	
16) Acetophenone	8.681	105	126852	2.768	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018441.D
Acq On : 28 Nov 2023 15:17
Operator : MA/JU
Sample : 05416-13
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG6


Quant Time: Nov 29 01:14:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 28 08:59:50 2023
Response via : Initial Calibration

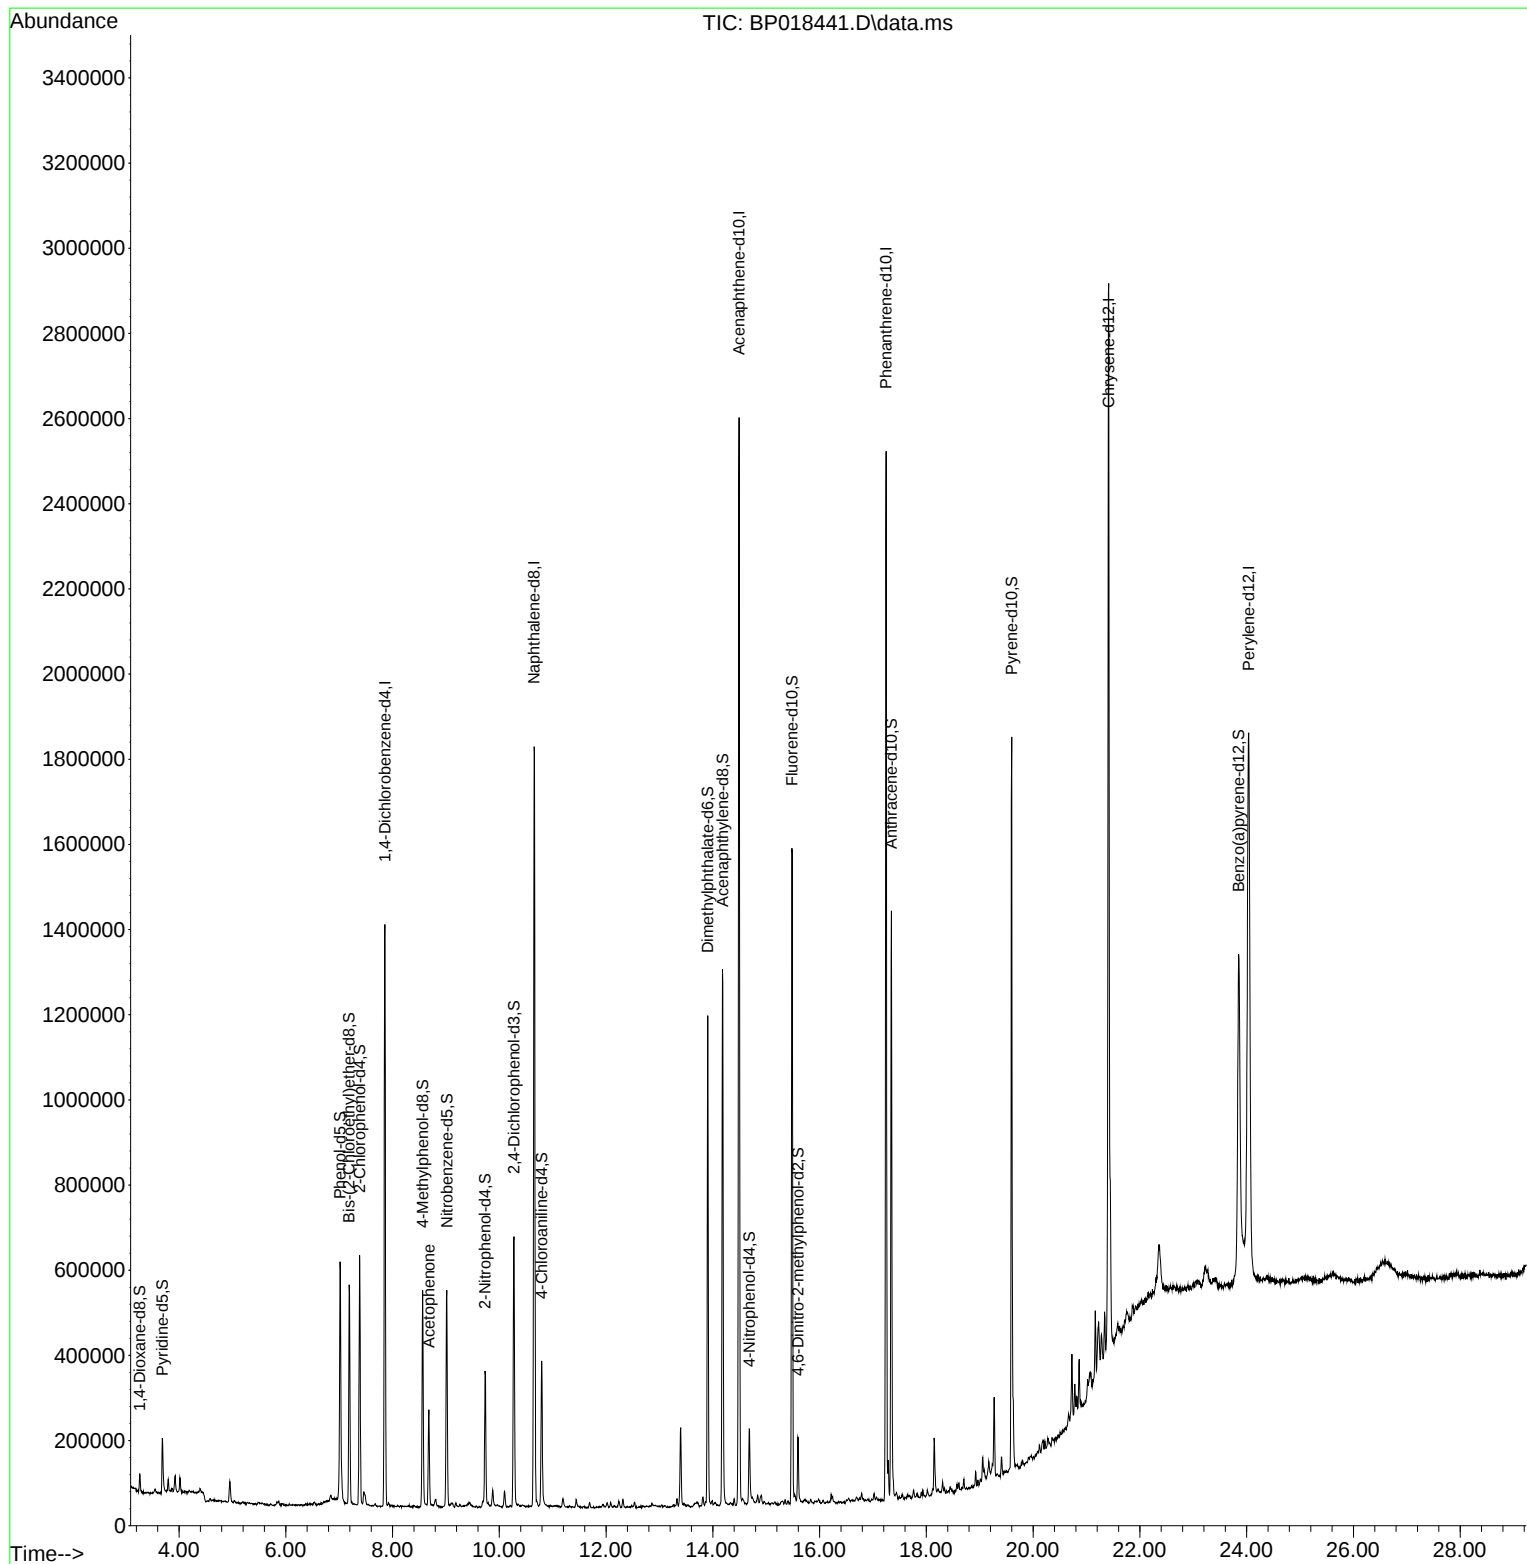

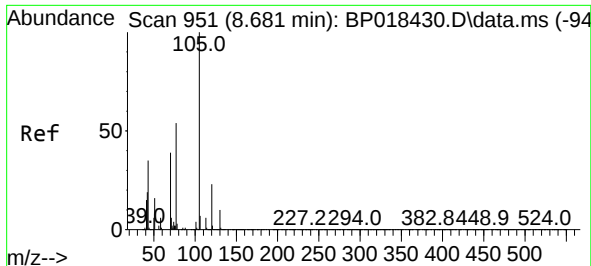

#16
Acetophenone
Concen: 2.768 ng/ul
RT: 8.681 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP018441.D
Acq: 28 Nov 2023 15:17

Instrument :
BNA_P
ClientSampleId :
C0AG6

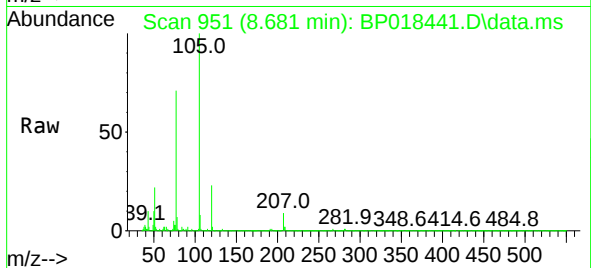

Tgt Ion:105 Resp: 126852
Ion Ratio Lower Upper
105 100
77 71.2 59.5 89.3
51 22.1 20.5 30.7

