

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018443.D
 Acq On : 28 Nov 2023 16:25
 Operator : MA/JU
 Sample : 05416-24
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH7

Quant Time: Nov 29 01:27:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 29 01:22:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	431460	20.000	ng/u1	0.00
20) Naphthalene-d8	10.651	136	1641533	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.492	164	915158	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	2042830	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	2083111	20.000	ng/u1	-0.02
88) Perylene-d12	24.062	264	2282626	20.000	ng/u1	-0.08
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	19445	1.688	ng/uL	0.00
4) Pyridine-d5	3.687	84	73849	2.333	ng/u1	0.00
7) Phenol-d5	7.016	99	321983	8.166	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	192377	8.159	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	275515	8.322	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	189077	5.942	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	113362	8.502	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	101816	8.269	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	234194	7.883	ng/u1	0.00
31) 4-Chloroaniline-d4	10.793	131	256517	6.402	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	689417	8.466	ng/u1	0.00
49) Acenaphthylene-d8	14.181	160	796334	8.582	ng/u1	0.00
54) 4-Nitrophenol-d4	14.686	143	33729	3.000	ng/u1	0.00
60) Fluorene-d10	15.481	176	642777	9.437	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	20093	2.311	ng/u1	0.00
73) Anthracene-d10	17.345	188	1026277	9.399	ng/u1	0.00
81) Pyrene-d10	19.598	212	1427716	8.612	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.874	264	1342944	10.148	ng/u1	-0.08
Target Compounds						
					Qvalue	
16) Acetophenone	8.681	105	106362	2.184	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018443.D
Acq On : 28 Nov 2023 16:25
Operator : MA/JU
Sample : 05416-24
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH7


Quant Time: Nov 29 01:27:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 29 01:22:40 2023
Response via : Initial Calibration

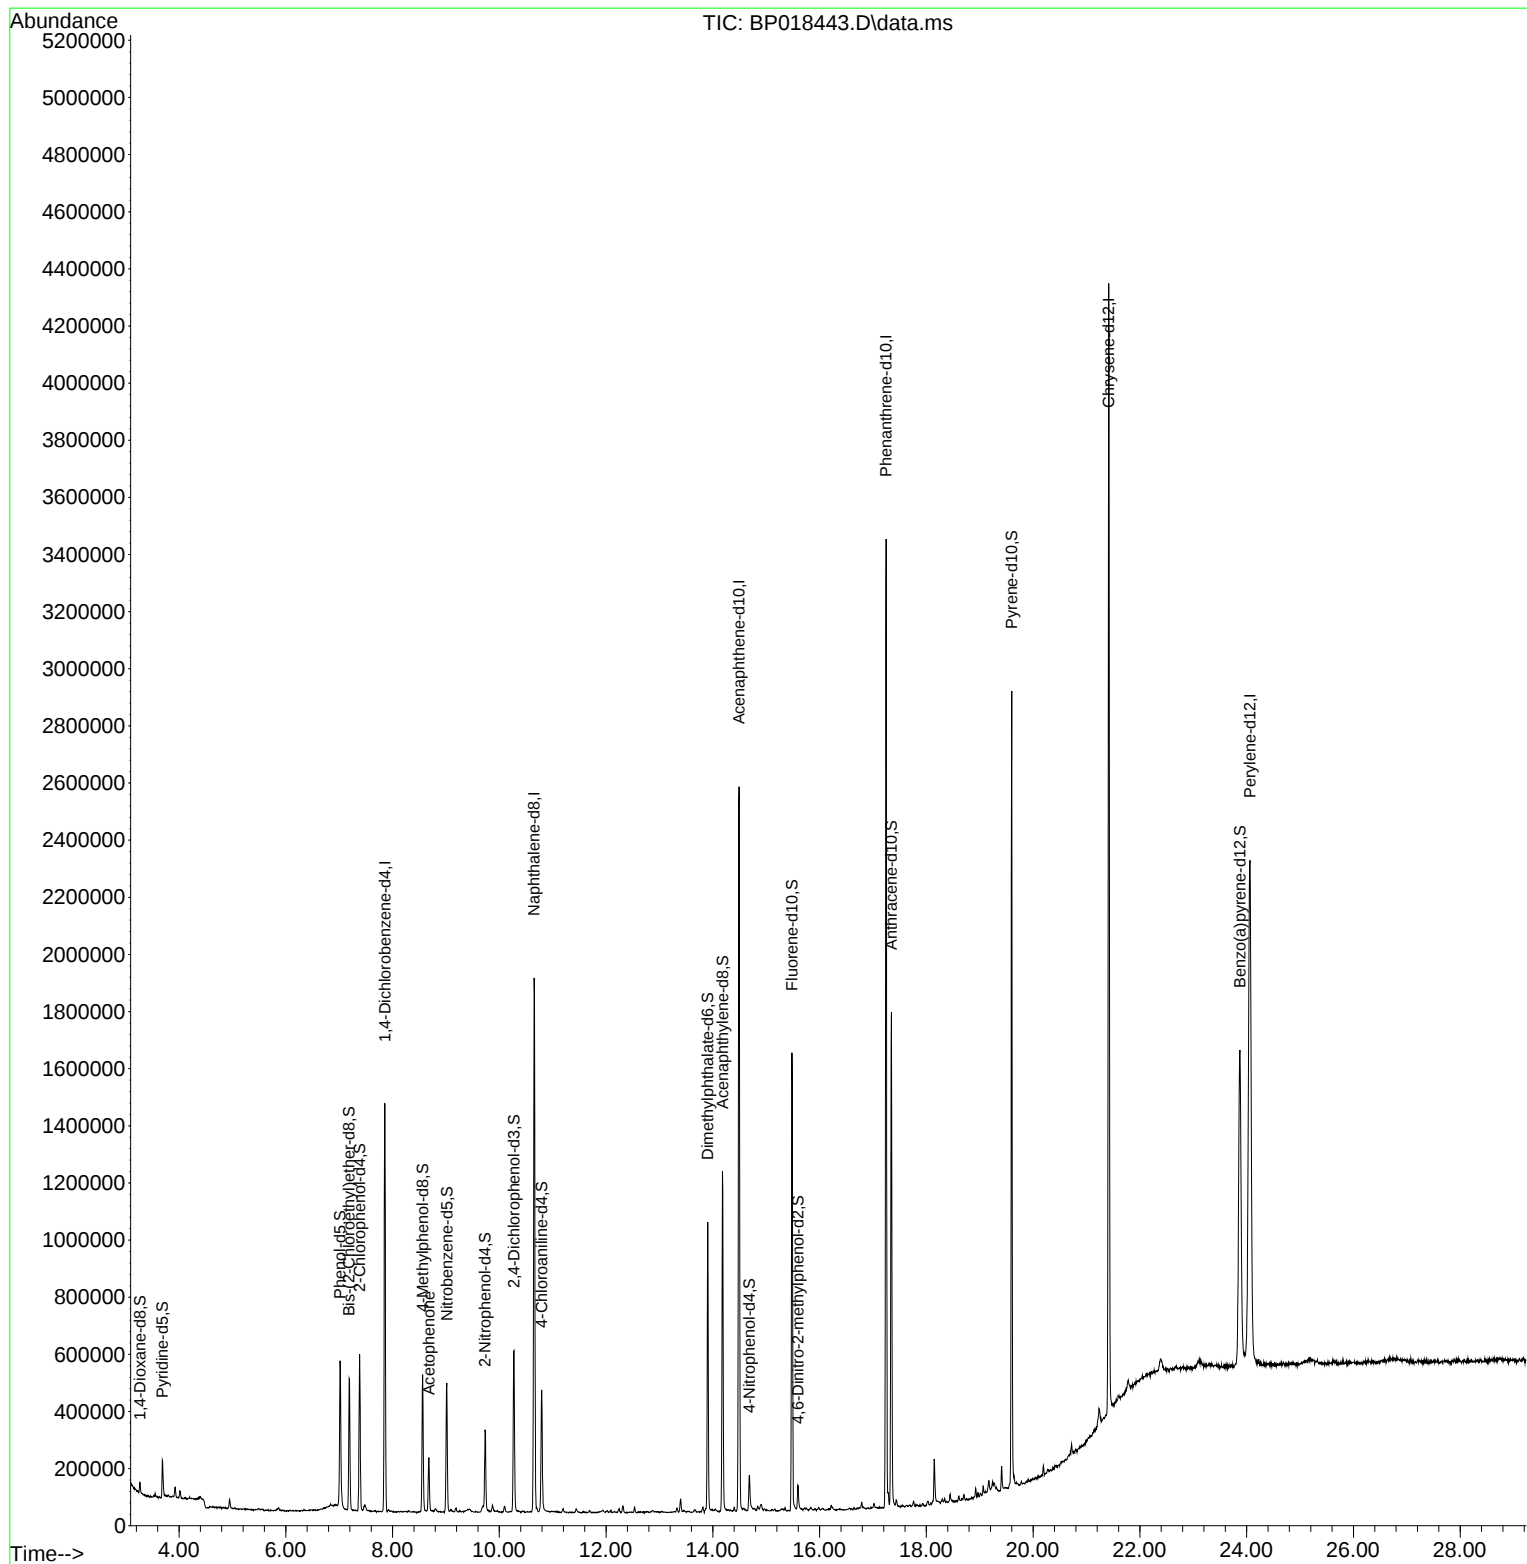

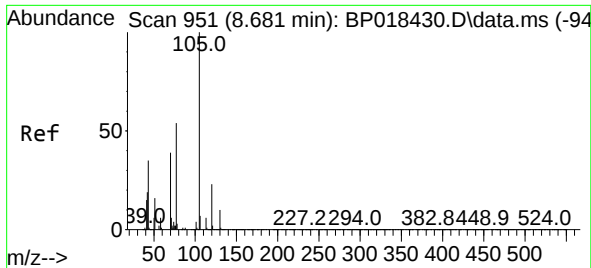

#16
 Acetophenone
 Concen: 2.184 ng/ul
 RT: 8.681 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP018443.D
 Acq: 28 Nov 2023 16:25

Instrument :
 BNA_P
 ClientSampleId :
 C0AH7

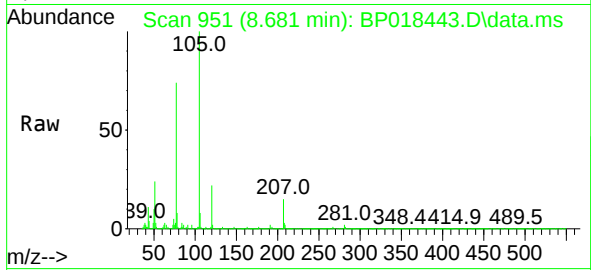

Tgt Ion:105 Resp: 106362
 Ion Ratio Lower Upper
 105 100
 77 74.0 59.5 89.3
 51 23.5 20.5 30.7

