

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018444.D
 Acq On : 28 Nov 2023 16:59
 Operator : MA/JU
 Sample : 05416-25
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH8

Quant Time: Nov 29 01:28:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 29 01:22:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	483756	20.000	ng/u1	0.00
20) Naphthalene-d8	10.652	136	1834026	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.493	164	1003499	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	1929833	20.000	ng/u1	0.00
79) Chrysene-d12	21.422	240	1931904	20.000	ng/u1	-0.02
88) Perylene-d12	24.069	264	2286420	20.000	ng/u1	-0.07
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	23197	1.796	ng/uL	0.00
4) Pyridine-d5	3.687	84	105985	2.986	ng/u1	0.00
7) Phenol-d5	7.022	99	367363	8.309	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	220880	8.355	ng/u1	0.00
11) 2-Chlorophenol-d4	7.387	132	311061	8.380	ng/u1	0.00
15) 4-Methylphenol-d8	8.564	113	263890	7.396	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	131895	8.854	ng/u1	0.00
24) 2-Nitrophenol-d4	9.740	143	112290	8.162	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	251057	7.564	ng/u1	0.00
31) 4-Chloroaniline-d4	10.793	131	256731	5.735	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	729256	8.167	ng/u1	0.00
49) Acenaphthylene-d8	14.181	160	836357	8.220	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	32628	2.647	ng/u1	0.00
60) Fluorene-d10	15.481	176	642730	8.606	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	17976	2.188	ng/u1	0.00
73) Anthracene-d10	17.340	188	998597	9.681	ng/u1	0.00
81) Pyrene-d10	19.598	212	1343868	8.740	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	1425389	10.753	ng/u1	-0.07
Target Compounds						
					Qvalue	
16) Acetophenone	8.681	105	103436	1.895	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018444.D
Acq On : 28 Nov 2023 16:59
Operator : MA/JU
Sample : 05416-25
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH8


Quant Time: Nov 29 01:28:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 29 01:22:40 2023
Response via : Initial Calibration

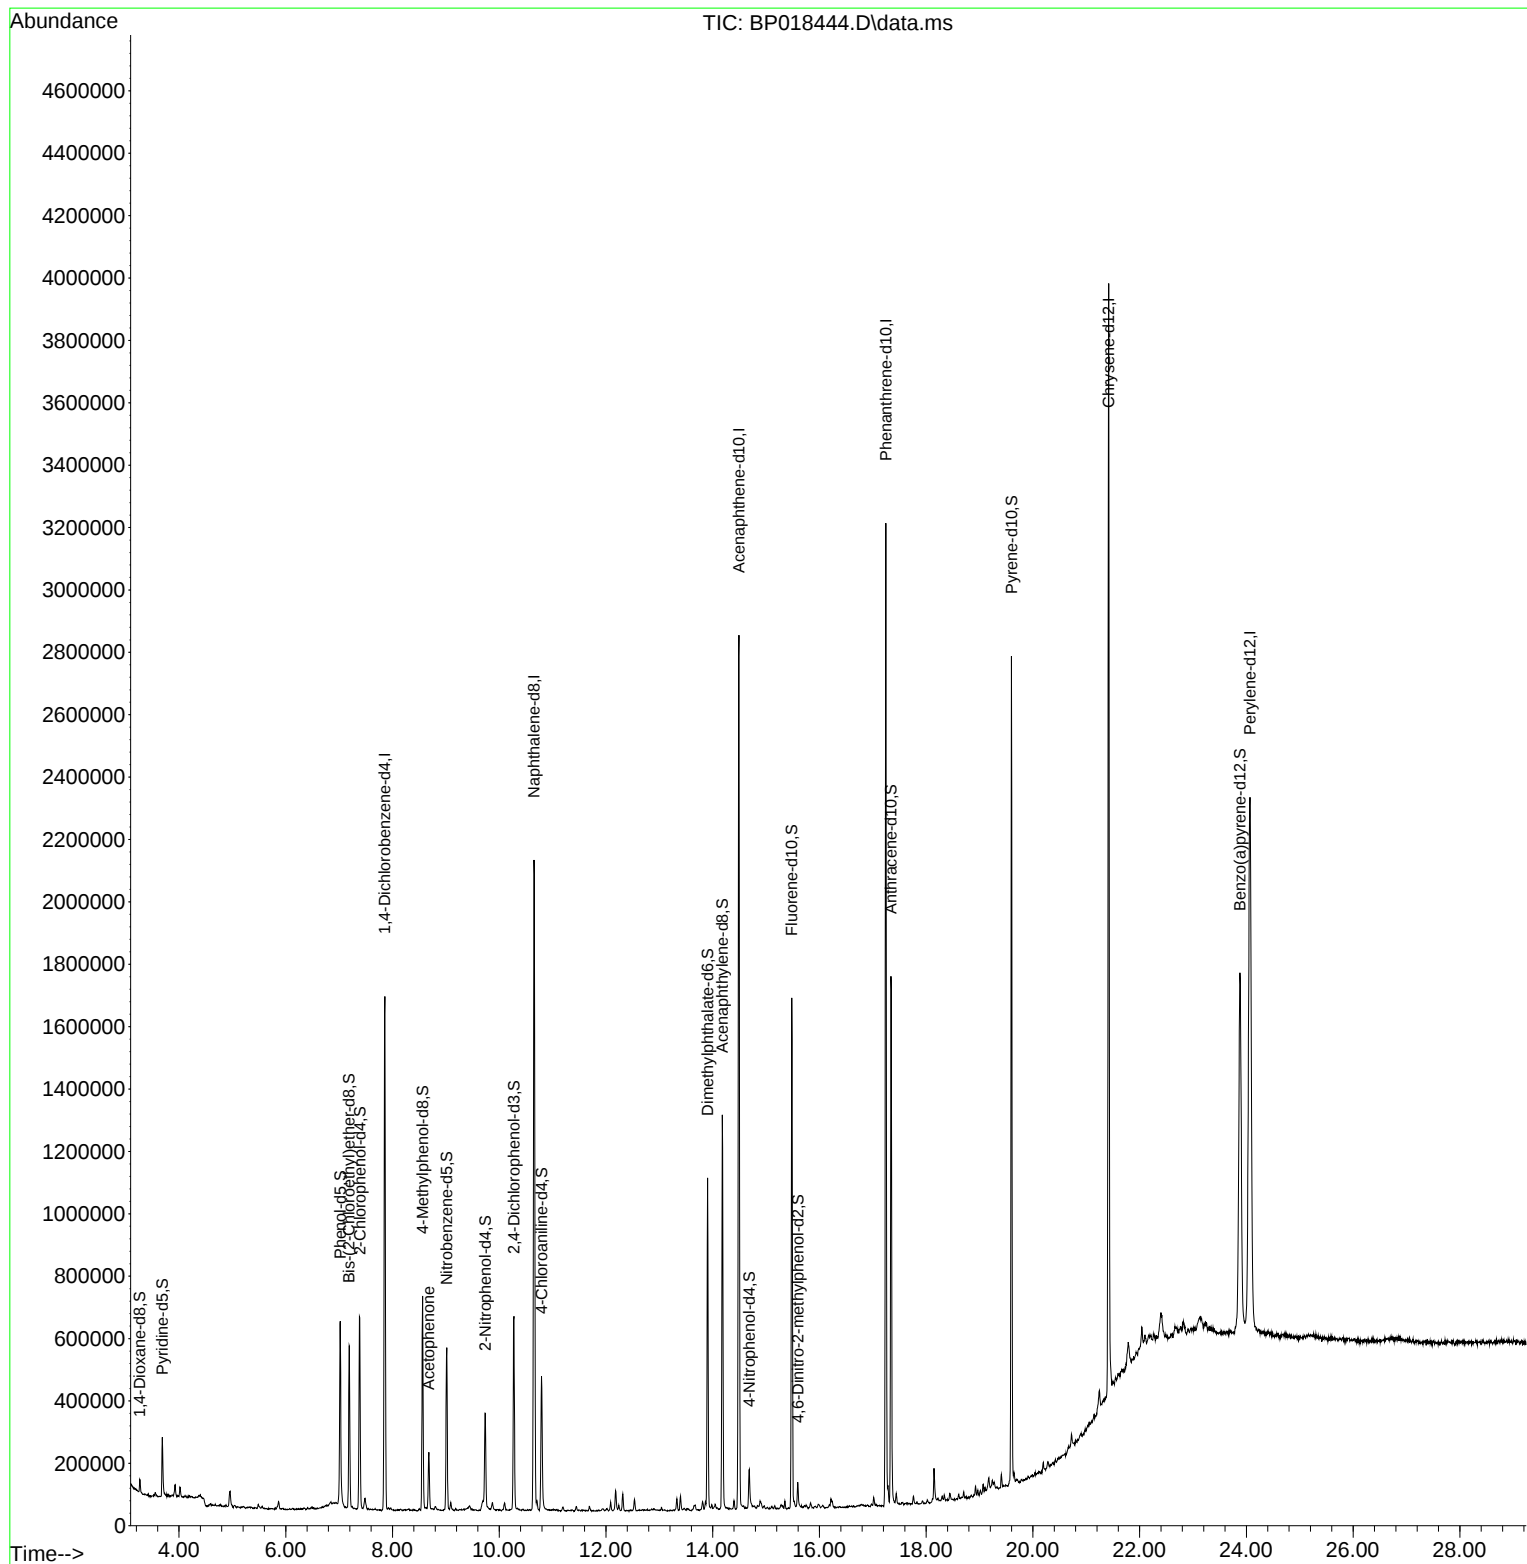

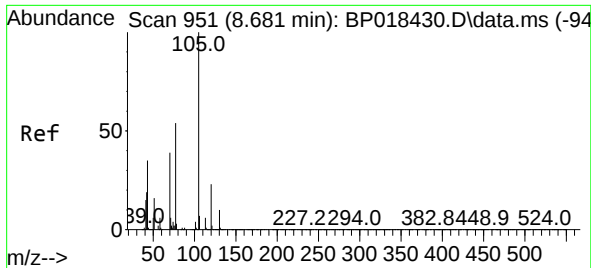

#16
Acetophenone
Concen: 1.895 ng/ul
RT: 8.681 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP018444.D
Acq: 28 Nov 2023 16:59

Instrument :
BNA_P
ClientSampleId :
C0AH8

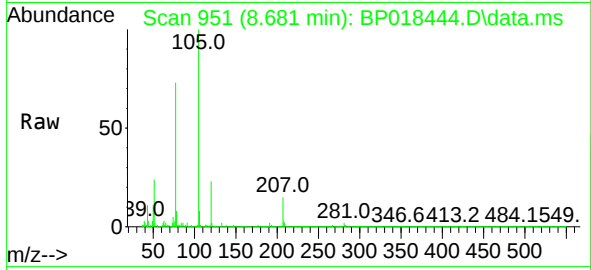

Tgt Ion:105 Resp: 103436
Ion Ratio Lower Upper
105 100
77 72.6 59.5 89.3
51 24.4 20.5 30.7

