

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018396.D
 Acq On : 27 Nov 2023 12:41
 Operator : MA/JU
 Sample : PB157279BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	36	rVB	119444	149476	2.09%	0.216%
2	3.675	96	100	118	rBV	1283672	1856556	25.94%	2.684%
3	4.017	154	158	161	rVB	18519	24003	0.34%	0.035%
4	7.016	661	668	680	rVB	1381355	2098562	29.32%	3.034%
5	7.187	691	697	709	rVB	1242785	1860787	26.00%	2.690%
6	7.381	723	730	744	rBV	1487563	2262758	31.62%	3.271%
7	7.852	803	810	819	rVB	1134665	1761824	24.62%	2.547%
8	8.175	860	865	868	rVB6	5660	7583	0.11%	0.011%
9	8.563	923	931	942	rBV	1606688	2551454	35.65%	3.688%
10	9.016	1000	1008	1015	rBV	1206750	1917216	26.79%	2.771%
11	9.434	1077	1079	1086	rVB7	6034	8657	0.12%	0.013%
12	9.740	1118	1131	1141	rBV	790709	1333922	18.64%	1.928%
13	10.275	1214	1222	1236	rBV	1488134	2500126	34.94%	3.614%
14	10.657	1279	1287	1296	rVB	1364880	2286240	31.95%	3.305%
15	10.793	1303	1310	1318	rBV	1502510	2481559	34.68%	3.587%
16	11.469	1418	1425	1428	rBV9	3426	8124	0.11%	0.012%
17	12.245	1551	1557	1561	rBV2	31320	49551	0.69%	0.072%
18	12.451	1590	1592	1598	rVB7	4868	8474	0.12%	0.012%
19	12.845	1653	1659	1660	rBV5	10451	13826	0.19%	0.020%
20	12.863	1660	1662	1668	rVB6	8697	13898	0.19%	0.020%
21	13.287	1732	1734	1741	rVB7	5881	8660	0.12%	0.013%
22	13.404	1749	1754	1758	rBV4	16600	27078	0.38%	0.039%
23	13.463	1761	1764	1770	rVV7	6302	12930	0.18%	0.019%
24	13.781	1813	1818	1822	rBV8	5839	13128	0.18%	0.019%
25	13.910	1834	1840	1852	rBV	2364287	3204992	44.79%	4.633%
26	14.187	1880	1887	1905	rBV	2798417	4081657	57.04%	5.900%
27	14.492	1933	1939	1949	rVB	1796405	2565551	35.85%	3.709%
28	14.687	1966	1972	1983	rBV	805161	1201551	16.79%	1.737%
29	15.492	2101	2109	2121	rBV	3345095	5007145	69.97%	7.238%
30	15.604	2121	2128	2140	rVV	517486	752473	10.51%	1.088%
31	15.728	2146	2149	2158	rVB3	17228	31431	0.44%	0.045%
32	16.751	2319	2323	2328	rVB4	16632	23728	0.33%	0.034%
33	16.928	2350	2353	2357	rVB5	7436	7915	0.11%	0.011%
34	17.033	2367	2371	2374	rBV6	4998	8402	0.12%	0.012%
35	17.122	2381	2386	2389	rBV7	11269	19047	0.27%	0.028%
36	17.251	2401	2408	2418	rBV	1885321	2813538	39.32%	4.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018396.D
Acq On : 27 Nov 2023 12:41
Operator : MA/JU
Sample : PB157279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	17.351	2418	2425	2441	rVV	3578329	5194959	72.59%	7.510%
38	17.828	2503	2506	2512	rVB7	11816	17030	0.24%	0.025%
39	18.157	2560	2562	2572	rVB10	9736	18564	0.26%	0.027%
40	18.751	2660	2663	2665	rBV3	9211	10290	0.14%	0.015%
41	19.169	2731	2734	2738	rVB2	47184	58389	0.82%	0.084%
42	19.239	2742	2746	2750	rBV	44784	59070	0.83%	0.085%
43	19.598	2801	2807	2813	rBV	5023956	6515142	91.04%	9.418%
44	21.380	3105	3110	3118	rBV	2755936	3461652	48.37%	5.004%
45	23.715	3499	3507	3518	rBV2	3279395	7156306	100.00%	10.345%
46	23.880	3528	3535	3548	rVB	1623931	3711018	51.86%	5.365%




Sum of corrected areas: 69176242

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018396.D
Acq On : 27 Nov 2023 12:41
Operator : MA/JU
Sample : PB157279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

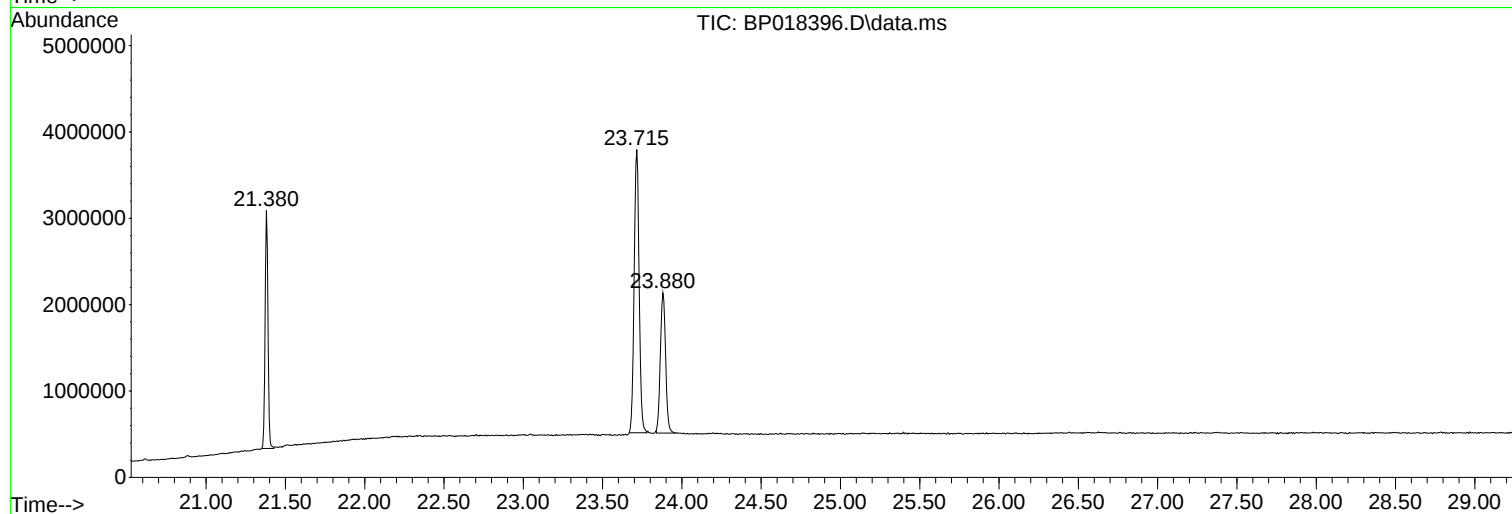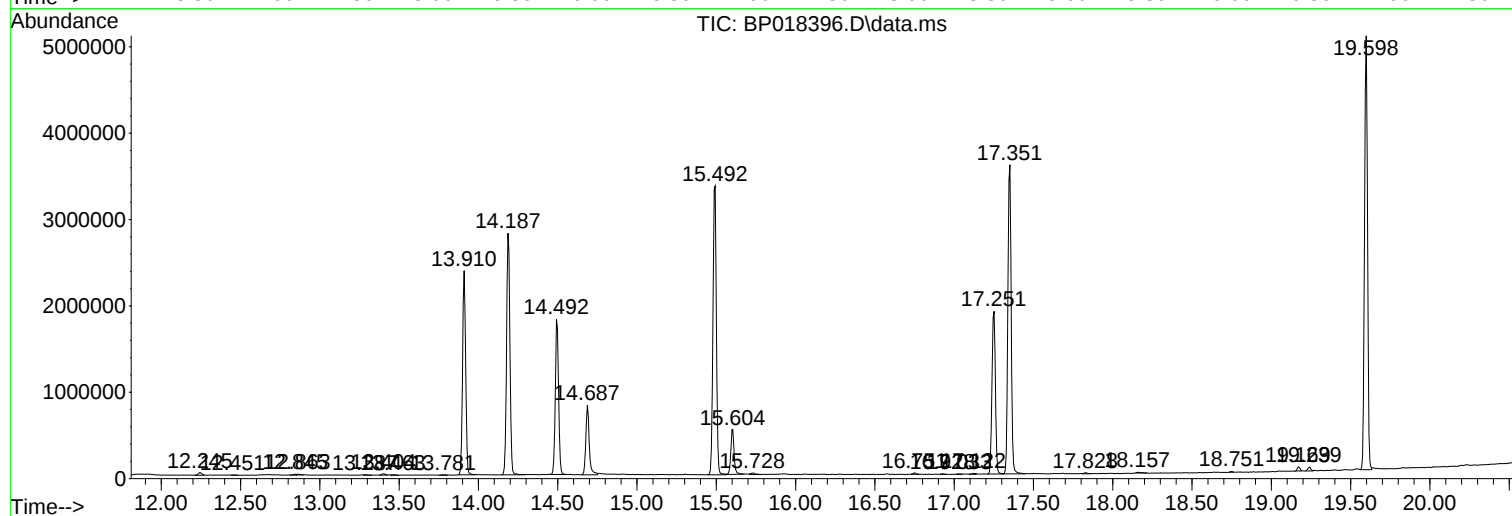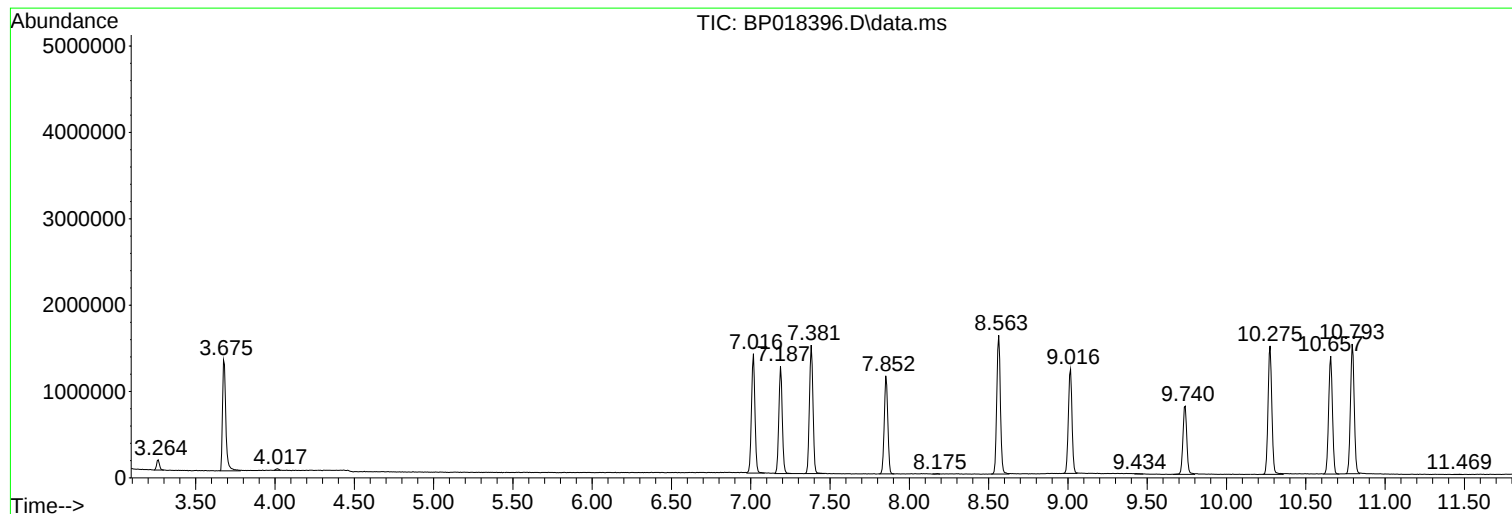

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018396.D
Acq On : 27 Nov 2023 12:41
Operator : MA/JU
Sample : PB157279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018396.D
Acq On : 27 Nov 2023 12:41
Operator : MA/JU
Sample : PB157279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc