

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018397.D
 Acq On : 27 Nov 2023 13:15
 Operator : MA/JU
 Sample : 05328-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rVB	75190	97950	1.59%	0.182%
2	3.687	98	102	115	rBV	335093	486767	7.91%	0.904%
3	3.928	140	143	148	rVB	14616	19924	0.32%	0.037%
4	4.022	156	159	165	rVB2	20917	28276	0.46%	0.052%
5	6.575	589	593	597	rBV5	3382	6667	0.11%	0.012%
6	7.022	663	669	678	rVB	234264	382803	6.22%	0.711%
7	7.193	691	698	707	rBV	953887	1497196	24.34%	2.780%
8	7.387	724	731	743	rBV	876550	1395834	22.69%	2.592%
9	7.487	747	748	755	rVB6	6206	8307	0.14%	0.015%
10	7.863	804	812	819	rBV	1068747	1675982	27.24%	3.112%
11	7.922	819	822	831	rVB7	9410	19878	0.32%	0.037%
12	8.569	925	932	944	rBV	653618	1000086	16.26%	1.857%
13	9.022	1001	1009	1020	rBV	945278	1517265	24.66%	2.817%
14	9.422	1075	1077	1079	rVV3	7321	9464	0.15%	0.018%
15	9.457	1079	1083	1088	rVB2	18347	31115	0.51%	0.058%
16	9.740	1122	1131	1144	rBV	577236	967093	15.72%	1.796%
17	10.275	1215	1222	1233	rBV	1058460	1773645	28.83%	3.293%
18	10.663	1280	1288	1297	rVB	1250552	2132762	34.67%	3.960%
19	10.798	1303	1311	1323	rBV	931950	1573462	25.58%	2.921%
20	11.451	1418	1422	1426	rBV6	3871	6611	0.11%	0.012%
21	11.945	1499	1506	1511	rVB7	5591	12197	0.20%	0.023%
22	12.245	1552	1557	1562	rBV	21274	33050	0.54%	0.061%
23	12.875	1659	1664	1666	rBV5	5138	9118	0.15%	0.017%
24	13.334	1738	1742	1748	rVB3	13975	18936	0.31%	0.035%
25	13.404	1748	1754	1760	rBV	48127	79218	1.29%	0.147%
26	13.910	1831	1840	1849	rBV	1902883	2612780	42.47%	4.851%
27	14.186	1880	1887	1901	rBV	2244474	3199796	52.01%	5.941%
28	14.398	1922	1923	1928	rVB5	5318	6647	0.11%	0.012%
29	14.492	1928	1939	1951	rBV	1619675	2421776	39.37%	4.496%
30	14.575	1951	1953	1958	rVB6	5264	6862	0.11%	0.013%
31	14.686	1966	1972	1985	rBV	93655	176135	2.86%	0.327%
32	14.845	1995	1999	2002	rBV6	6361	9126	0.15%	0.017%
33	14.910	2007	2010	2016	rVB7	8912	11682	0.19%	0.022%
34	15.486	2101	2108	2117	rBV	2868985	4061348	66.02%	7.540%
35	15.598	2121	2127	2135	rBV	415860	581718	9.46%	1.080%
36	15.728	2145	2149	2154	rVB2	13105	20915	0.34%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018397.D
 Acq On : 27 Nov 2023 13:15
 Operator : MA/JU
 Sample : 05328-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.651	2303	2306	2312	rBV8	7698	11085	0.18%	0.021%
38	16.745	2315	2322	2325	rBV9	6258	11573	0.19%	0.021%
39	17.022	2365	2369	2370	rBV4	6449	7738	0.13%	0.014%
40	17.110	2383	2384	2391	rBV6	4818	8999	0.15%	0.017%
41	17.245	2400	2407	2415	rBV	1954426	2623333	42.64%	4.871%
42	17.345	2418	2424	2442	rVB	3089148	4339021	70.53%	8.056%
43	17.933	2520	2524	2527	rBV6	6785	9066	0.15%	0.017%
44	18.145	2556	2560	2564	rBV	98667	133649	2.17%	0.248%
45	18.451	2609	2612	2617	rBV6	9423	14810	0.24%	0.027%
46	18.604	2635	2638	2643	rVB5	13814	17837	0.29%	0.033%
47	19.169	2730	2734	2738	rBV3	42603	52052	0.85%	0.097%
48	19.233	2741	2745	2749	rBV	40588	56970	0.93%	0.106%
49	19.392	2769	2772	2777	rBV4	33017	40963	0.67%	0.076%
50	19.592	2800	2806	2816	rBV	4280661	5649608	91.84%	10.489%
51	21.127	3064	3067	3072	rBV2	72998	98207	1.60%	0.182%
52	21.374	3104	3109	3119	rBV	2562539	3234246	52.57%	6.005%
53	23.704	3497	3505	3517	rBV2	2781927	6151774	100.00%	11.422%
54	23.868	3526	3533	3547	rVB	1522186	3507203	57.01%	6.512%




Sum of corrected areas: 53860525

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018397.D
Acq On : 27 Nov 2023 13:15
Operator : MA/JU
Sample : 05328-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

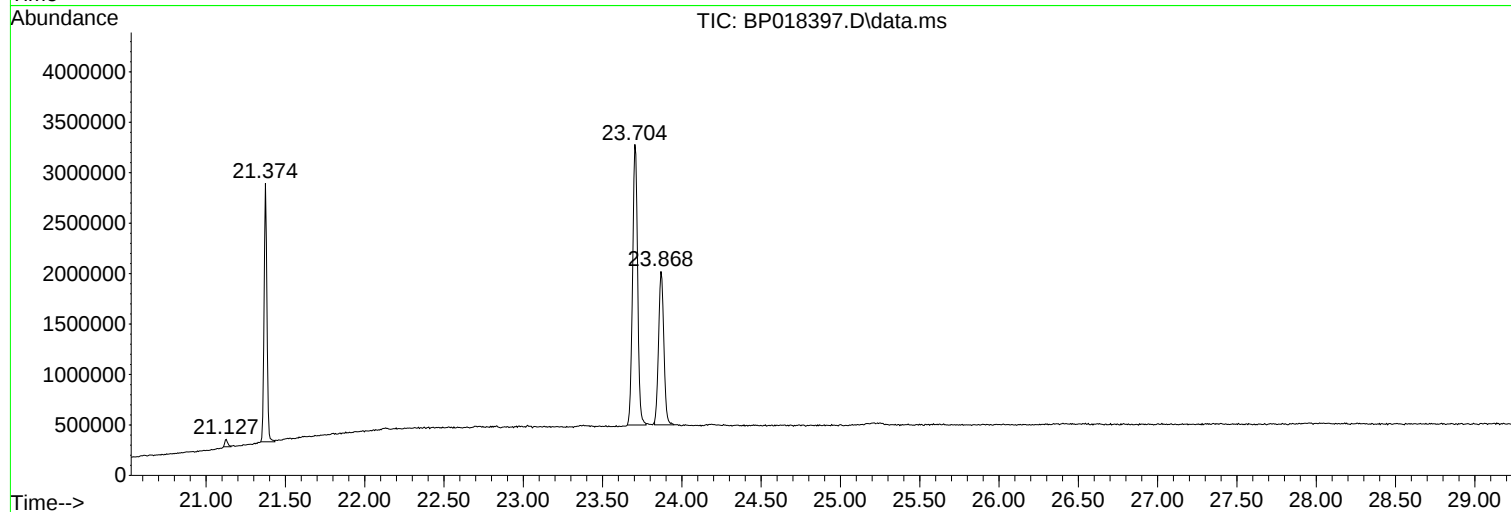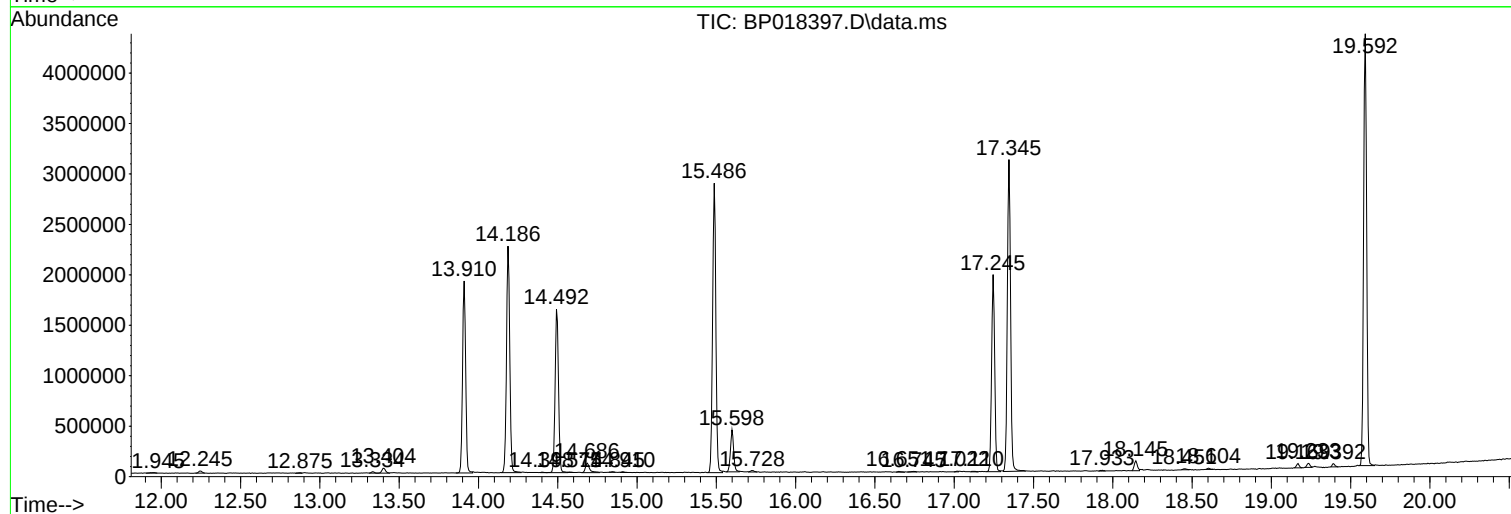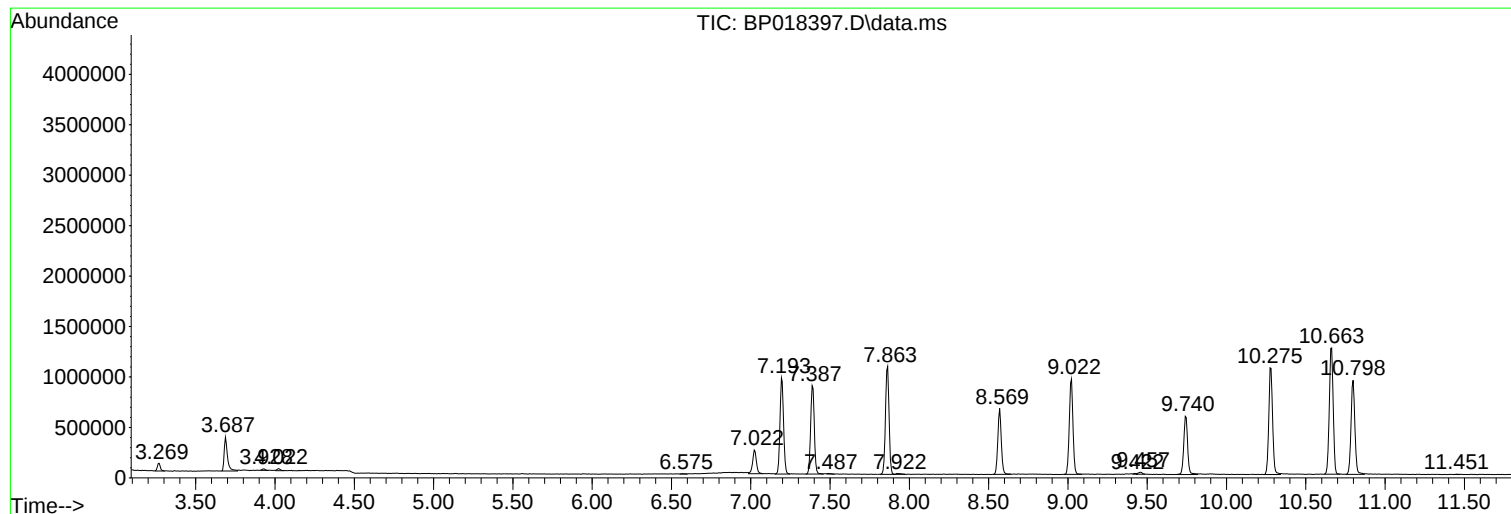

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018397.D
Acq On : 27 Nov 2023 13:15
Operator : MA/JU
Sample : 05328-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018397.D
Acq On : 27 Nov 2023 13:15
Operator : MA/JU
Sample : 05328-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------