

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018398.D
 Acq On : 27 Nov 2023 13:49
 Operator : MA/JU
 Sample : 05328-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	43	rVB	101548	130301	1.69%	0.171%
2	3.552	77	79	83	rBV3	8352	10835	0.14%	0.014%
3	3.687	98	102	116	rBV	536098	783050	10.18%	1.030%
4	4.022	156	159	164	rVB2	23625	33785	0.44%	0.044%
5	4.964	315	319	326	rVB4	9213	15414	0.20%	0.020%
6	5.569	417	422	428	rVB7	6960	12818	0.17%	0.017%
7	5.946	481	486	493	rBV6	7222	13859	0.18%	0.018%
8	7.022	664	669	679	rVB	300922	475263	6.18%	0.625%
9	7.199	690	699	707	rBV	1257876	1976210	25.69%	2.598%
10	7.387	722	731	741	rBV	1130684	1789387	23.26%	2.353%
11	7.469	741	745	754	rVV4	31408	67017	0.87%	0.088%
12	7.863	804	812	820	rBV	1678491	2612045	33.96%	3.434%
13	7.934	820	824	831	rVB2	16176	26298	0.34%	0.035%
14	8.569	925	932	945	rBV	882721	1380477	17.95%	1.815%
15	9.022	1002	1009	1020	rBV	1354523	2117596	27.53%	2.784%
16	9.199	1035	1039	1043	rVB7	5718	9111	0.12%	0.012%
17	9.457	1079	1083	1088	rVB2	31639	52560	0.68%	0.069%
18	9.746	1122	1132	1139	rBV	831043	1388435	18.05%	1.825%
19	10.281	1214	1223	1232	rBV	1498369	2549161	33.14%	3.352%
20	10.663	1280	1288	1298	rVB	2109306	3547041	46.12%	4.664%
21	10.799	1302	1311	1323	rBV	1480913	2437571	31.69%	3.205%
22	11.946	1499	1506	1513	rBV	9234	17685	0.23%	0.023%
23	12.251	1551	1558	1564	rBV2	32571	59489	0.77%	0.078%
24	12.898	1667	1668	1674	rVB6	5471	8199	0.11%	0.011%
25	13.122	1701	1706	1712	rVB7	9426	16033	0.21%	0.021%
26	13.334	1738	1742	1747	rBV4	15918	22968	0.30%	0.030%
27	13.404	1747	1754	1761	rVV	115733	190430	2.48%	0.250%
28	13.469	1761	1765	1773	rVB9	7159	14721	0.19%	0.019%
29	13.728	1806	1809	1815	rVB7	7639	11000	0.14%	0.014%
30	13.910	1833	1840	1849	rBV	2911823	4022027	52.29%	5.288%
31	14.187	1877	1887	1897	rBV	3375872	4860992	63.20%	6.391%
32	14.404	1920	1924	1927	rBV5	7168	11216	0.15%	0.015%
33	14.493	1933	1939	1953	rBV	2890956	4295065	55.84%	5.647%
34	14.687	1966	1972	1978	rBV	110242	179514	2.33%	0.236%
35	14.845	1997	1999	2004	rVB6	8385	13114	0.17%	0.017%
36	14.910	2004	2010	2017	rBV6	9724	19029	0.25%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018398.D
 Acq On : 27 Nov 2023 13:49
 Operator : MA/JU
 Sample : 05328-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.310	2073	2078	2082	rBV8	6786	14398	0.19%	0.019%
38	15.487	2101	2108	2121	rBV	4036165	5843324	75.97%	7.683%
39	15.598	2121	2127	2136	rBV	592613	814520	10.59%	1.071%
40	15.728	2146	2149	2157	rVB3	22478	34554	0.45%	0.045%
41	16.269	2240	2241	2248	rVB7	6328	8903	0.12%	0.012%
42	16.651	2302	2306	2312	rBV8	7711	12158	0.16%	0.016%
43	16.745	2318	2322	2325	rBV6	6228	8009	0.10%	0.011%
44	16.922	2350	2352	2356	rVB5	8597	10415	0.14%	0.014%
45	17.028	2364	2370	2374	rBV6	11570	21675	0.28%	0.028%
46	17.063	2374	2376	2380	rVB5	8298	9252	0.12%	0.012%
47	17.245	2400	2407	2417	rBV	2898762	3944079	51.28%	5.186%
48	17.345	2418	2424	2435	rVV	4026227	5524906	71.83%	7.264%
49	17.628	2467	2472	2475	rBV6	7856	13727	0.18%	0.018%
50	17.934	2520	2524	2529	rVB5	13748	17086	0.22%	0.022%
51	18.145	2555	2560	2569	rBV	249367	350648	4.56%	0.461%
52	18.445	2607	2611	2612	rBV4	10774	14655	0.19%	0.019%
53	18.604	2636	2638	2642	rVB5	11062	11589	0.15%	0.015%
54	19.169	2730	2734	2738	rBV2	48140	59442	0.77%	0.078%
55	19.233	2742	2745	2749	rVV	43783	57843	0.75%	0.076%
56	19.392	2768	2772	2776	rBV3	81039	101764	1.32%	0.134%
57	19.592	2800	2806	2815	rBV	5005415	6457991	83.96%	8.491%
58	21.127	3063	3067	3075	rBV2	180684	304624	3.96%	0.401%
59	21.375	3104	3109	3119	rBV	3457637	4430212	57.60%	5.825%
60	23.710	3498	3506	3520	rVB	3506940	7691498	100.00%	10.113%
61	23.874	3526	3534	3548	rVB	2184668	5131856	66.72%	6.747%




Sum of corrected areas: 76058844

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018398.D
Acq On : 27 Nov 2023 13:49
Operator : MA/JU
Sample : 05328-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

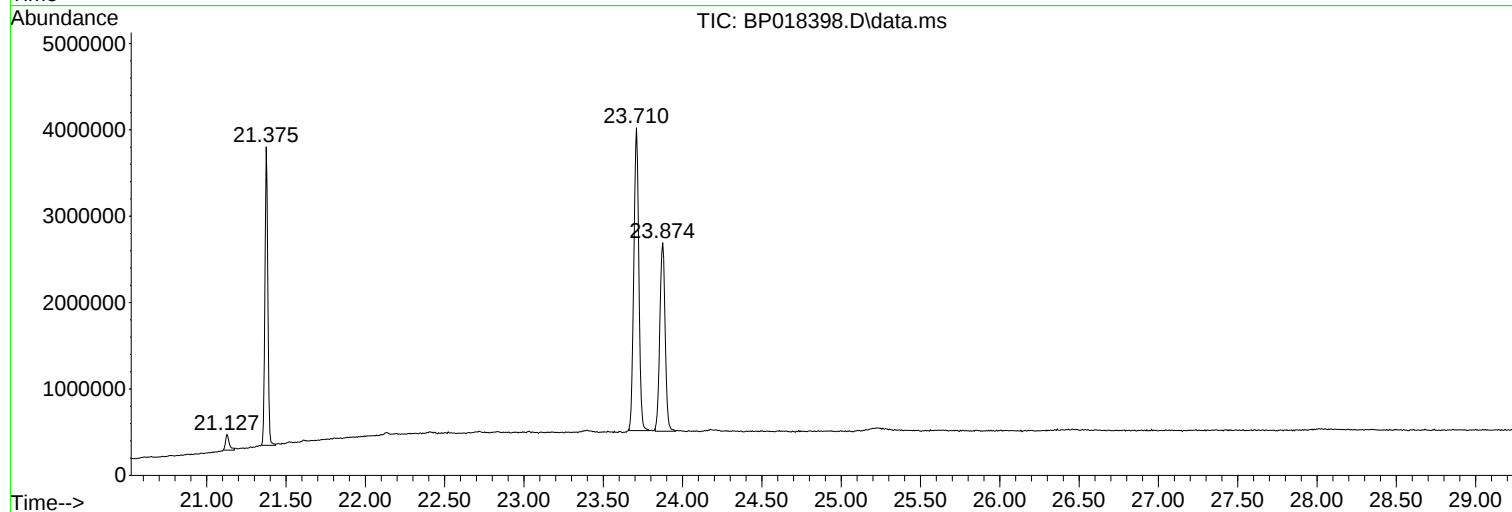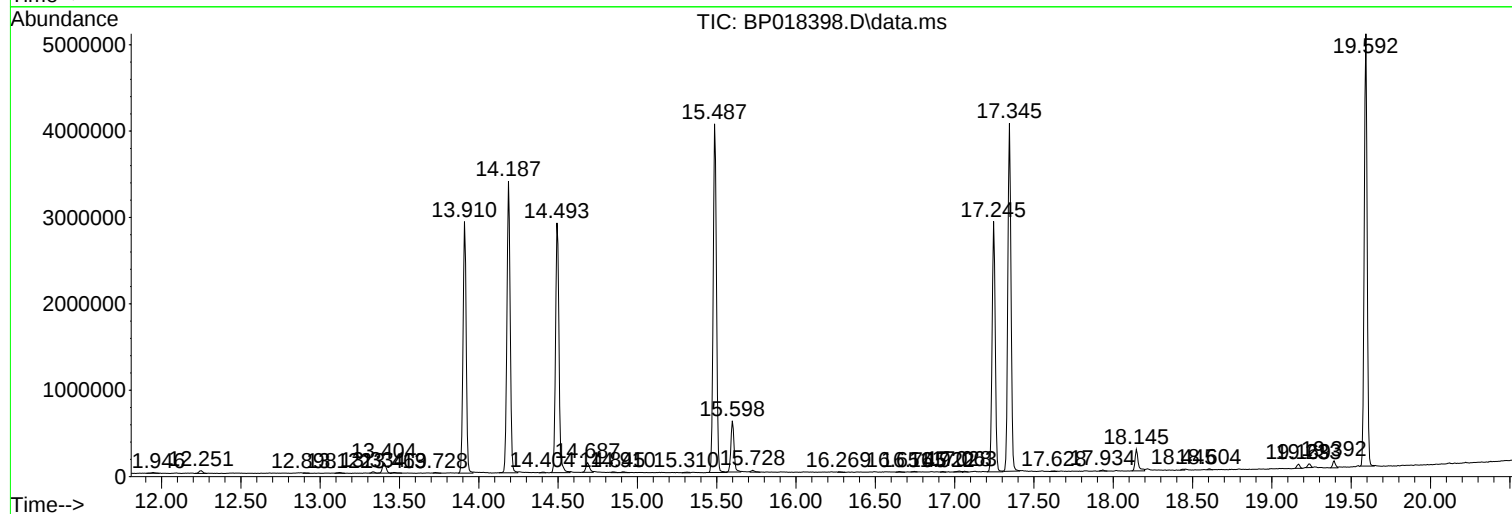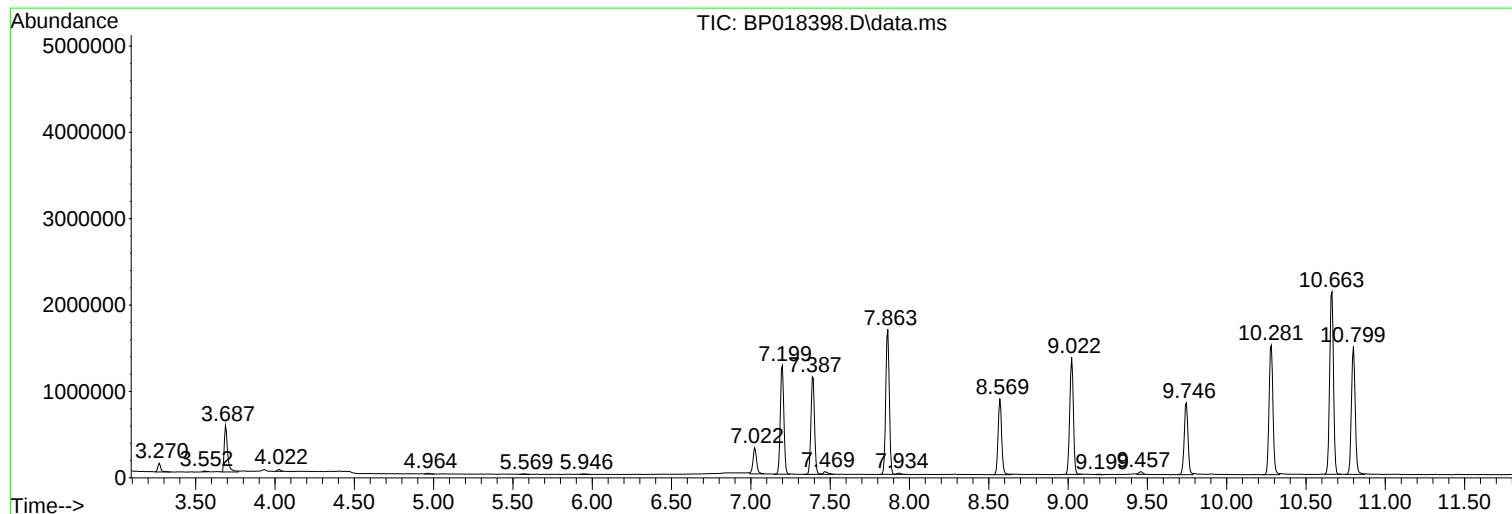

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018398.D
Acq On : 27 Nov 2023 13:49
Operator : MA/JU
Sample : 05328-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018398.D
Acq On : 27 Nov 2023 13:49
Operator : MA/JU
Sample : 05328-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc