

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018402.D
 Acq On : 27 Nov 2023 16:05
 Operator : MA/JU
 Sample : 05328-18
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49Z8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rVB	97577	121218	1.59%	0.143%
2	3.687	98	102	113	rBV	588783	842182	11.02%	0.994%
3	3.928	140	143	148	rVB2	19922	32677	0.43%	0.039%
4	4.022	155	159	164	rBV	24492	34329	0.45%	0.041%
5	4.969	316	320	324	rVB6	6973	10682	0.14%	0.013%
6	5.946	482	486	490	rVB6	6268	9920	0.13%	0.012%
7	6.840	634	638	643	rBV7	7790	13715	0.18%	0.016%
8	7.022	663	669	683	rVB	332180	543598	7.12%	0.642%
9	7.199	691	699	711	rVB	1408439	2198330	28.78%	2.596%
10	7.387	723	731	741	rBV	1247306	2010715	26.32%	2.374%
11	7.481	741	747	753	rVB5	11900	30584	0.40%	0.036%
12	7.863	801	812	820	rBV	1690627	2671105	34.96%	3.154%
13	7.934	820	824	829	rVB3	17556	28709	0.38%	0.034%
14	8.569	924	932	944	rBV	1012737	1547626	20.26%	1.827%
15	9.022	1002	1009	1017	rBV	1545297	2456062	32.15%	2.900%
16	9.199	1032	1039	1044	rVB	3842	10608	0.14%	0.013%
17	9.457	1076	1083	1090	rVB	55020	90784	1.19%	0.107%
18	9.746	1122	1132	1143	rBV	1018139	1706827	22.34%	2.015%
19	9.898	1152	1158	1163	rBV7	7157	14304	0.19%	0.017%
20	10.281	1215	1223	1233	rBV	1819701	2994315	39.20%	3.536%
21	10.663	1280	1288	1297	rVB	2233985	3800582	49.75%	4.488%
22	10.798	1302	1311	1324	rBV	1758284	2947282	38.58%	3.480%
23	11.951	1502	1507	1513	rVB4	17232	30191	0.40%	0.036%
24	12.245	1550	1557	1564	rBV	40829	70048	0.92%	0.083%
25	12.457	1590	1593	1598	rVB7	5390	8712	0.11%	0.010%
26	12.898	1667	1668	1673	rVB5	5769	8302	0.11%	0.010%
27	13.122	1700	1706	1712	rVB6	8803	17326	0.23%	0.020%
28	13.334	1737	1742	1747	rBV2	24614	34740	0.45%	0.041%
29	13.404	1748	1754	1760	rVV	45459	75229	0.98%	0.089%
30	13.463	1760	1764	1774	rVB7	9714	19989	0.26%	0.024%
31	13.722	1806	1808	1815	rVB6	5413	9908	0.13%	0.012%
32	13.910	1833	1840	1853	rBV	3522954	4802323	62.86%	5.671%
33	14.186	1880	1887	1899	rBV	3913861	5821597	76.20%	6.874%
34	14.404	1920	1924	1928	rBV5	9233	12961	0.17%	0.015%
35	14.492	1932	1939	1950	rBV	3294486	4817865	63.07%	5.689%
36	14.686	1966	1972	1984	rBV	126961	228492	2.99%	0.270%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018402.D
 Acq On : 27 Nov 2023 16:05
 Operator : MA/JU
 Sample : 05328-18
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49Z8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.851	1995	2000	2003	rVV6	10017	16927	0.22%	0.020%
38	14.910	2007	2010	2014	rVB6	13151	19125	0.25%	0.023%
39	15.310	2074	2078	2082	rBV5	7227	10924	0.14%	0.013%
40	15.357	2082	2086	2091	rVB8	6748	9256	0.12%	0.011%
41	15.486	2101	2108	2121	rBV	4919341	7064404	92.47%	8.342%
42	15.598	2121	2127	2143	rVV	776443	1076442	14.09%	1.271%
43	15.722	2145	2148	2155	rVB2	21122	35880	0.47%	0.042%
44	15.928	2181	2183	2188	rVB6	7627	8798	0.12%	0.010%
45	16.269	2240	2241	2246	rVB4	9636	12173	0.16%	0.014%
46	16.651	2303	2306	2310	rVB5	8839	11652	0.15%	0.014%
47	16.745	2319	2322	2327	rVB6	5810	7742	0.10%	0.009%
48	16.851	2338	2340	2346	rVB7	6930	8521	0.11%	0.010%
49	17.016	2365	2368	2371	rBV5	10123	15418	0.20%	0.018%
50	17.057	2373	2375	2379	rVB5	8694	10624	0.14%	0.013%
51	17.122	2382	2386	2389	rBV4	11498	13904	0.18%	0.016%
52	17.245	2399	2407	2417	rBV	3336220	4683437	61.31%	5.530%
53	17.345	2417	2424	2435	rVV2	4677259	6625143	86.72%	7.823%
54	17.622	2468	2471	2475	rBV6	7464	14780	0.19%	0.017%
55	17.933	2520	2524	2527	rBV5	13377	16904	0.22%	0.020%
56	18.016	2536	2538	2543	rBV6	7696	9862	0.13%	0.012%
57	18.145	2555	2560	2570	rBV	247088	371493	4.86%	0.439%
58	18.445	2608	2611	2618	rVB7	15080	27977	0.37%	0.033%
59	18.604	2635	2638	2645	rBV7	14660	19910	0.26%	0.024%
60	19.163	2730	2733	2738	rVB2	58061	80855	1.06%	0.095%
61	19.233	2741	2745	2749	rBV	55322	79297	1.04%	0.094%
62	19.392	2768	2772	2779	rBV2	80001	105792	1.38%	0.125%
63	19.592	2800	2806	2814	rBV	5338617	7101110	92.95%	8.385%
64	21.127	3063	3067	3073	rBV2	192952	327062	4.28%	0.386%
65	21.374	3104	3109	3118	rBV	3284832	4309137	56.41%	5.088%
66	23.715	3498	3507	3521	rVB	3350160	7639438	100.00%	9.021%
67	23.880	3527	3535	3547	rVB	2080259	4878206	63.86%	5.760%




Sum of corrected areas: 84686030

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018402.D
Acq On : 27 Nov 2023 16:05
Operator : MA/JU
Sample : 05328-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

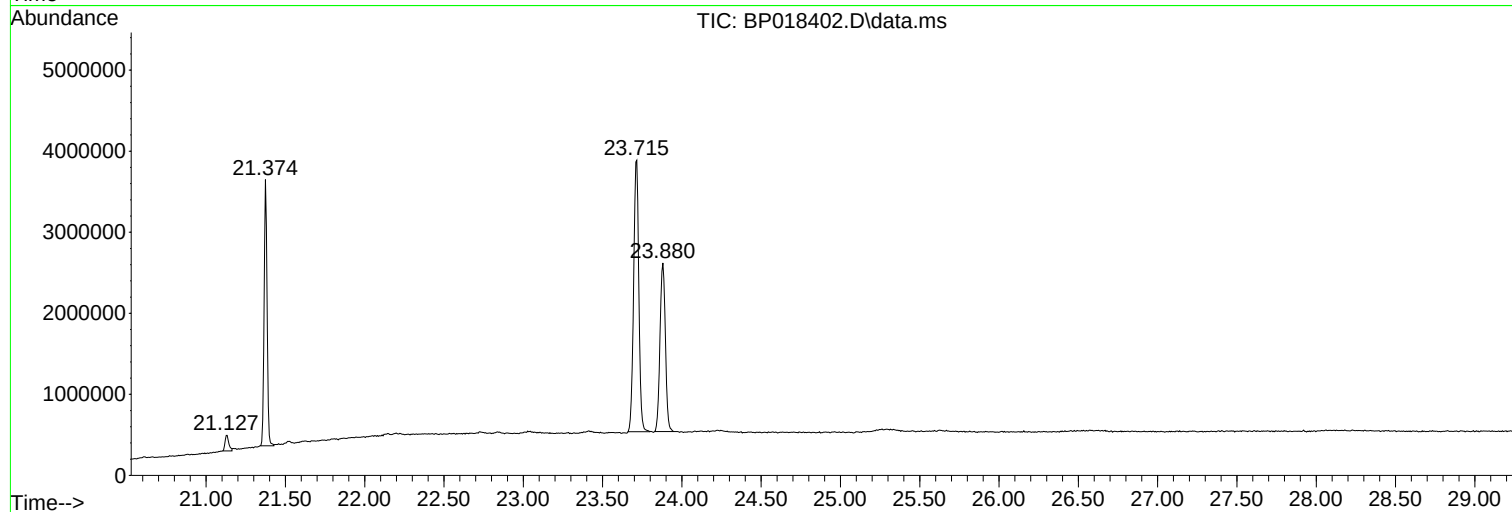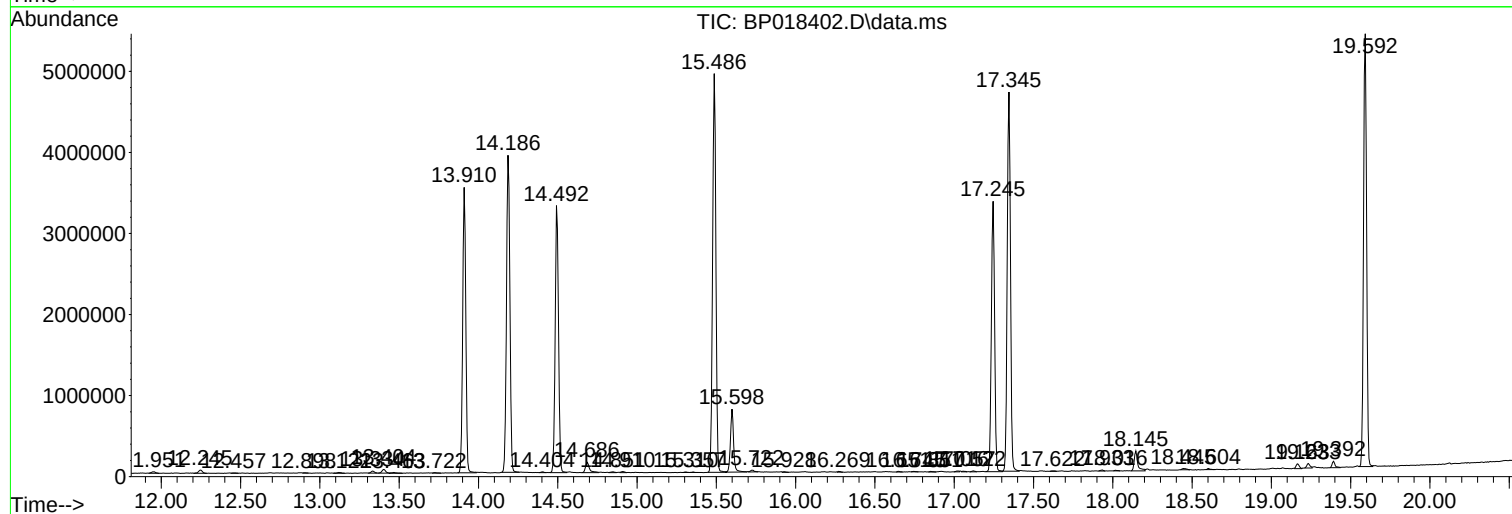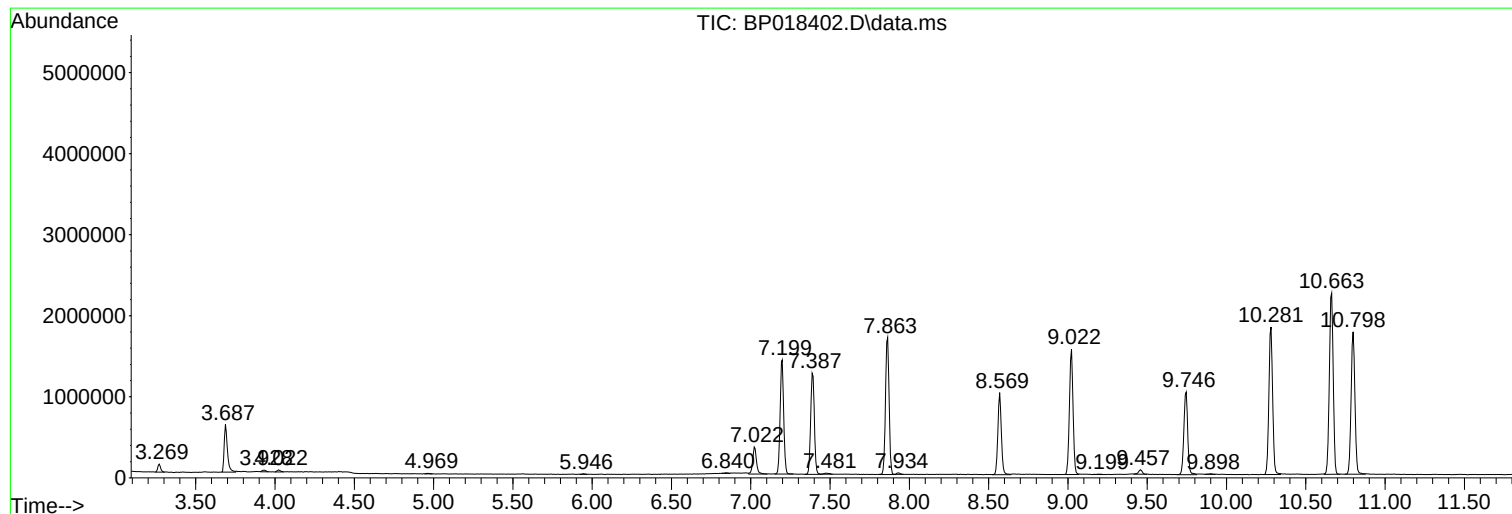

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018402.D
Acq On : 27 Nov 2023 16:05
Operator : MA/JU
Sample : 05328-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018402.D
Acq On : 27 Nov 2023 16:05
Operator : MA/JU
Sample : 05328-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc