

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018405.D
 Acq On : 27 Nov 2023 17:47
 Operator : MA/JU
 Sample : 05341-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	38	rVB	88804	111573	1.41%	0.145%
2	3.687	98	102	119	rBV	462411	669820	8.46%	0.869%
3	3.928	141	143	149	rVB2	20016	25043	0.32%	0.032%
4	4.022	156	159	164	rVB2	24542	34125	0.43%	0.044%
5	4.963	316	319	326	rVB2	12638	18114	0.23%	0.024%
6	5.134	345	348	351	rBV	9515	10828	0.14%	0.014%
7	6.840	632	638	639	rBV5	5565	11117	0.14%	0.014%
8	7.022	663	669	679	rVB	319187	505366	6.38%	0.656%
9	7.193	691	698	708	rVB	1413847	2207092	27.88%	2.864%
10	7.387	724	731	743	rBV	1242830	1985426	25.08%	2.576%
11	7.863	802	812	819	rBV	1526989	2434890	30.76%	3.160%
12	8.569	924	932	944	rBV	953605	1486314	18.78%	1.929%
13	9.022	1002	1009	1023	rBV	1471706	2401024	30.33%	3.116%
14	9.457	1079	1083	1090	rVB4	16080	31119	0.39%	0.040%
15	9.745	1122	1132	1145	rBV	953276	1585829	20.03%	2.058%
16	10.281	1216	1223	1234	rBV	1655493	2737084	34.58%	3.552%
17	10.657	1279	1287	1298	rVB	1951697	3301035	41.70%	4.284%
18	10.798	1303	1311	1321	rBV	1545329	2541920	32.11%	3.299%
19	11.481	1420	1427	1429	rVV6	9211	15840	0.20%	0.021%
20	12.186	1541	1547	1553	rBV	149057	232945	2.94%	0.302%
21	12.245	1553	1557	1563	rVB2	36774	59626	0.75%	0.077%
22	12.863	1660	1662	1669	rVB8	5803	11392	0.14%	0.015%
23	13.281	1726	1733	1736	rBV8	3519	8683	0.11%	0.011%
24	13.398	1748	1753	1758	rVB8	13256	21938	0.28%	0.028%
25	13.463	1760	1764	1770	rBV6	7633	11412	0.14%	0.015%
26	13.910	1832	1840	1854	rBV	3044791	4114823	51.98%	5.340%
27	14.186	1880	1887	1901	rBV	3559371	5177239	65.40%	6.719%
28	14.492	1929	1939	1951	rBV	2625796	3898960	49.25%	5.060%
29	14.686	1966	1972	1983	rBV	104942	189673	2.40%	0.246%
30	14.910	2005	2010	2014	rBV8	10368	17212	0.22%	0.022%
31	15.486	2101	2108	2121	rBV	4306120	6238874	78.81%	8.096%
32	15.598	2121	2127	2139	rVV	609147	842824	10.65%	1.094%
33	15.727	2145	2149	2155	rVB4	23146	35927	0.45%	0.047%
34	16.751	2318	2323	2327	rVB7	7354	12710	0.16%	0.016%
35	17.027	2367	2370	2373	rBV4	6073	8089	0.10%	0.010%
36	17.245	2401	2407	2417	rBV	2672195	3733268	47.16%	4.845%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018405.D
Acq On : 27 Nov 2023 17:47
Operator : MA/JU
Sample : 05341-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	17.345	2417	2424	2436	rBV2	4133835	6041508	76.32%	7.840%
38	18.145	2555	2560	2569	rBV2	92707	146636	1.85%	0.190%
39	19.163	2729	2733	2738	rVB2	56483	75466	0.95%	0.098%
40	19.233	2741	2745	2749	rBV	51872	73232	0.93%	0.095%
41	19.392	2767	2772	2777	rBV2	91898	130839	1.65%	0.170%
42	19.592	2800	2806	2813	rBV	5416866	6968432	88.03%	9.043%
43	21.374	3104	3109	3119	rBV	3269454	4253776	53.73%	5.520%
44	23.715	3499	3507	3523	rVB2	3436464	7916349	100.00%	10.273%
45	23.886	3528	3536	3552	rVB	1948859	4723724	59.67%	6.130%




Sum of corrected areas: 77059116

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018405.D
Acq On : 27 Nov 2023 17:47
Operator : MA/JU
Sample : 05341-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

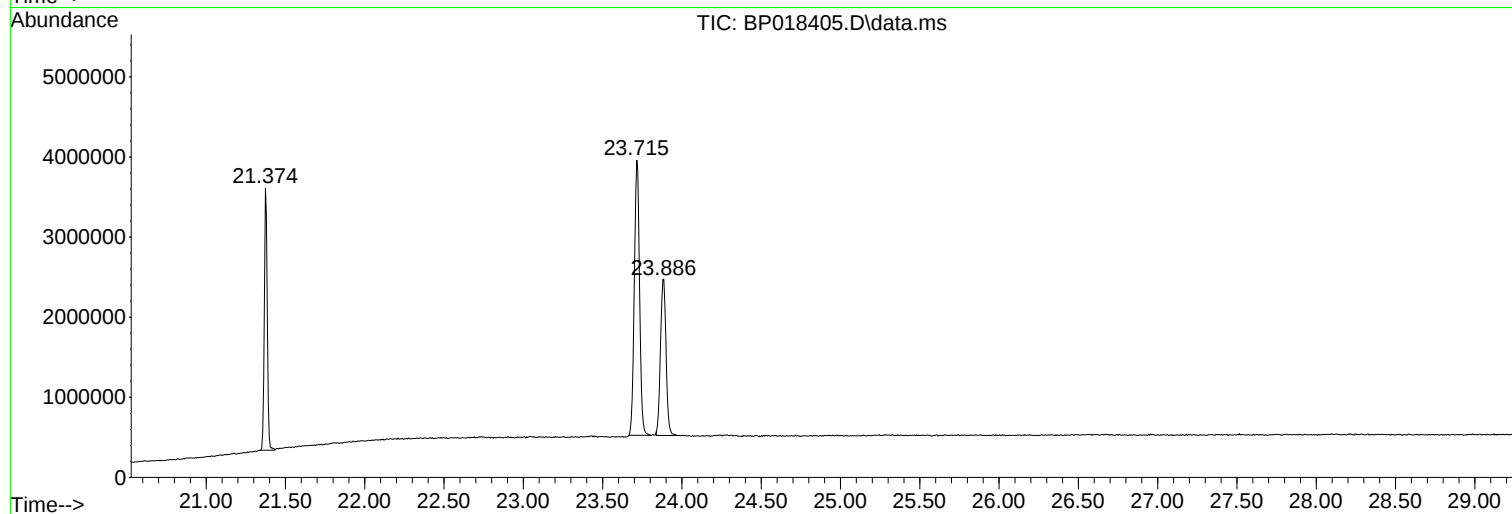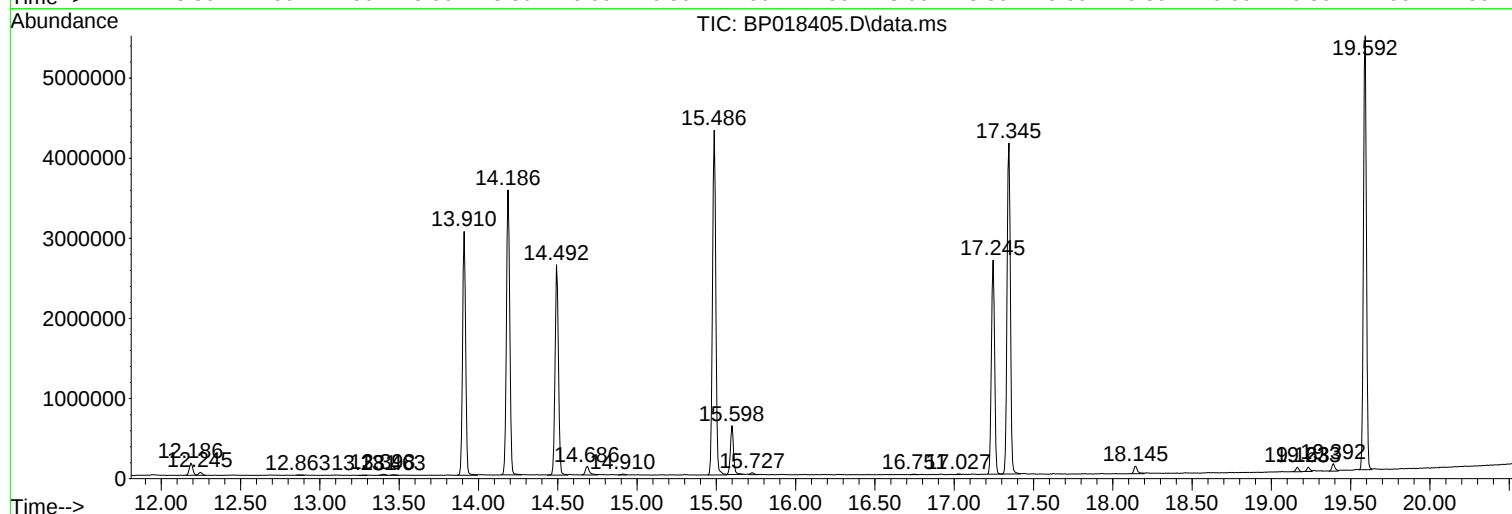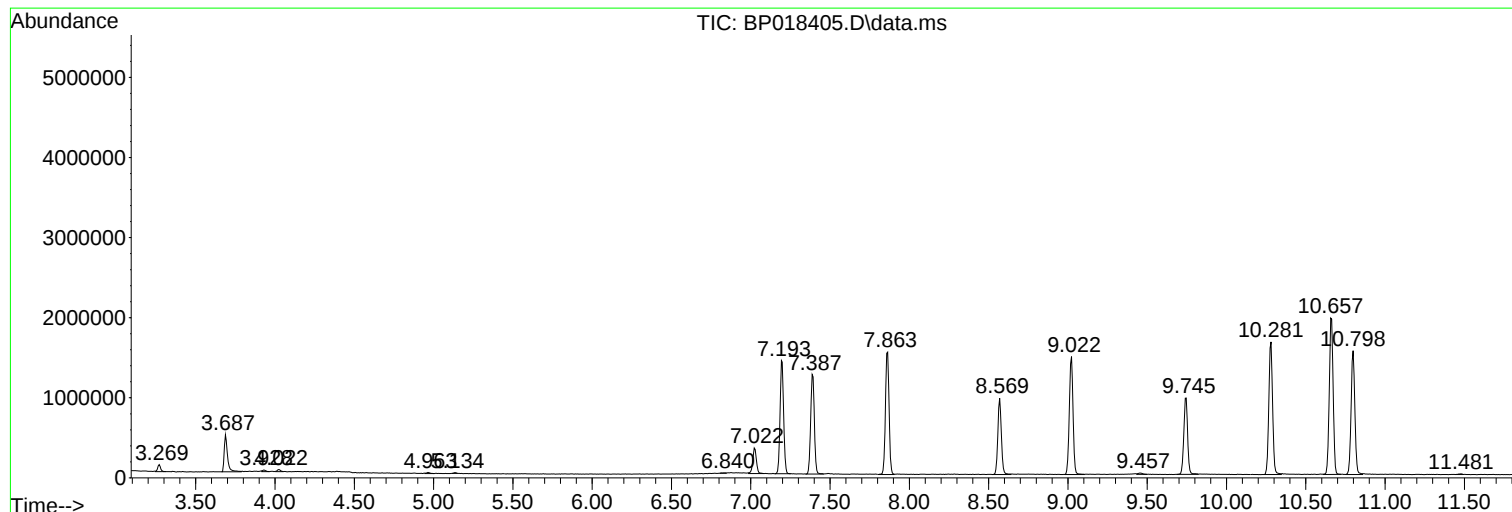

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018405.D
Acq On : 27 Nov 2023 17:47
Operator : MA/JU
Sample : 05341-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018405.D
Acq On : 27 Nov 2023 17:47
Operator : MA/JU
Sample : 05341-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc