

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018406.D
 Acq On : 27 Nov 2023 18:21
 Operator : MA/JU
 Sample : 05341-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	40	rVB	98035	125570	1.31%	0.133%
2	3.687	98	102	110	rBV	382278	546760	5.71%	0.579%
3	3.928	138	143	148	rVB3	21848	39450	0.41%	0.042%
4	4.023	156	159	165	rVB	29389	39366	0.41%	0.042%
5	7.022	663	669	677	rVB	420772	647415	6.76%	0.686%
6	7.193	692	698	707	rVB	1618398	2538482	26.50%	2.690%
7	7.387	724	731	738	rBV	1503532	2367557	24.71%	2.509%
8	7.487	745	748	754	rVB7	9459	18403	0.19%	0.020%
9	7.858	804	811	819	rBV	1701881	2695451	28.13%	2.856%
10	8.569	924	932	945	rBV	1204003	1891115	19.74%	2.004%
11	9.022	1001	1009	1022	rBV	1824047	2888082	30.14%	3.060%
12	9.411	1069	1075	1077	rBV7	5350	11958	0.12%	0.013%
13	9.458	1079	1083	1090	rVB6	17931	29228	0.31%	0.031%
14	9.740	1122	1131	1147	rBV	1191716	2002900	20.91%	2.122%
15	10.275	1214	1222	1239	rBV	2069371	3503757	36.57%	3.713%
16	10.658	1278	1287	1296	rBV	2285345	3852053	40.21%	4.082%
17	10.799	1303	1311	1329	rBV	1659543	2810461	29.33%	2.978%
18	11.475	1421	1426	1429	rVB7	8113	13976	0.15%	0.015%
19	11.557	1435	1440	1445	rVB9	5082	11014	0.11%	0.012%
20	11.946	1502	1506	1510	rBV4	6584	11116	0.12%	0.012%
21	12.246	1553	1557	1562	rVB	46395	70387	0.73%	0.075%
22	13.404	1747	1754	1759	rBV7	16512	26443	0.28%	0.028%
23	13.910	1832	1840	1853	rBV	4117303	5594392	58.39%	5.928%
24	14.187	1880	1887	1901	rBV	4606075	6845360	71.45%	7.254%
25	14.493	1932	1939	1950	rBV	3266232	4797304	50.07%	5.084%
26	14.581	1950	1954	1959	rVB8	5671	10810	0.11%	0.011%
27	14.687	1964	1972	1983	rBV	161809	297044	3.10%	0.315%
28	14.851	1995	2000	2006	rBV9	5825	12763	0.13%	0.014%
29	14.910	2006	2010	2016	rVB9	17000	25143	0.26%	0.027%
30	15.487	2101	2108	2120	rBV	5931517	8471922	88.43%	8.978%
31	15.598	2121	2127	2141	rVV	932471	1283099	13.39%	1.360%
32	15.722	2144	2148	2156	rVB	28054	44599	0.47%	0.047%
33	16.057	2201	2205	2211	rVB9	6501	11492	0.12%	0.012%
34	16.269	2236	2241	2245	rVB7	8839	12387	0.13%	0.013%
35	16.745	2318	2322	2327	rBV6	7247	10893	0.11%	0.012%
36	16.928	2348	2353	2357	rVB8	6910	12648	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018406.D
 Acq On : 27 Nov 2023 18:21
 Operator : MA/JU
 Sample : 05341-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.028	2365	2370	2373	rBV5	9466	17160	0.18%	0.018%
38	17.128	2382	2387	2390	rBV7	6345	11917	0.12%	0.013%
39	17.245	2398	2407	2417	rBV	3235813	4583066	47.84%	4.857%
40	17.345	2417	2424	2436	rBV	6066147	8395665	87.63%	8.897%
41	18.139	2555	2559	2565	rBV	111656	155808	1.63%	0.165%
42	19.163	2729	2733	2739	rBV4	69402	94677	0.99%	0.100%
43	19.234	2741	2745	2749	rBV	66502	90572	0.95%	0.096%
44	19.392	2768	2772	2779	rBV	105938	137487	1.44%	0.146%
45	19.592	2800	2806	2814	rBV	6634252	8620391	89.98%	9.135%
46	21.375	3104	3109	3118	rBV	3221485	4269956	44.57%	4.525%
47	23.722	3499	3508	3521	rBV2	4170075	9580691	100.00%	10.153%
48	23.886	3528	3536	3548	rVB	2022901	4838633	50.50%	5.127%




Sum of corrected areas: 94366823

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018406.D
Acq On : 27 Nov 2023 18:21
Operator : MA/JU
Sample : 05341-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

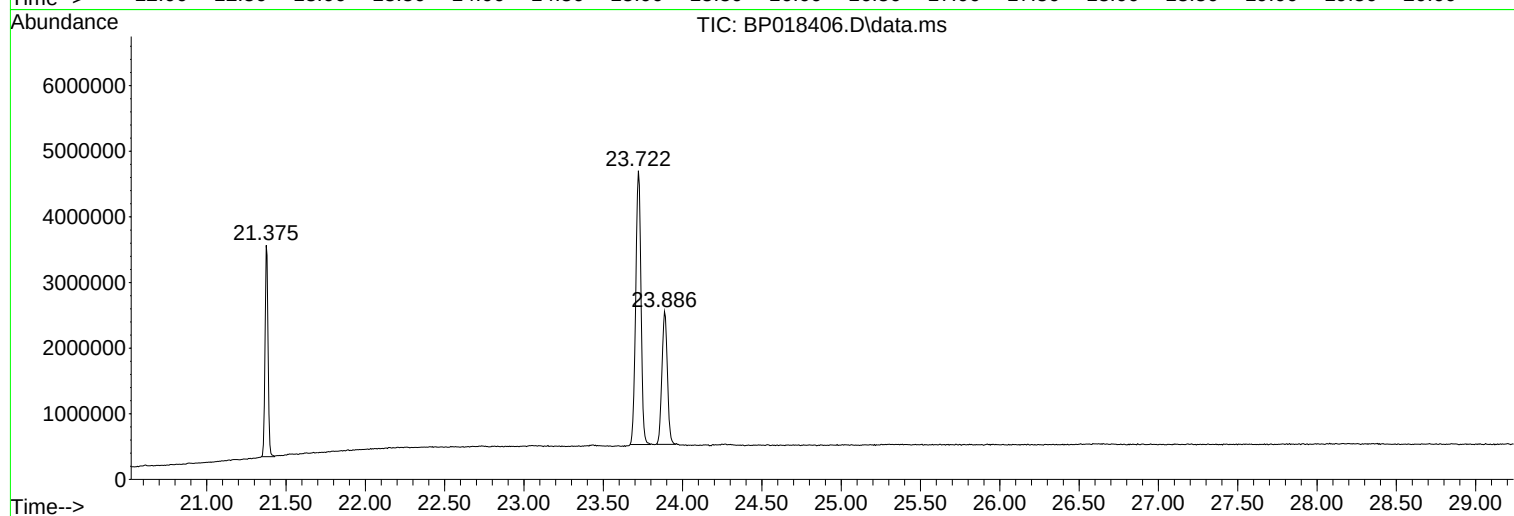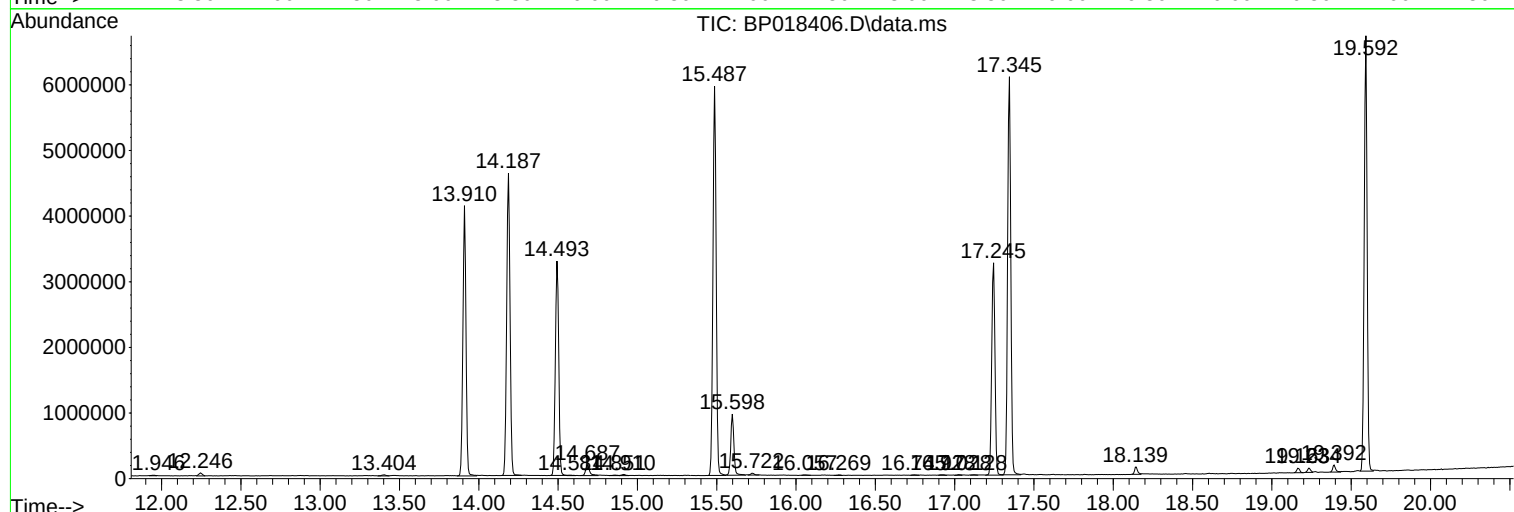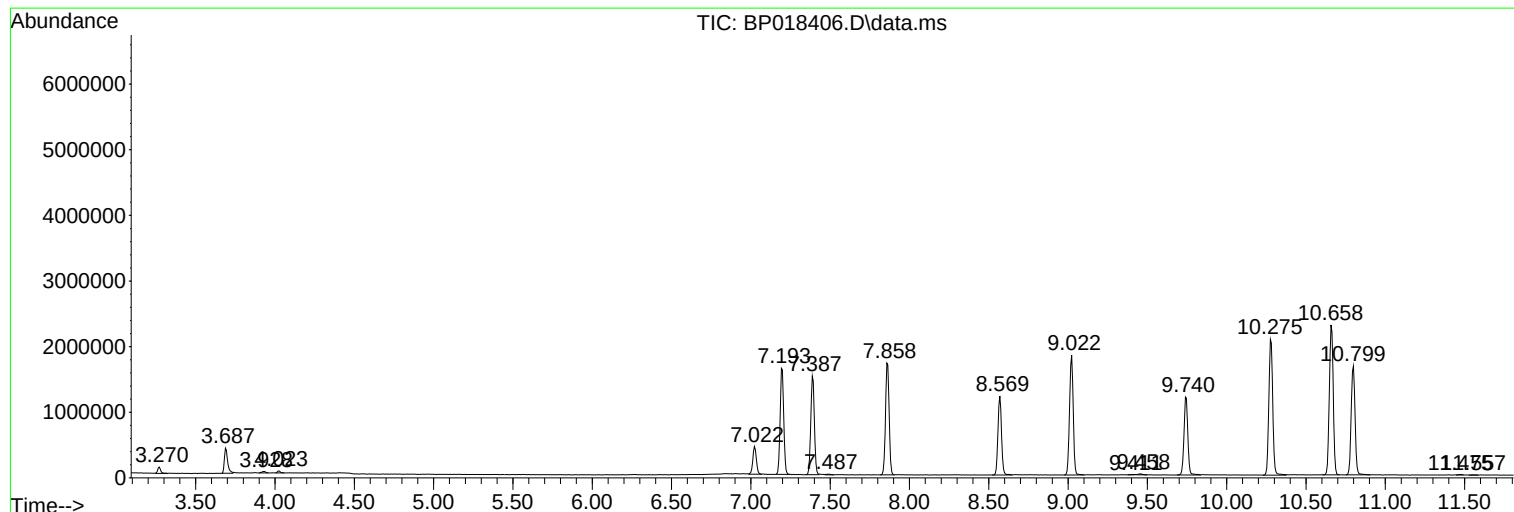

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018406.D
Acq On : 27 Nov 2023 18:21
Operator : MA/JU
Sample : 05341-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018406.D
Acq On : 27 Nov 2023 18:21
Operator : MA/JU
Sample : 05341-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc